
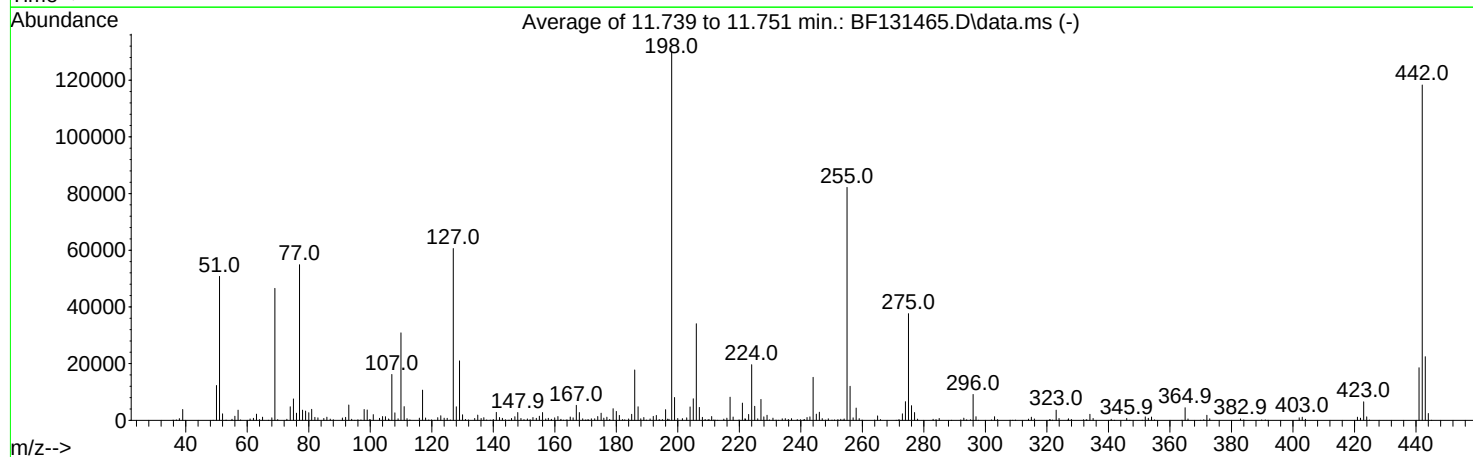


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113022\
 Data File : BF131465.D
 Acq On : 30 Nov 2022 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 12:46:17 2022

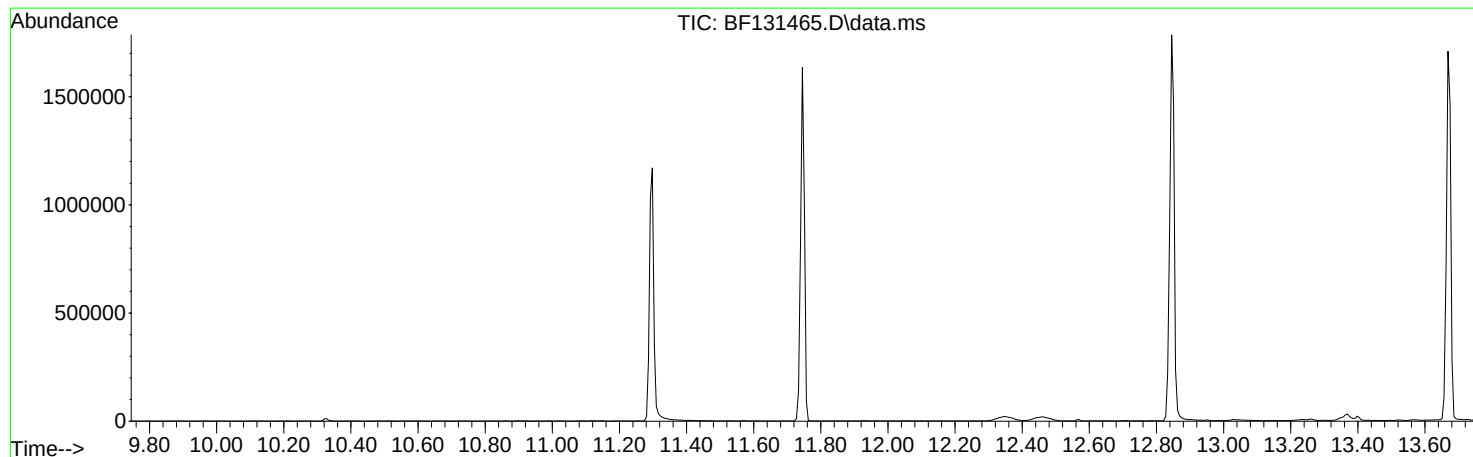




AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	50773	PASS
68	69	0.00	2	1.9	907	PASS
69	198	0.00	100	35.9	46536	PASS
70	69	0.00	2	0.5	250	PASS
127	198	10	80	46.7	60635	PASS
197	198	0.00	2	0.3	453	PASS
198	198	100	100	100.0	129803	PASS
199	198	5	9	6.2	8053	PASS
275	198	10	60	29.0	37632	PASS
365	198	1	100	3.4	4408	PASS
441	198	0.01	100	14.3	18532	PASS
442	442	50	100	100.0	118333	PASS
443	442	15	24	19.0	22450	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113022\  
Data File : BF131465.D  
Acq On    : 30 Nov 2022  09:31  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 01 04:31:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 01:09:58 2022
Response via : Initial Calibration

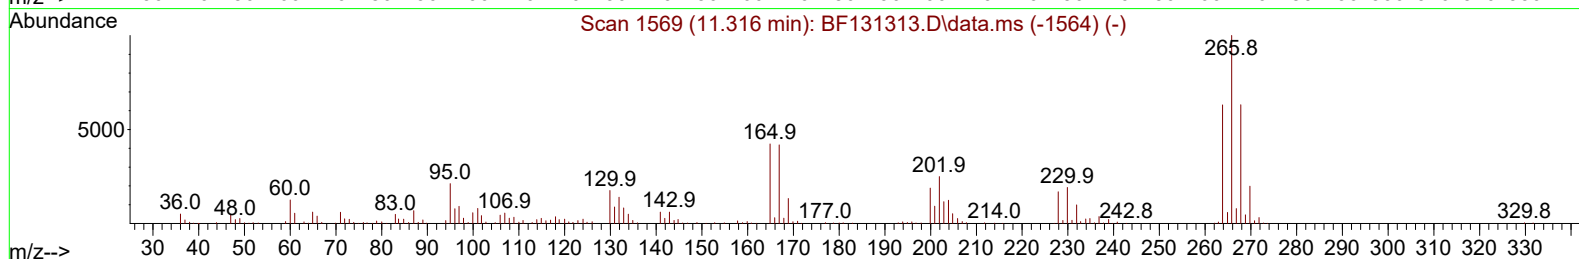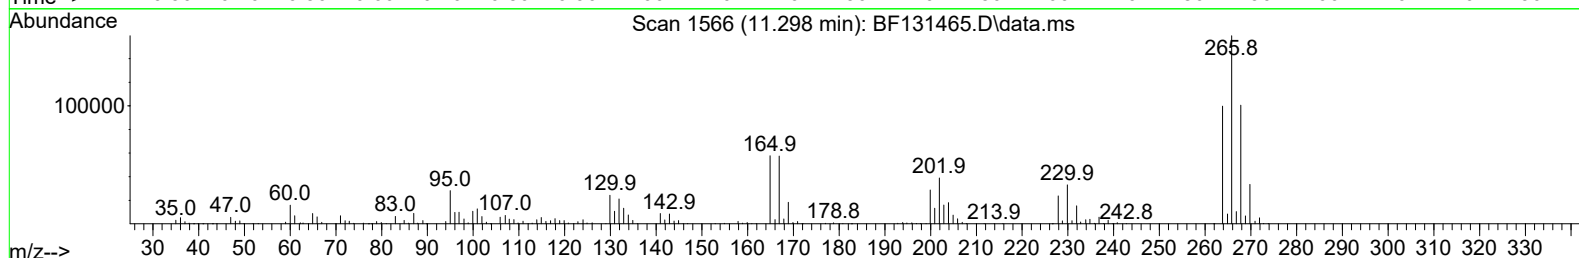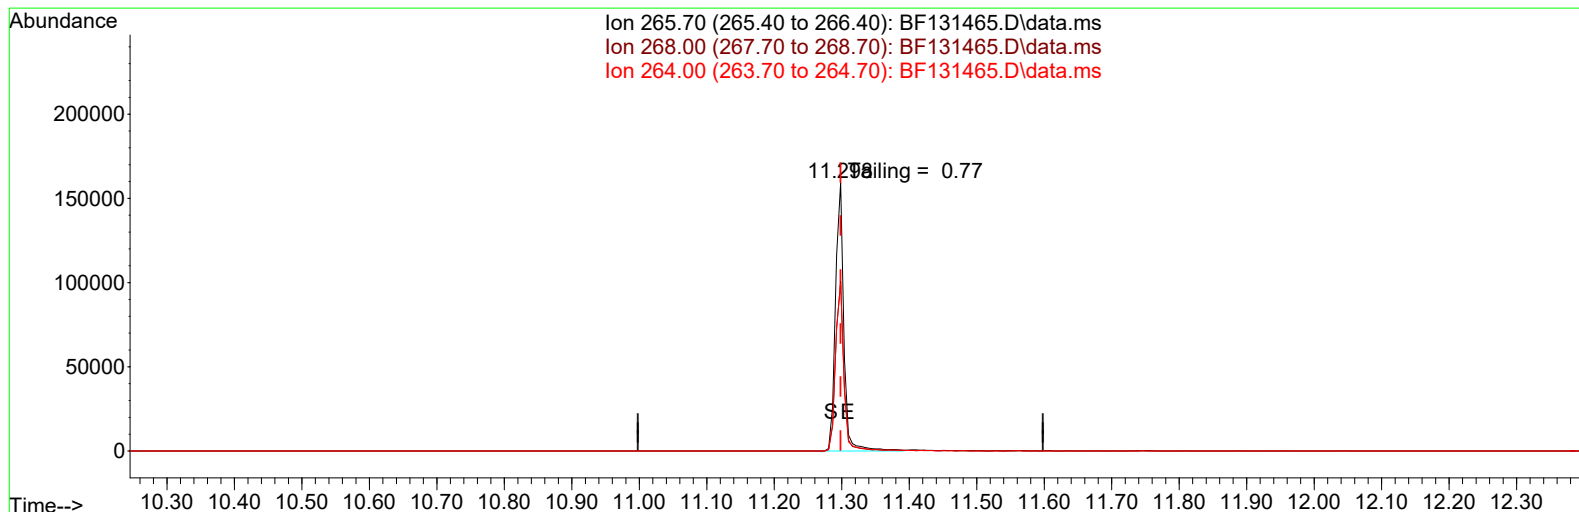

TIC: BF131465.D\data.ms

(70) Pentachlorophenol (C)

11.298min (+ 0.000) 31166.31 ng




response **137706**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.09
264.00	63.00	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113022\
Data File : BF131465.D
Acq On : 30 Nov 2022 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 01 04:31:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 01:09:58 2022
Response via : Initial Calibration

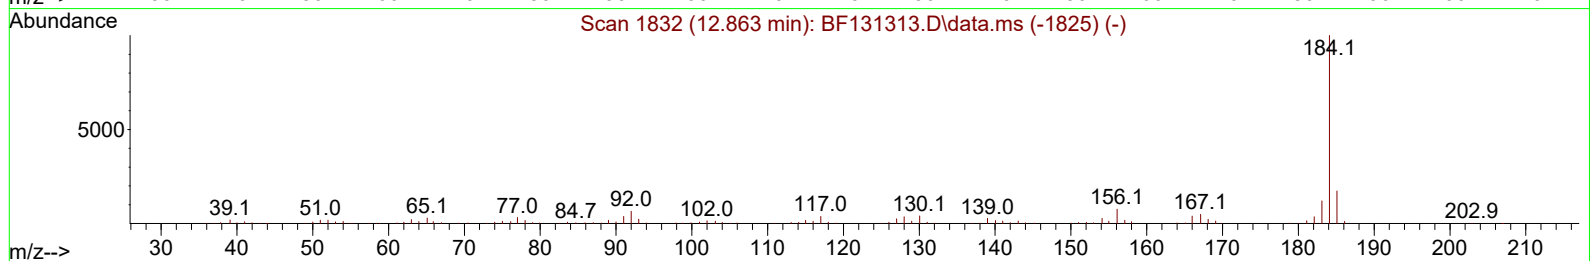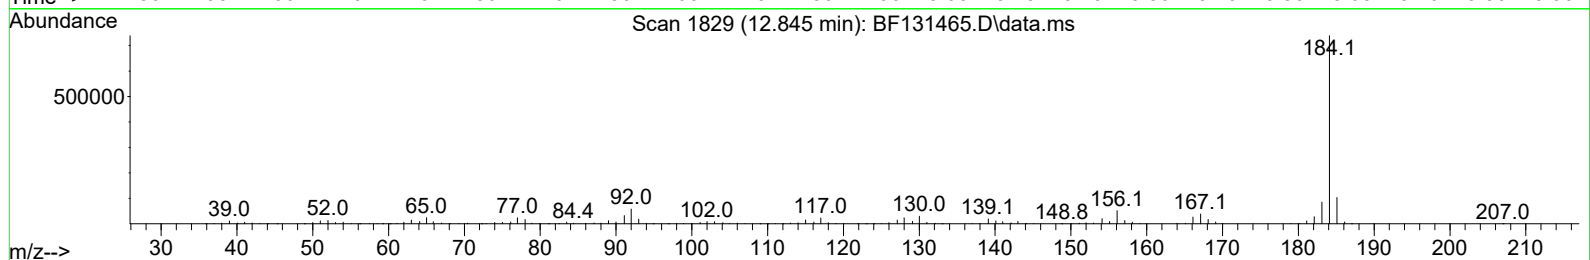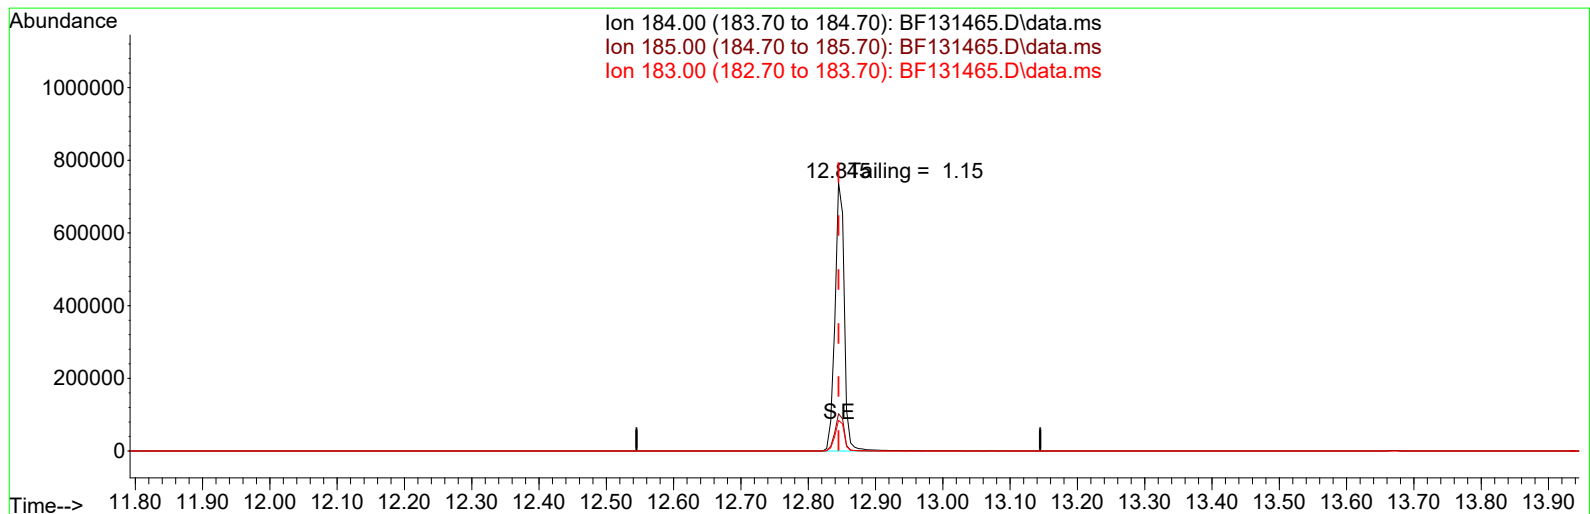

TIC: BF131465.D\data.ms

(77) Benzidine

12.845min (+ 0.000) 0.00 ng

response 709142

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	13.94
183.00	12.00	11.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2022	BNA_F	<u>BF131465.D</u>
Compound Name	Response	Retention Time
DDT	319296	13.669
DDD	5497	13.398
DDE	813	13.027
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6310	325606	1.94

Instrument :
BNA_F
ClientSampleId :
DFTPP