
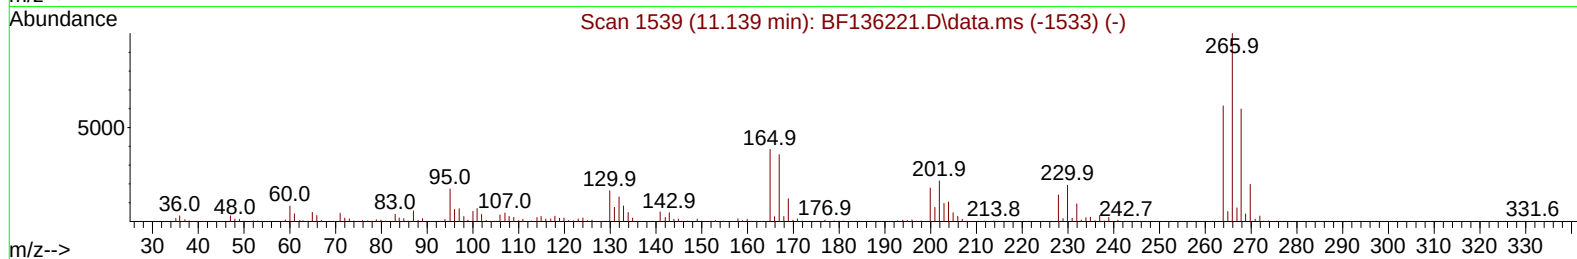
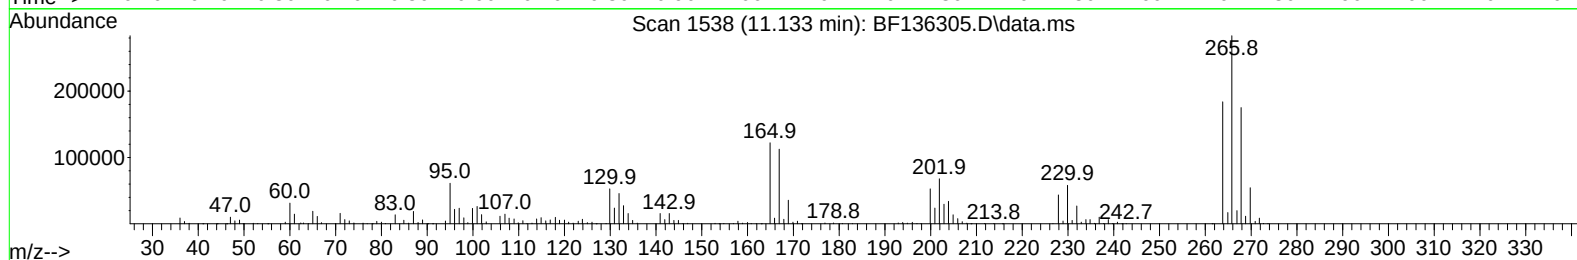


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF113023\  
Data File : BF136305.D  
Acq On : 30 Nov 2023 10:33  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 11:58:22 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 28 03:04:20 2023  
Response via : Initial Calibration

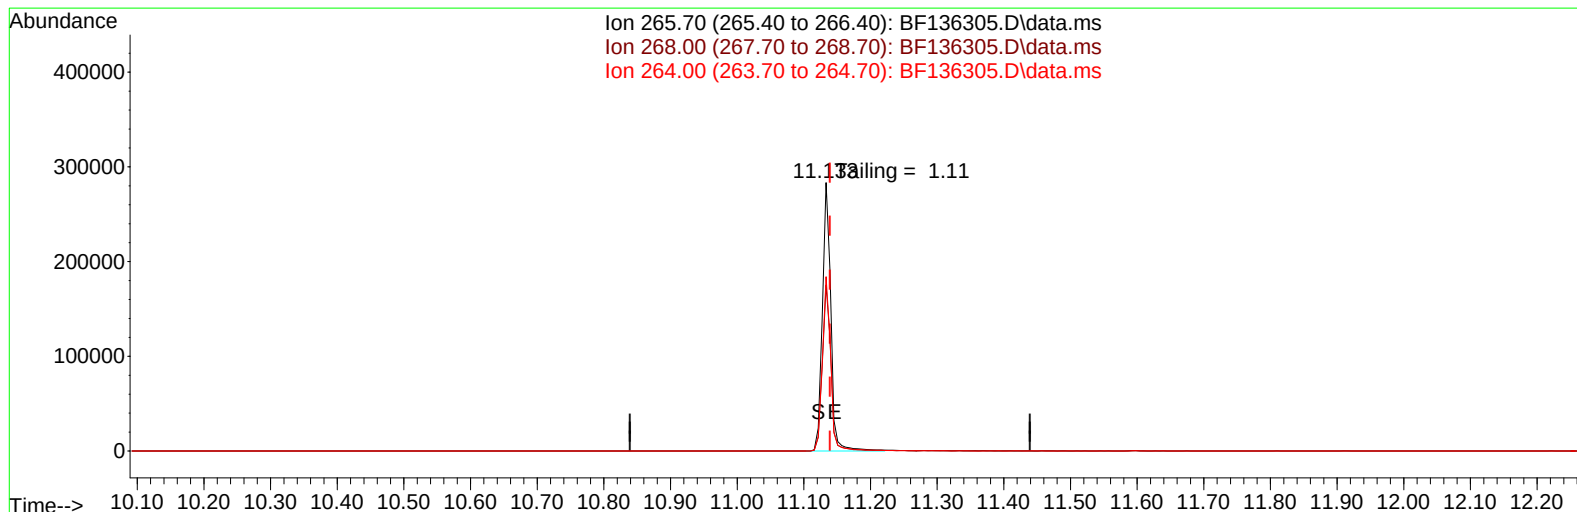

TIC: BF136305.D\data.ms

**(70) Pentachlorophenol (C)**




**11.133min (-0.006) 57311.66 ng**

**response 251520**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.90  | 61.79  |
| 264.00 | 61.40  | 64.91  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF113023\  
Data File : BF136305.D  
Acq On : 30 Nov 2023 10:33  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 11:58:22 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 28 03:04:20 2023  
Response via : Initial Calibration

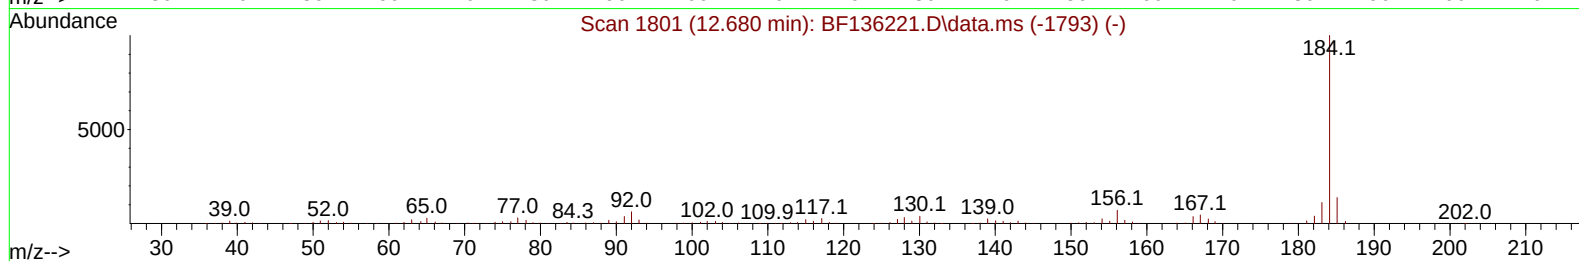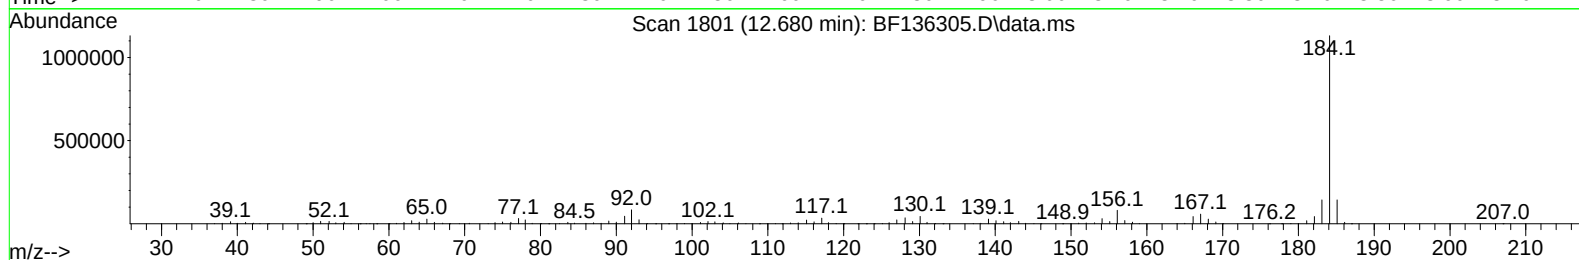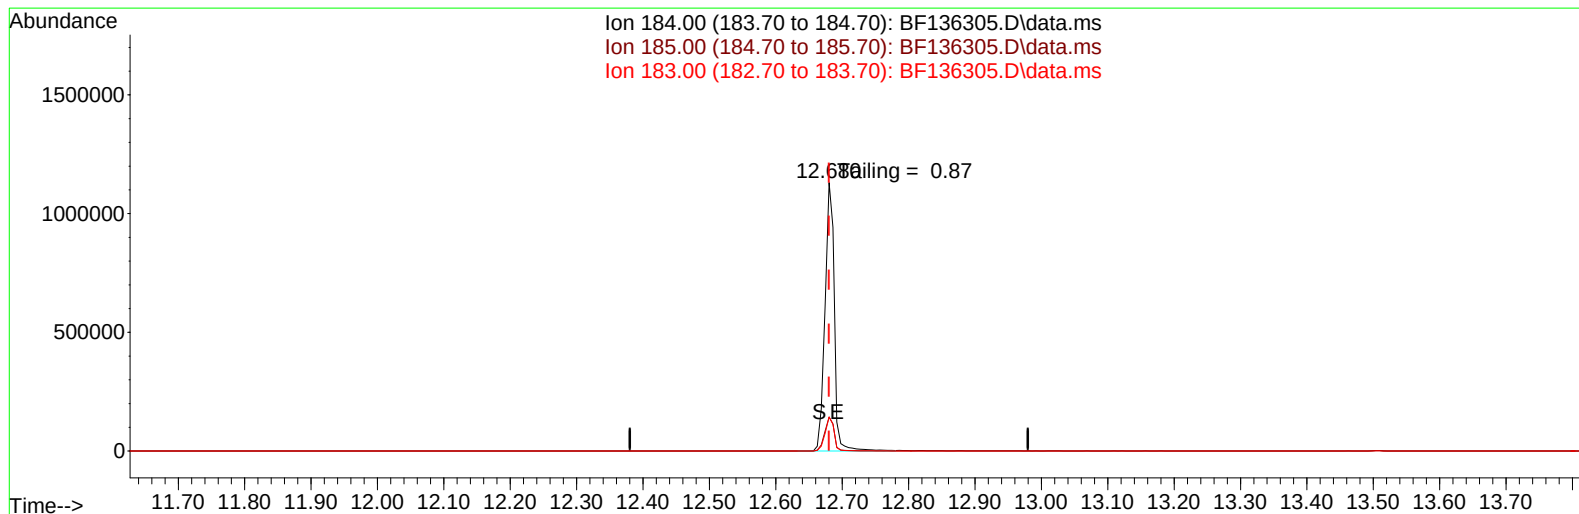

TIC: BF136305.D\data.ms

**(77) Benzidine****12.680min (+ 0.000) 193099.87 ng****response 1110979**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 12.66  |
| 183.00 | 11.20  | 12.70  |
| 0.00   | 0.00   | 0.00   |