


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113023\
Data File : BF136305.D
Acq On : 30 Nov 2023 10:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 28 03:04:20 2023

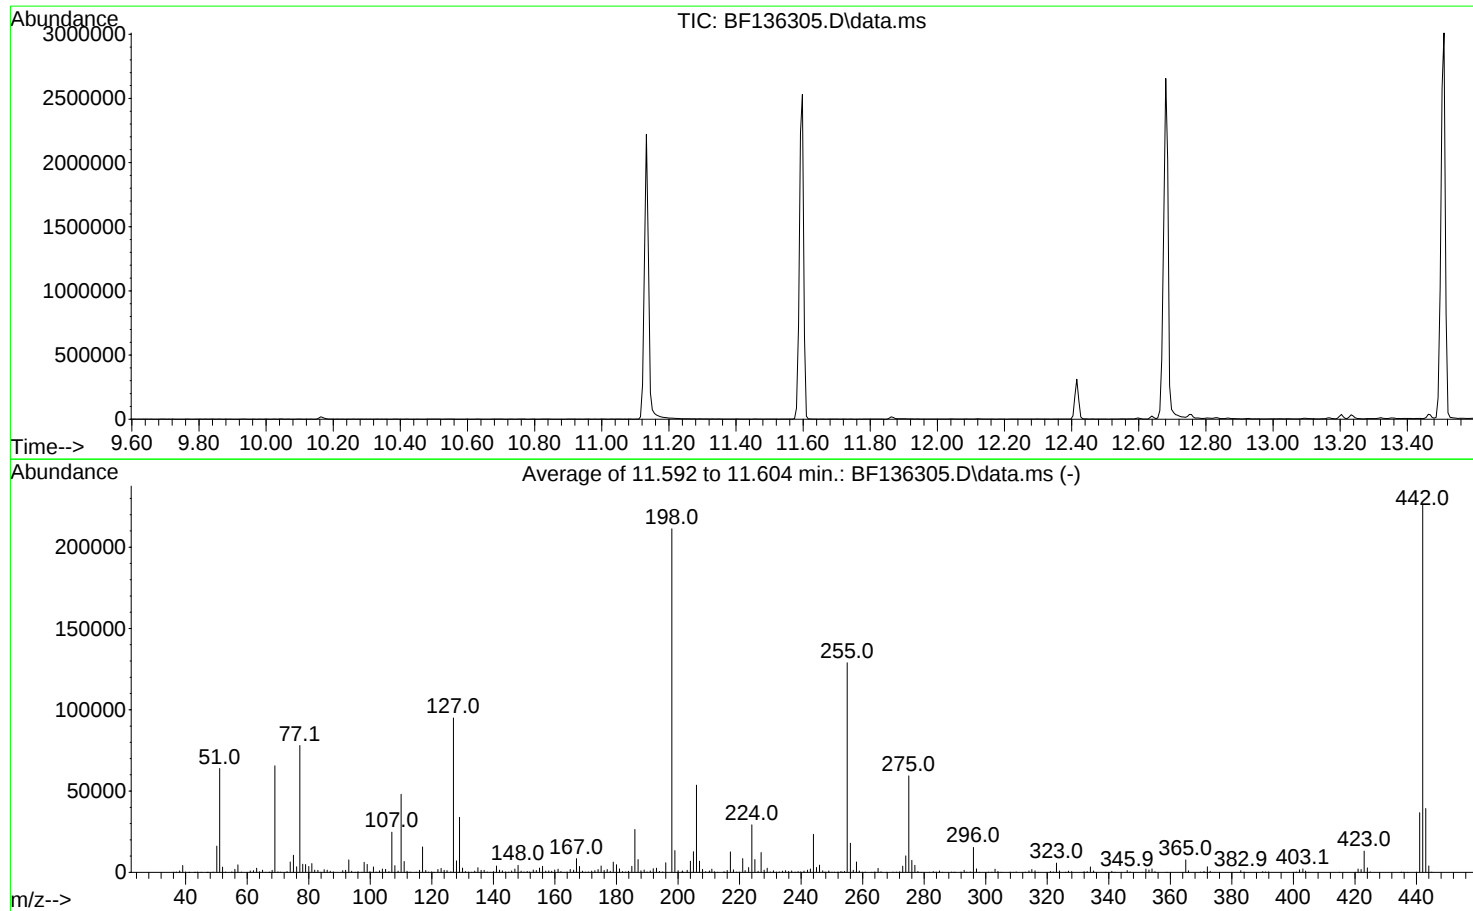




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	63854	PASS
68	69	0.00	2	1.9	1271	PASS
69	198	0.00	100	31.0	65562	PASS
70	69	0.00	2	0.5	335	PASS
127	198	10	80	45.0	95011	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	211253	PASS
199	198	5	9	6.3	13384	PASS
275	198	10	60	28.1	59363	PASS
365	198	1	100	3.6	7700	PASS
441	198	0.01	100	17.4	36685	PASS
442	442	50	100	100.0	226261	PASS
443	442	15	24	17.4	39296	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113023\
 Data File : BF136305.D
 Acq On : 30 Nov 2023 10:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 30 11:58:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 28 03:04:20 2023
 Response via : Initial Calibration

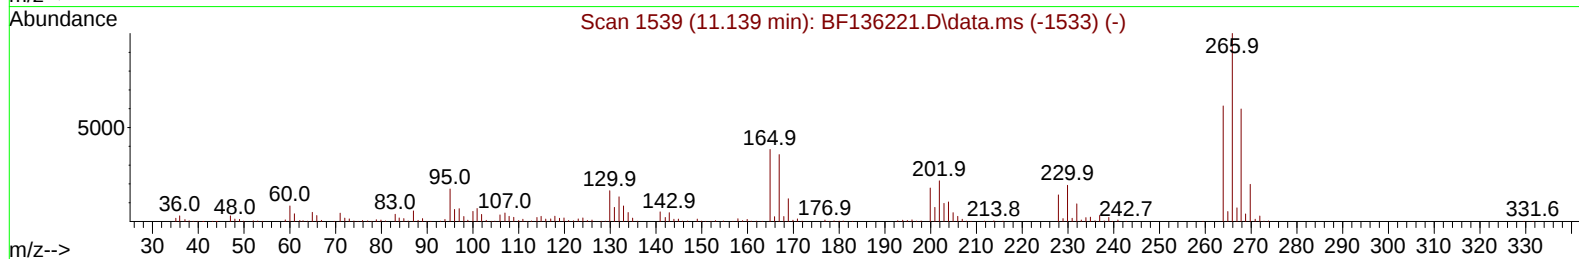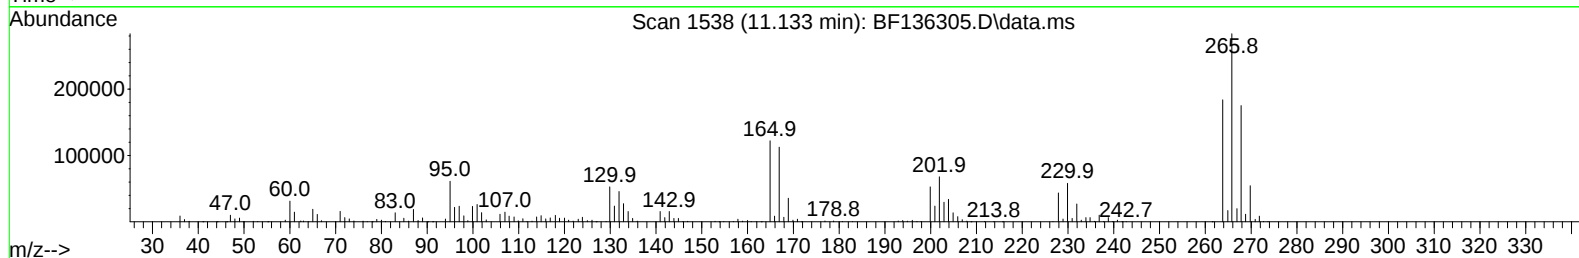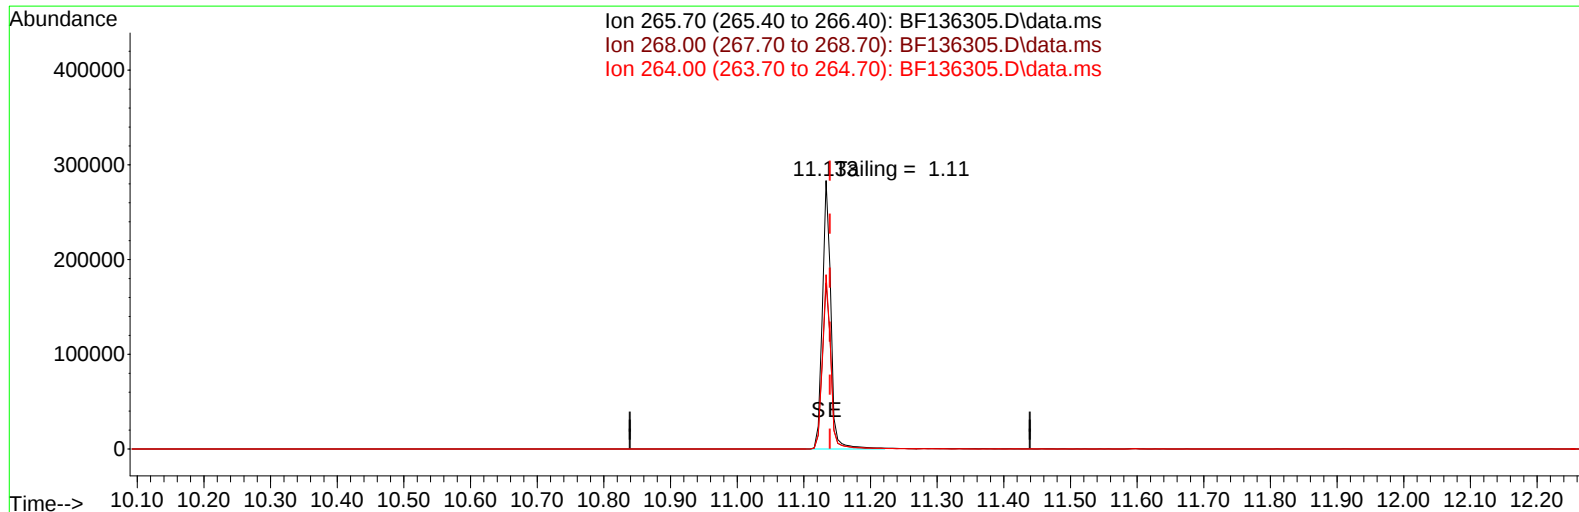

TIC: BF136305.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 57311.66 ng




response 251520

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.79
264.00	61.40	64.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113023\
Data File : BF136305.D
Acq On : 30 Nov 2023 10:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 30 11:58:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

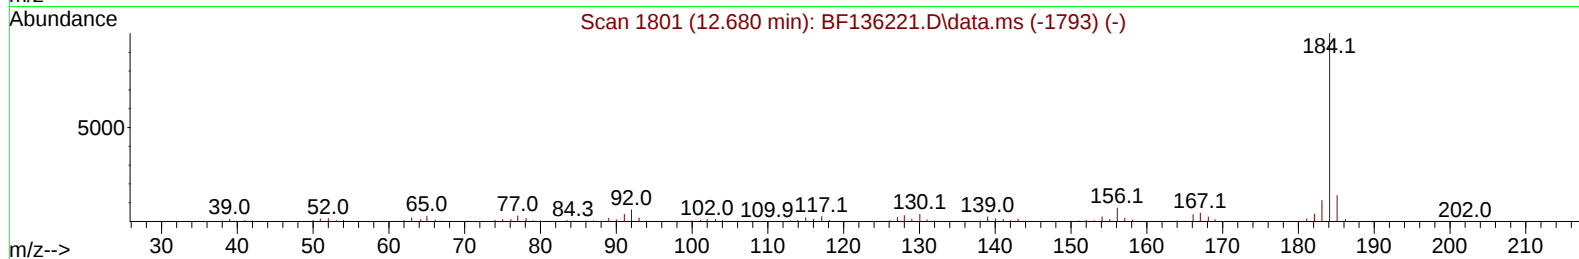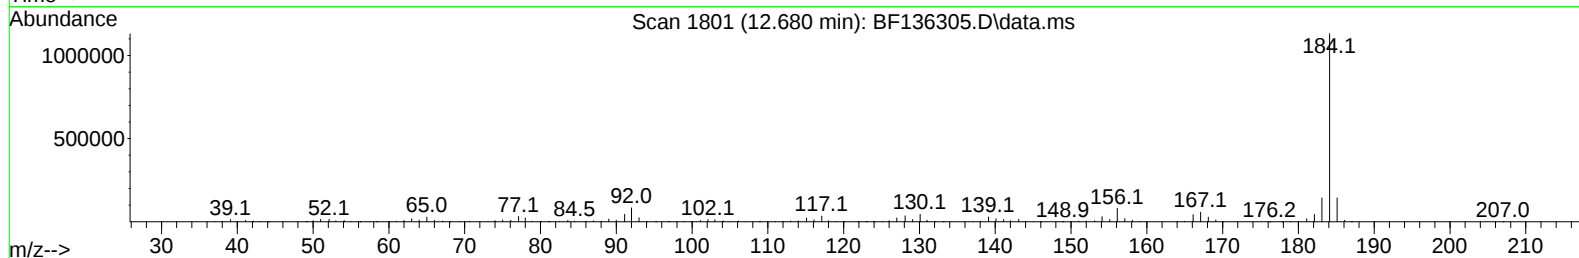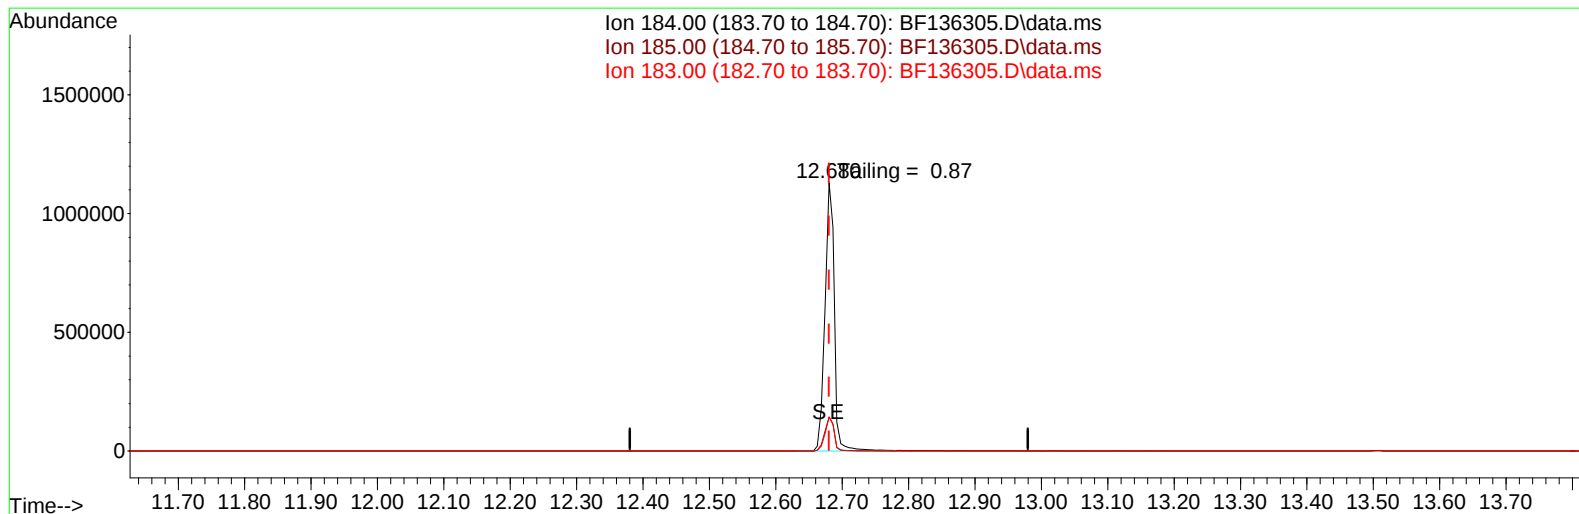

TIC: BF136305.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 193099.87 ng

response 1110979

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	12.66
183.00	11.20	12.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2023	BNA_F	<u>BF136305.D</u>
Compound Name	Response	Retention Time
DDT	587943	13.51
DDD	11082	13.204
DDE	1123	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12205	600148	2.03

Instrument :
BNA_F
ClientSampleId :
DFTPP