

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120115\
 Data File : BF083405.D
 Acq On : 2 Dec 2015 7:46
 Operator : UM/IZ
 Sample : G4586-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 112515-A263-F-U-B

Quant Time: Dec 02 09:32:52 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 01:17:16 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.54	152	165646	20.00	ng	0.00
21) Naphthalene-d8	7.84	136	638880	20.00	ng	0.00
38) Acenaphthene-d10	9.58	164	319272	20.00	ng	0.00
63) Phenanthrene-d10	11.13	188	575274	20.00	ng	0.00
75) Chrysene-d12	14.75	240	415425	20.00	ng	-0.01
86) Perylene-d12	16.82	264	412092	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	420328	38.08	ng	0.00
7) Phenol-d6	6.21	99	341273	22.59	ng	-0.01
23) Nitrobenzene-d5	7.12	82	1128131	77.62	ng	-0.01
41) 2,4,6-Tribromophenol	10.37	330	233225	72.77	ng	-0.01
44) 2-Fluorobiphenyl	8.92	172	1924587	85.90	ng	0.00
78) Terphenyl-d14	13.22	244	1543869	88.63	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120115\
Data File : BF083405.D
Acq On : 2 Dec 2015 7:46
Operator : UM/IZ
Sample : G4586-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112515-A263-F-U-B

Quant Time: Dec 02 09:32:52 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

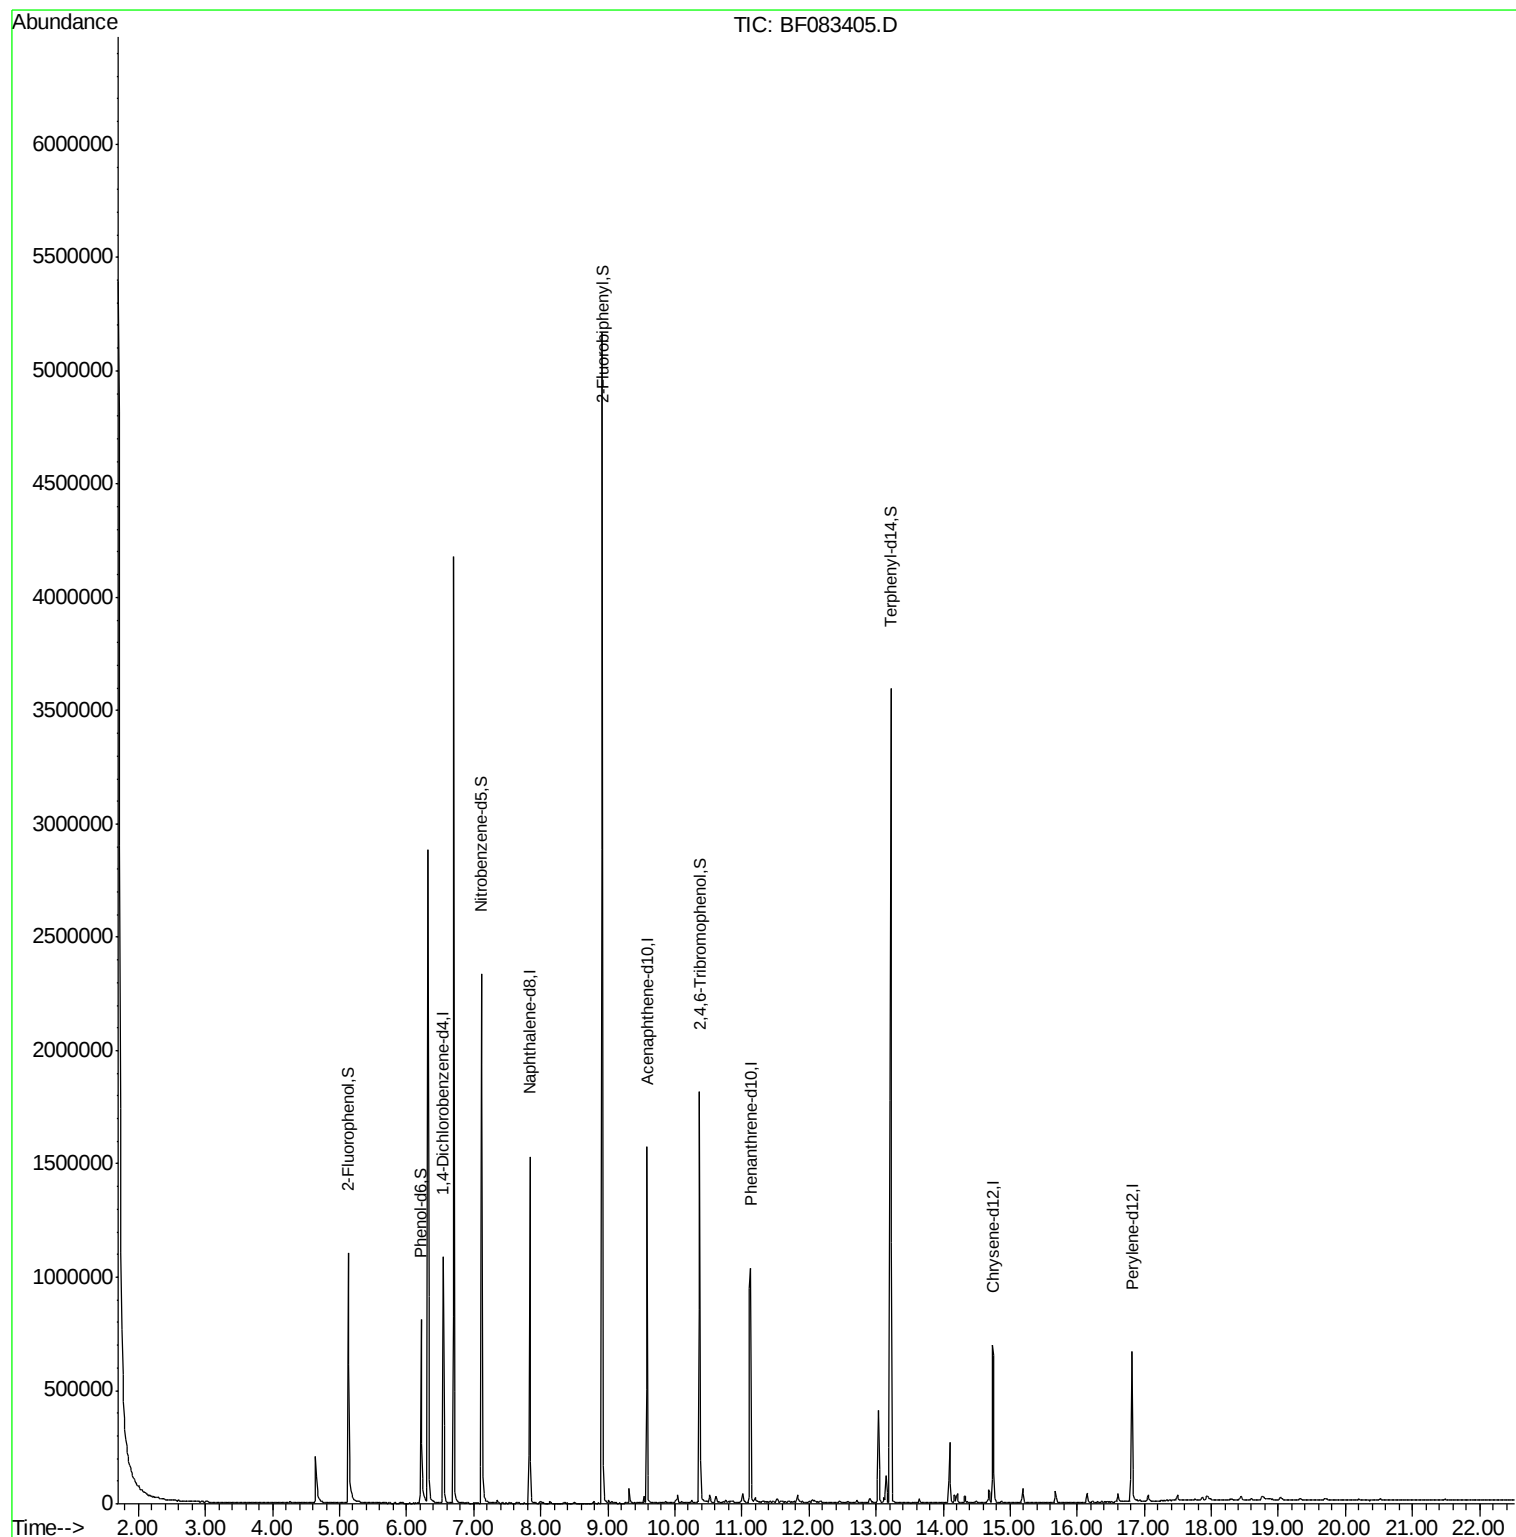

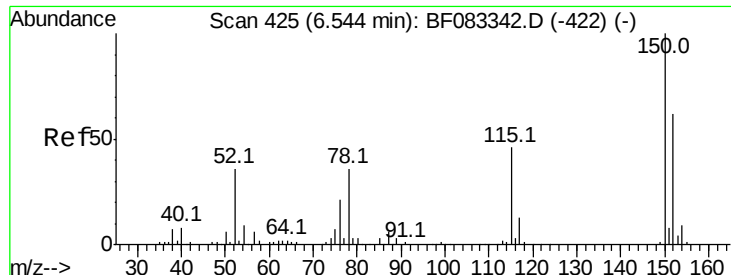

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.54 min Scan# 425

Delta R.T. -0.00 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46

Instrument :

BNA_F

ClientSampleId :

112515-A263-F-U-B


Tot Ion:152 Resp: 165646

Ion Ratio Lower Upper

152 100

150 156.4 129.8 194.8




115 68.9 59.2 88.8

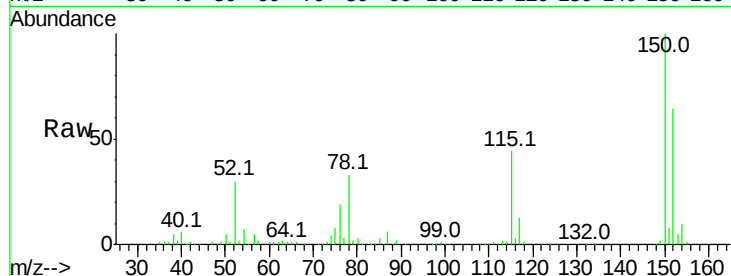

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

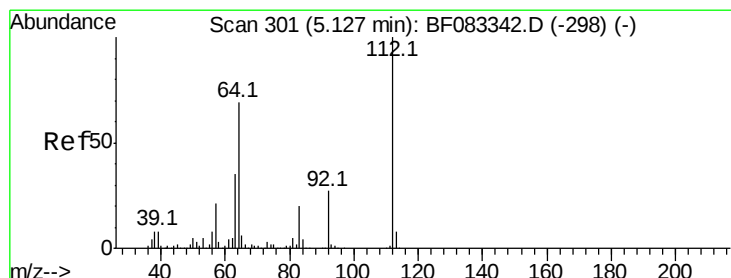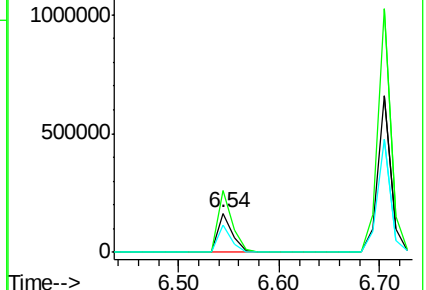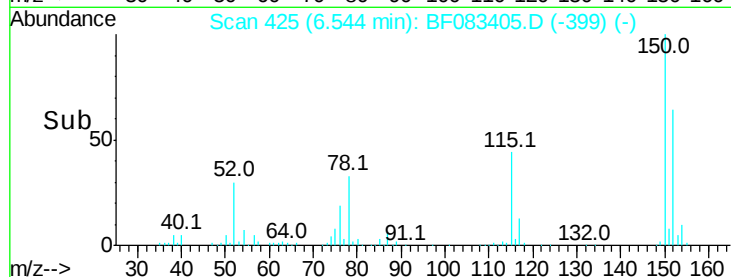

#5

2-Fluorophenol

Concen: 38.08 ng

RT: 5.13 min Scan# 301

Delta R.T. -0.00 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46


Tgt Ion:112 Resp: 420328

Ion Ratio Lower Upper

112 100

64 72.9 55.6 83.4



63 35.8 28.2 42.2

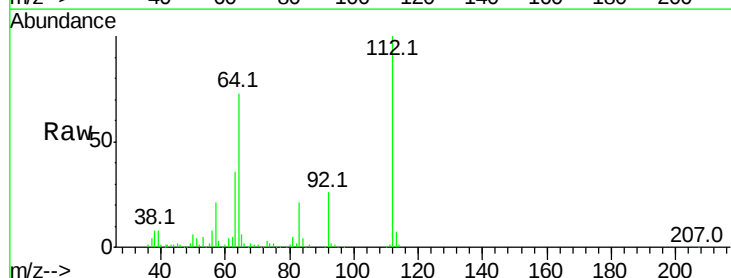


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

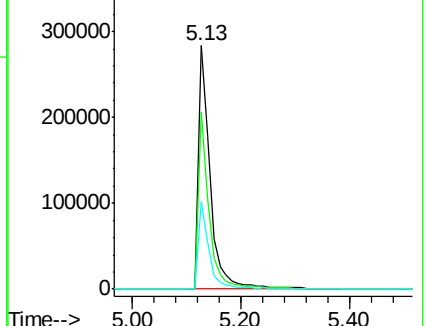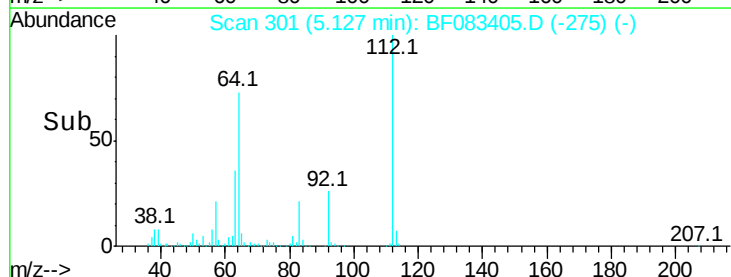

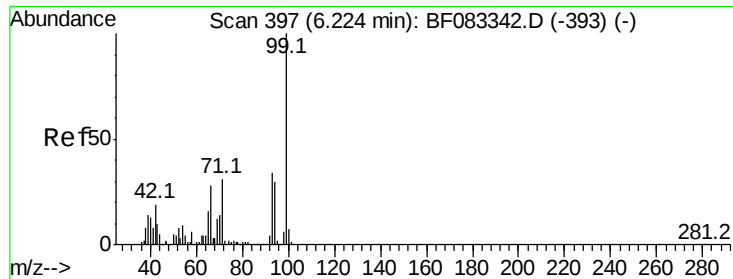

#7

Phenol-d6

Concen: 22.59 ng

RT: 6.21 min Scan# 396

Delta R.T. -0.01 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46

Instrument :

BNA_F

ClientSampleId :

112515-A263-F-U-B





Tot Ion: 99 Resp: 341273

Ion Ratio Lower Upper

99 100

42 19.1 14.9 22.3

71 31.5 24.7 37.1

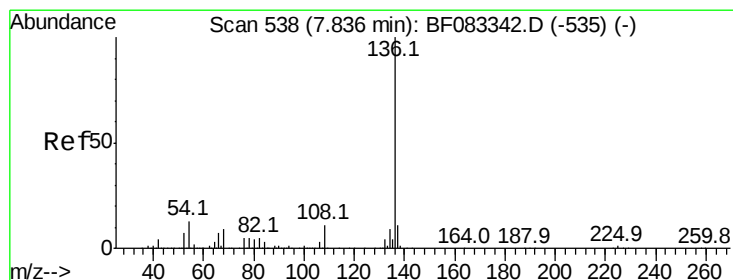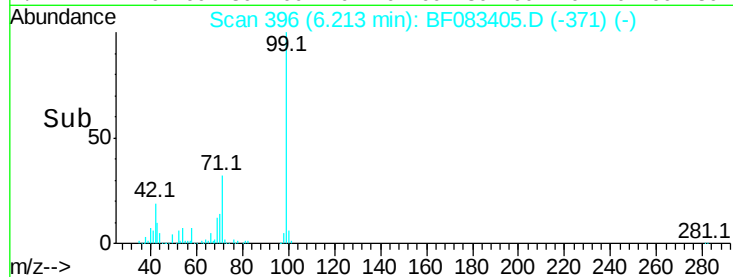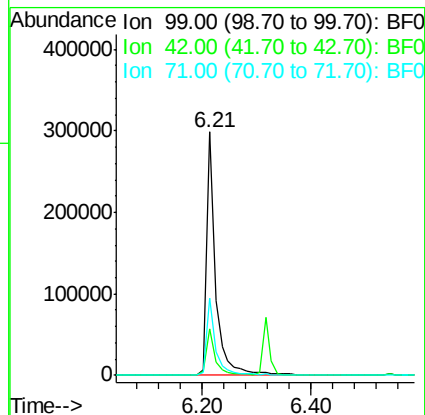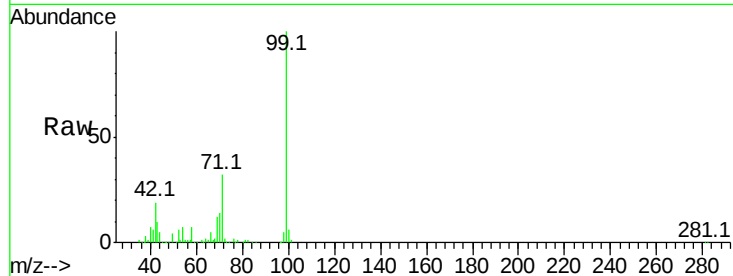

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.84 min Scan# 538

Delta R.T. -0.00 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46

Tgt Ion: 136 Resp: 638880




Ion Ratio Lower Upper


136 100

137 11.1 9.0 13.4

54 10.0 10.1 15.1#

68 7.0 7.1 10.7#

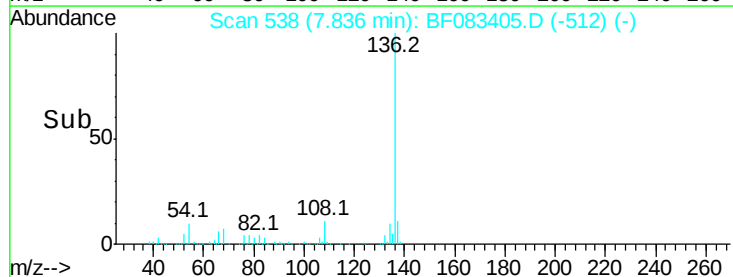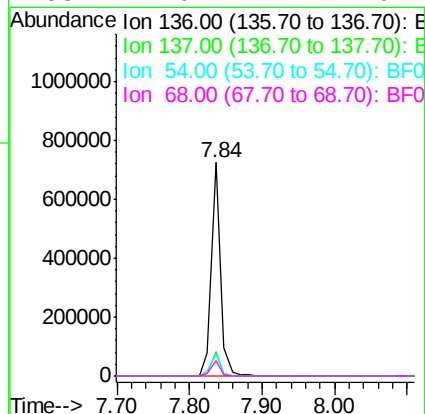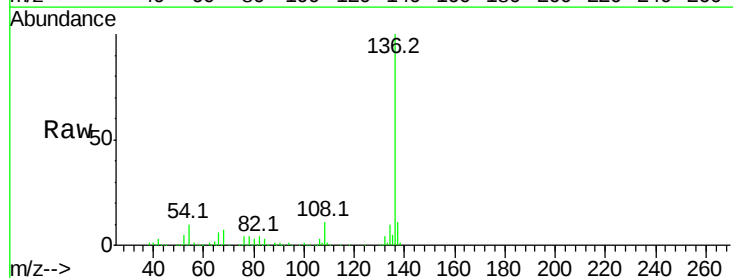




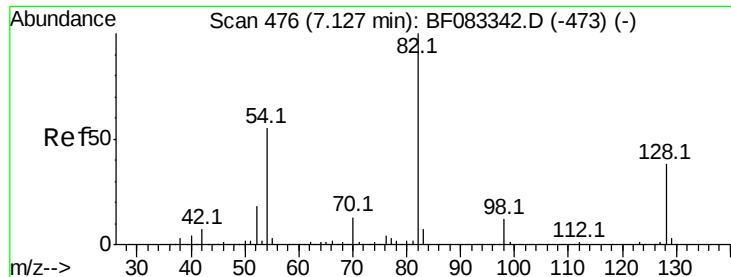


#23
 Nitrobenzene-d5
 Concen: 77.62 ng
 RT: 7.12 min Scan# 475
 Delta R.T. -0.01 min
 Lab File: BF083405.D
 Acq: 2 Dec 2015 7:46

Instrument :
 BNA_F
 ClientSampleId :
 112515-A263-F-U-B

Tot Ion: 82 Resp: 1128131




Ion	Ratio	Lower	Upper
82	100		
128	35.0	30.6	46.0
54	56.3	43.8	65.6

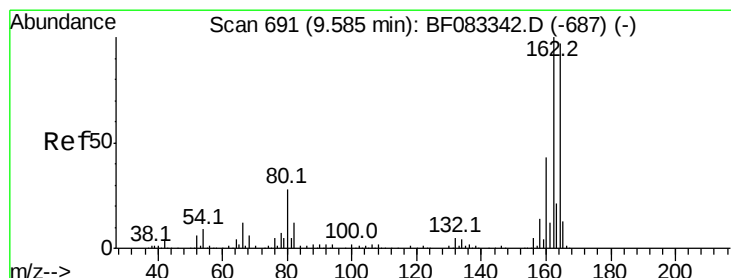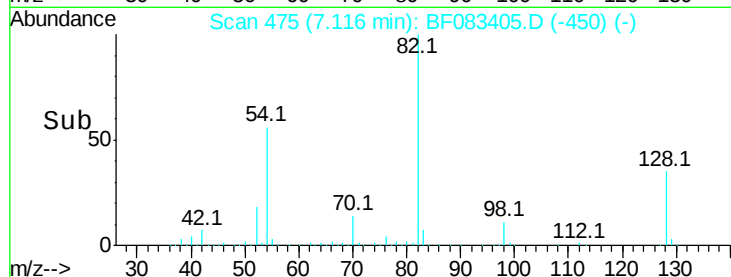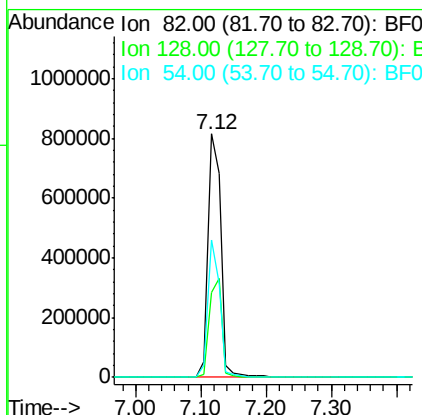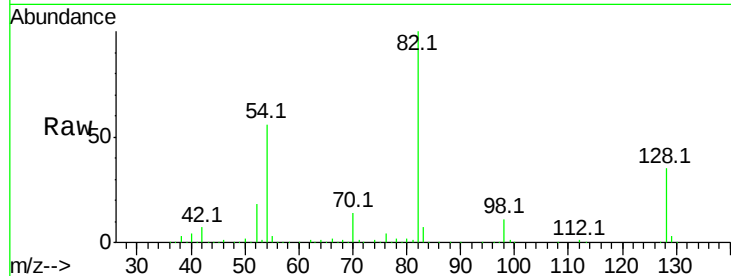


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.58 min Scan# 691
 Delta R.T. -0.00 min
 Lab File: BF083405.D
 Acq: 2 Dec 2015 7:46

Tgt Ion: 164 Resp: 319272

Ion	Ratio	Lower	Upper
164	100		
162	105.7	82.6	123.8
160	45.6	35.3	52.9

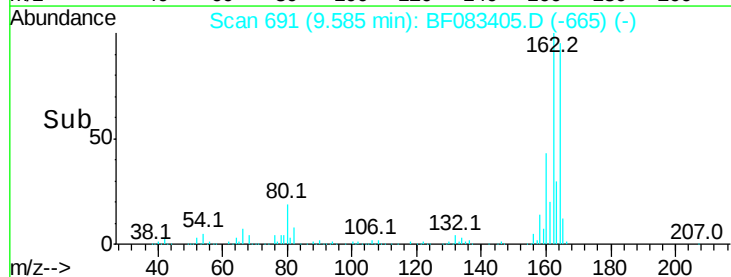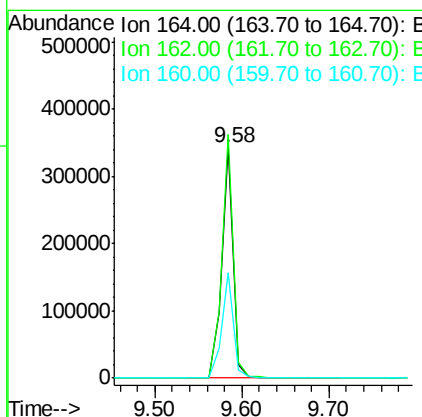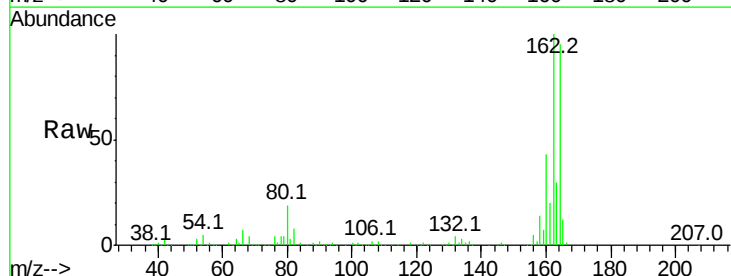


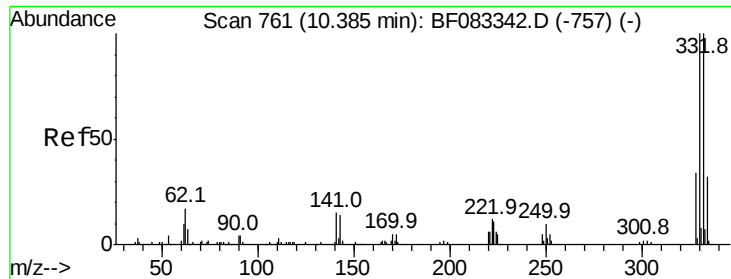




#41
 2,4,6-Tribromophenol
 Concen: 72.77 ng
 RT: 10.37 min Scan# 760
 Delta R.T. -0.01 min
 Lab File: BF083405.D
 Acq: 2 Dec 2015 7:46

Instrument :
 BNA_F
 ClientSampleId :
 112515-A263-F-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.2	77.8	116.6
141	37.3	29.4	44.0

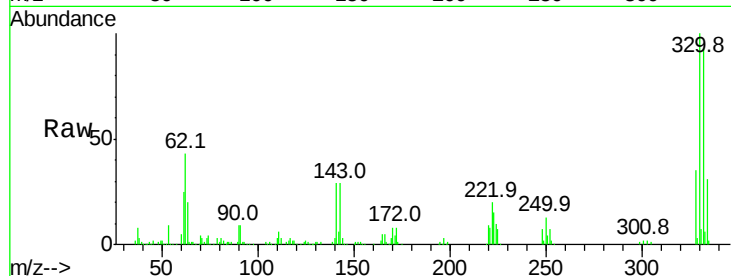


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

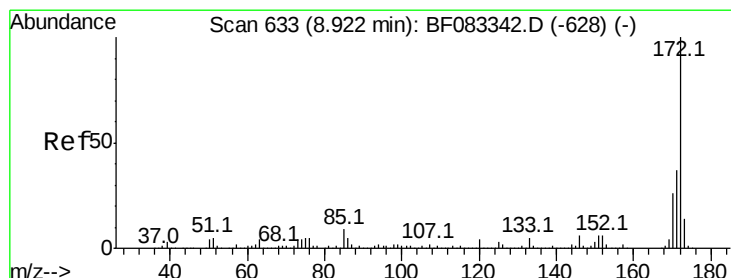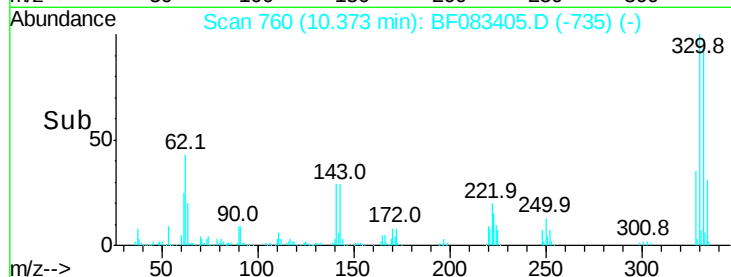
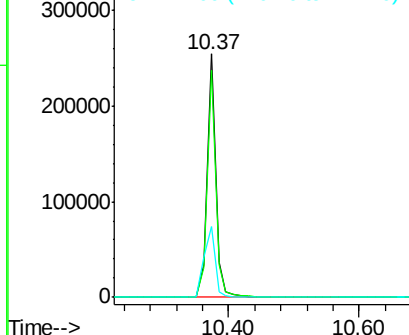



#44
 2-Fluorobiphenyl
 Concen: 85.90 ng
 RT: 8.92 min Scan# 633
 Delta R.T. -0.00 min
 Lab File: BF083405.D
 Acq: 2 Dec 2015 7:46

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.4	44.0
170	24.5	20.4	30.6

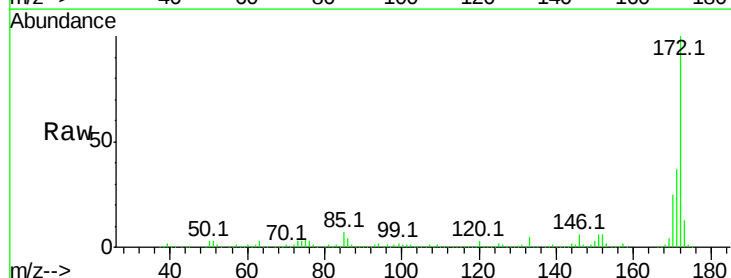

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

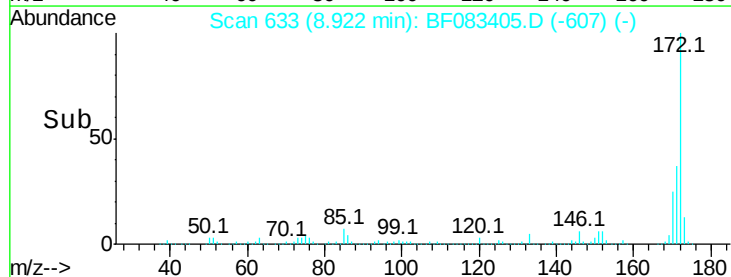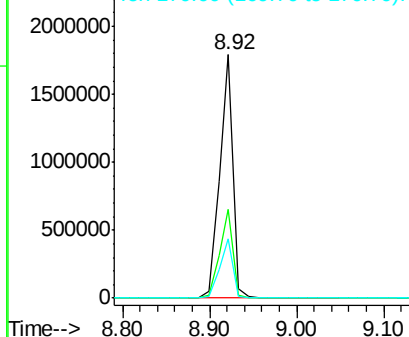

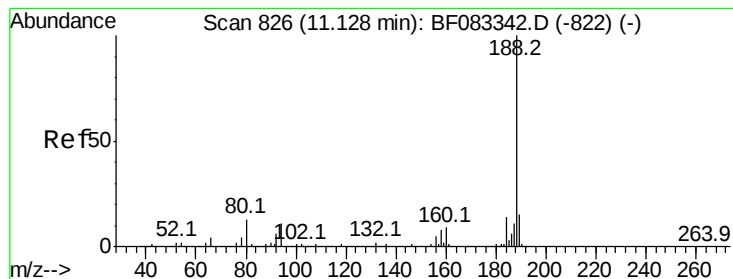

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.13 min Scan# 826

Delta R.T. -0.00 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46

Instrument :

BNA_F

ClientSampleId :

112515-A263-F-U-B


Tot Ion:188 Resp: 575274

Ion Ratio Lower Upper

188 100

94 7.3 8.7 13.1#




80 8.5 10.3 15.5#

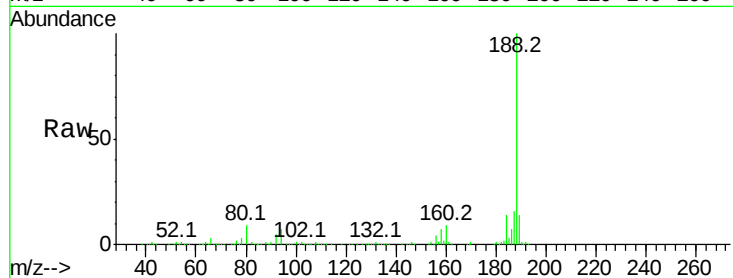

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

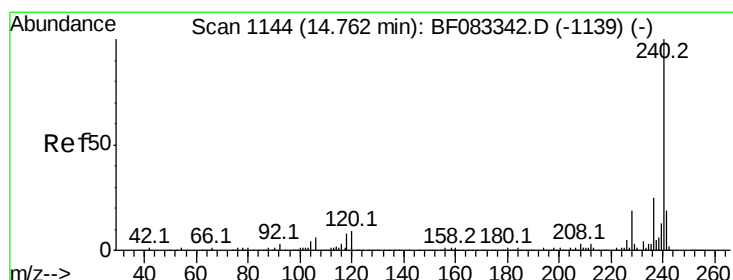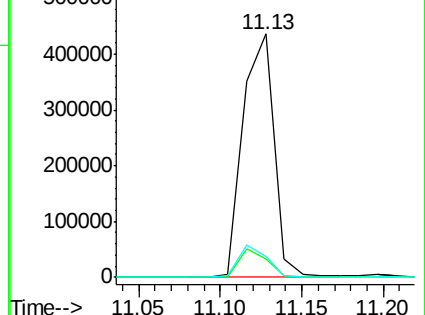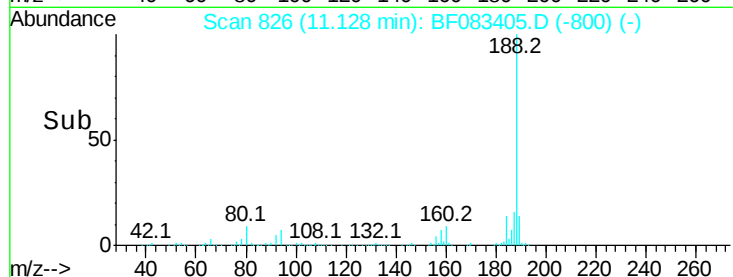

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.75 min Scan# 1143

Delta R.T. -0.01 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46


Tgt Ion:240 Resp: 415425

Ion Ratio Lower Upper

240 100

120 8.5 6.9 10.3



236 25.1 19.8 29.6

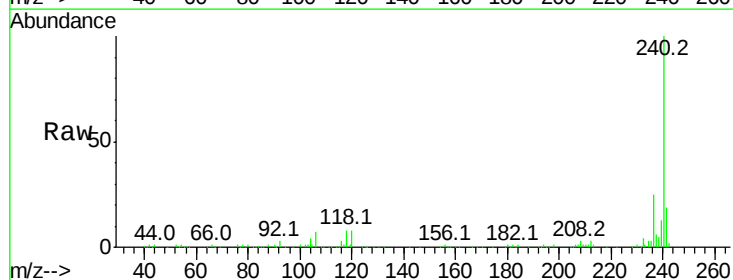


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

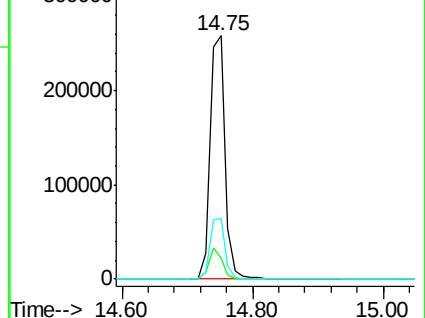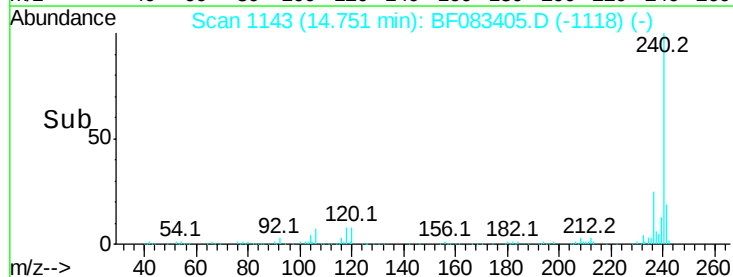

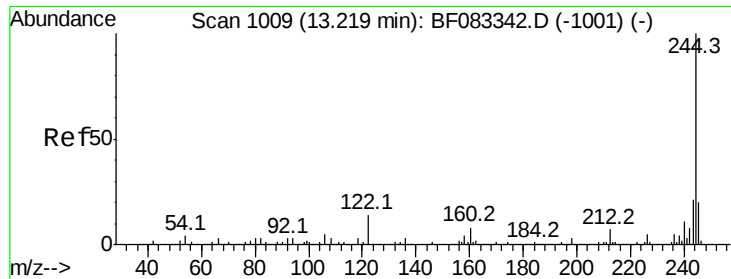

#78

Terphenyl-d14

Concen: 88.63 ng

RT: 13.22 min Scan# 1009

Delta R.T. -0.00 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46

Instrument :

BNA_F

ClientSampleId :

112515-A263-F-U-B


Tot Ion:244 Resp: 1543869

Ion Ratio Lower Upper




244 100

212 7.6 5.8 8.8

122 12.6 11.0 16.4

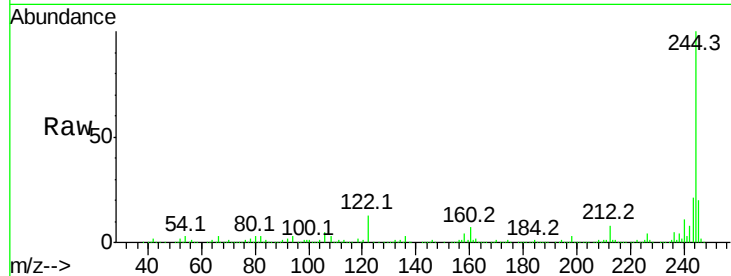

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

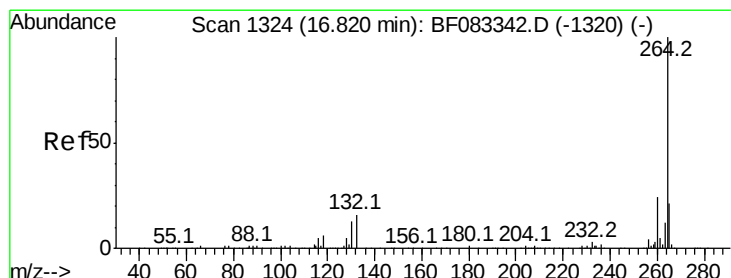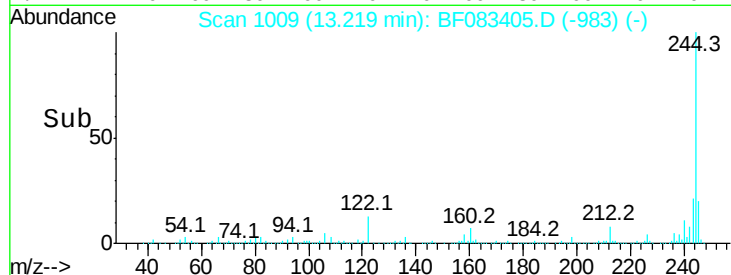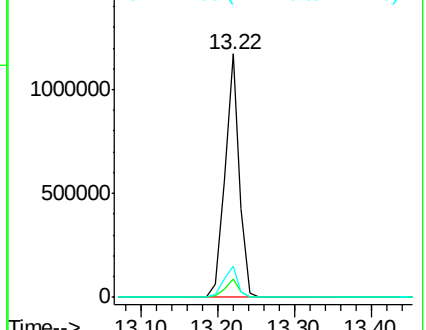

#86

Perylene-d12

Concen: 20.00 ng

RT: 16.82 min Scan# 1324

Delta R.T. -0.00 min

Lab File: BF083405.D

Acq: 2 Dec 2015 7:46


Tgt Ion:264 Resp: 412092

Ion Ratio Lower Upper

264 100

260 23.1 19.0 28.4

265 21.1 16.8 25.2

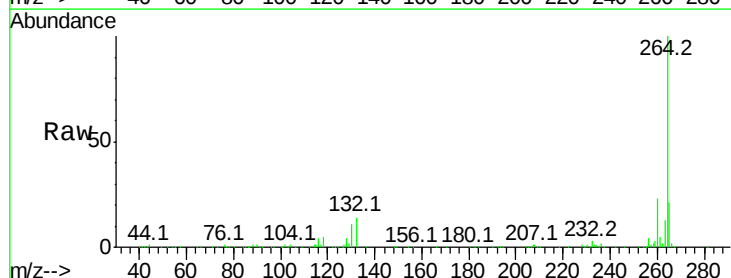

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

