

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120115\
 Data File : BF083398.D
 Acq On : 2 Dec 2015 4:05
 Operator : UM/IZ
 Sample : G4587-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-05

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.647	256	259	272	rBV	411127	635092	9.70%	1.519%
2	5.127	299	301	318	rBV	2064716	2439155	37.25%	5.836%
3	6.213	394	396	403	rBV	1473529	1536606	23.47%	3.676%
4	6.316	403	405	408	rBV	3943071	4104302	62.69%	9.819%
5	6.545	423	425	428	rBV	1145681	1059939	16.19%	2.536%
6	6.705	437	439	441	rBV	4427077	4095463	62.55%	9.798%
7	7.116	473	475	478	rBV	2549714	3535182	53.99%	8.458%
8	7.836	535	538	540	rBV	1557325	1395378	21.31%	3.338%
9	8.922	630	633	635	rBV	5815193	6547287	100.00%	15.664%
10	9.322	666	668	670	rBV	128079	116492	1.78%	0.279%
11	9.585	688	691	693	rBV	1674891	1611950	24.62%	3.857%
12	10.374	757	760	763	rBV	3537144	3677736	56.17%	8.799%
13	10.522	771	773	776	rVV	42931	66561	1.02%	0.159%
14	10.614	779	781	784	rVB2	75230	79464	1.21%	0.190%
15	11.128	823	826	828	rBV	1251034	1666541	25.45%	3.987%
16	11.825	884	887	892	rBV2	68150	122271	1.87%	0.293%
17	12.899	979	981	988	rBV3	34268	71280	1.09%	0.171%
18	13.220	1005	1009	1012	rBV	3939672	6398771	97.73%	15.309%
19	14.683	1133	1137	1140	rBV	35877	92618	1.41%	0.222%
20	14.740	1140	1142	1146	rVV	879414	1401909	21.41%	3.354%
21	16.808	1320	1323	1331	rBV	722814	1143646	17.47%	2.736%


Sum of corrected areas: 41797643

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120115\
Data File : BF083398.D
Acq On : 2 Dec 2015 4:05
Operator : UM/IZ
Sample : G4587-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

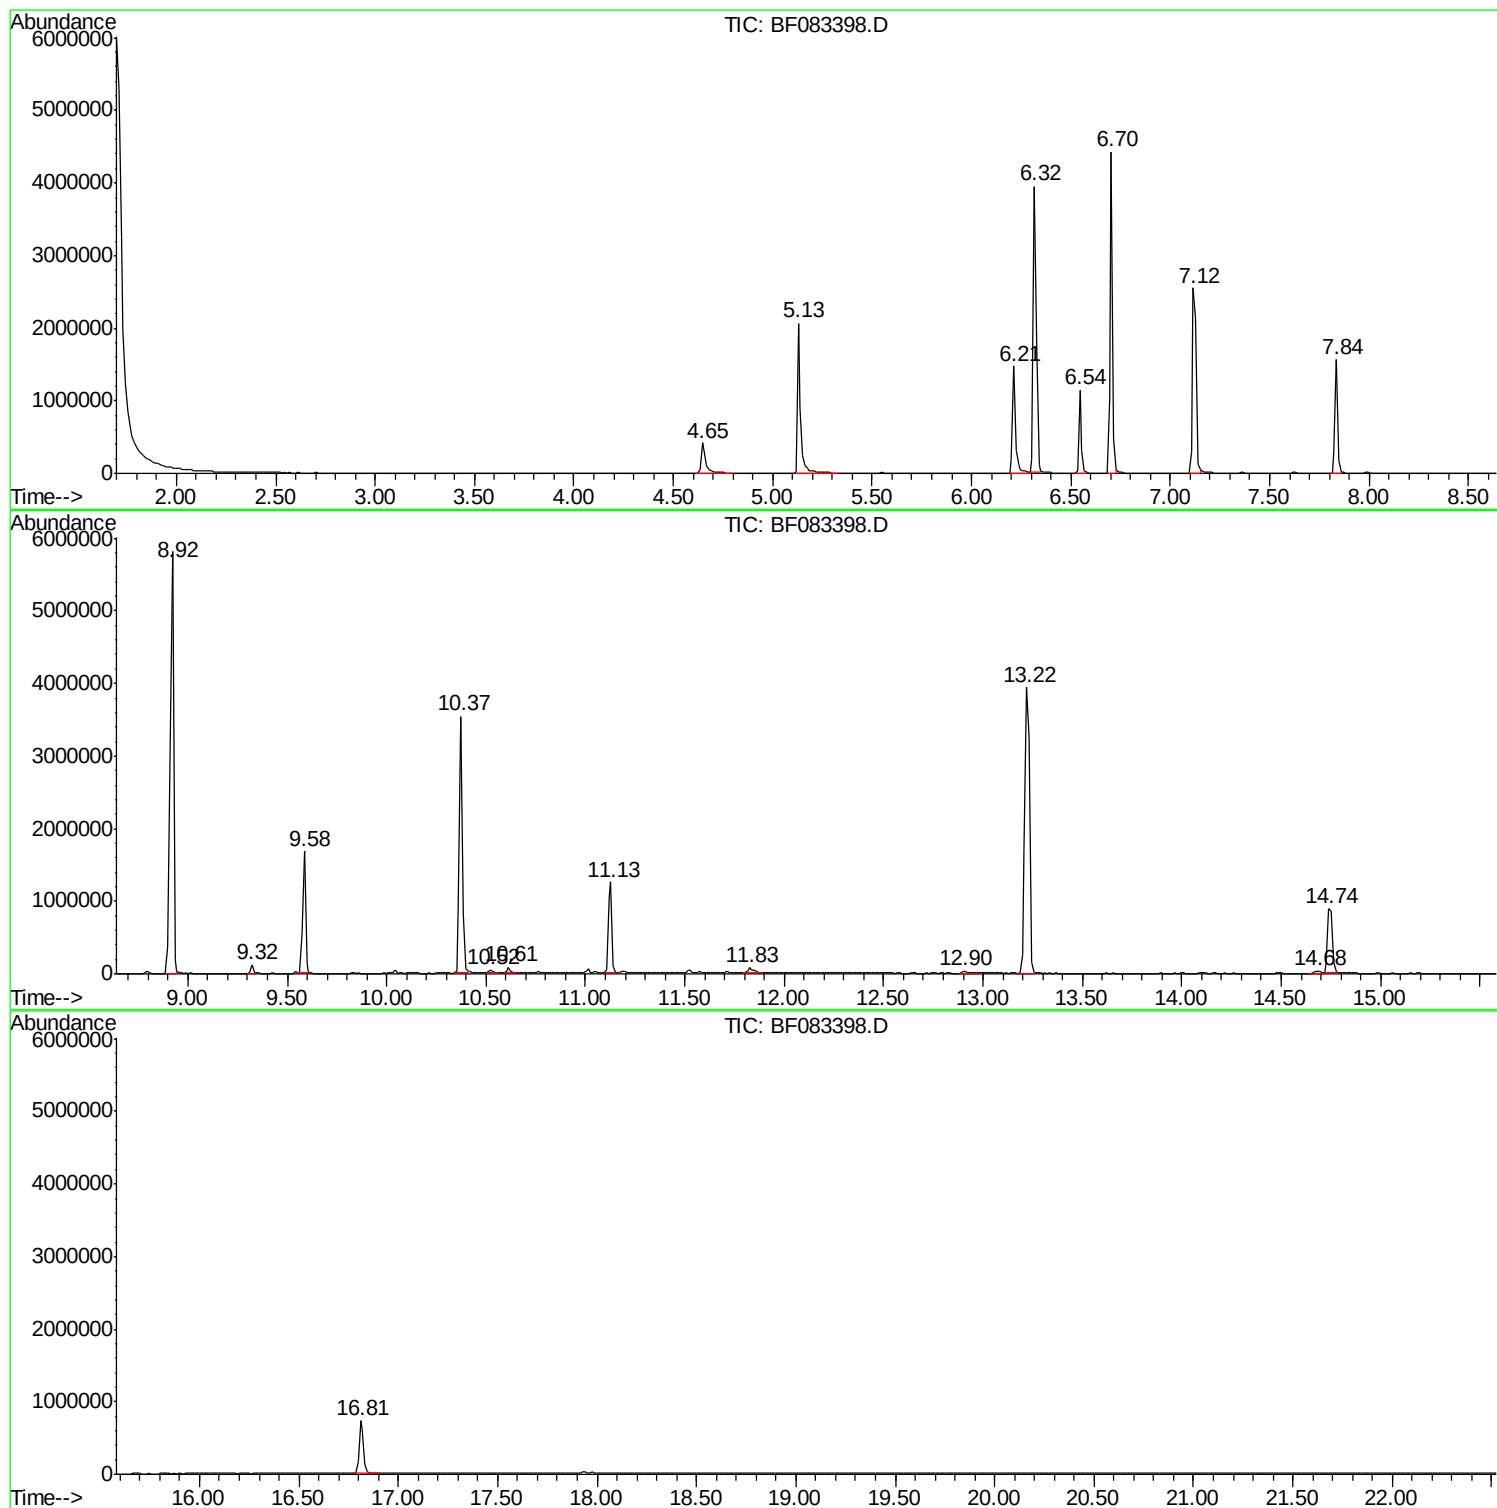

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120115\
Data File : BF083398.D
Acq On : 2 Dec 2015 4:05
Operator : UM/IZ
Sample : G4587-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.65	11.98 ng	635092	1,4-Dichlorobenzene-d4	6.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
3		3-Hexanol	102	C6H14O	000623-37-0	33
4		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
5		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25

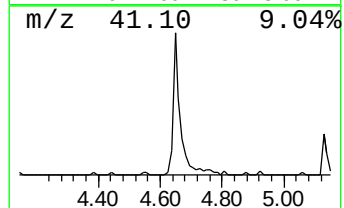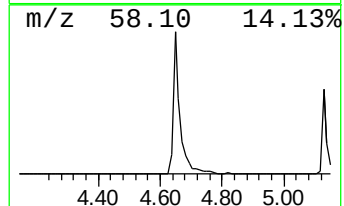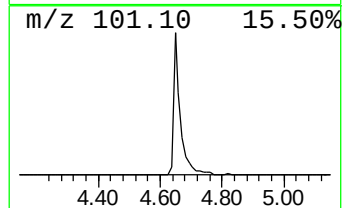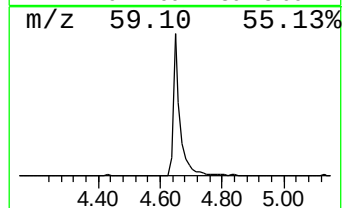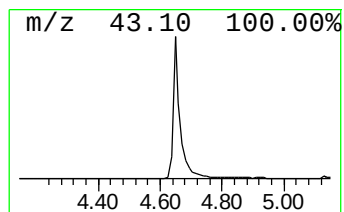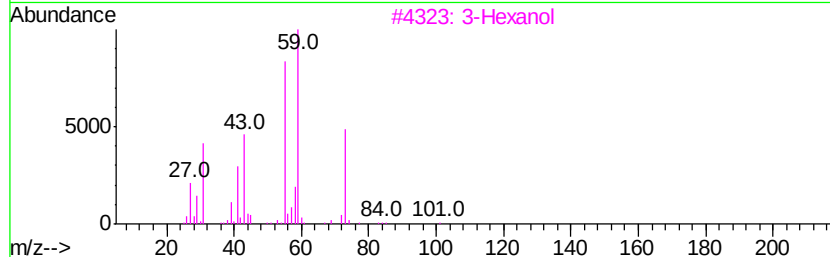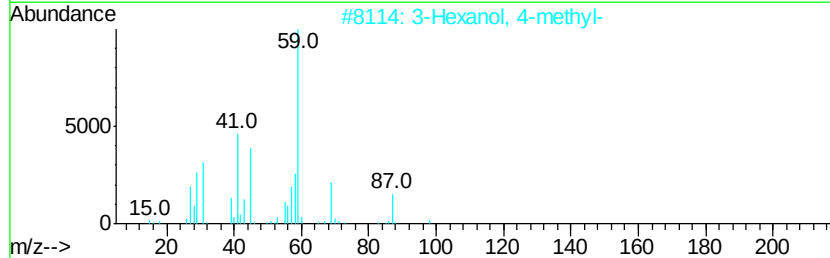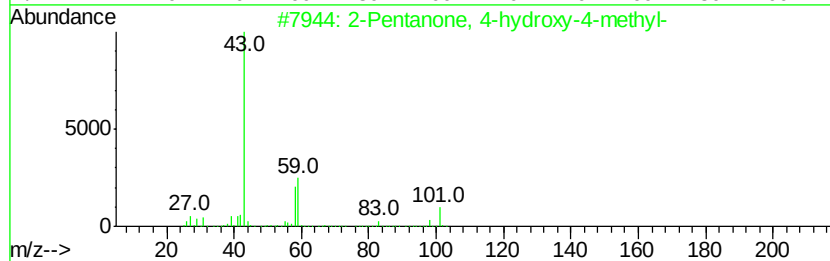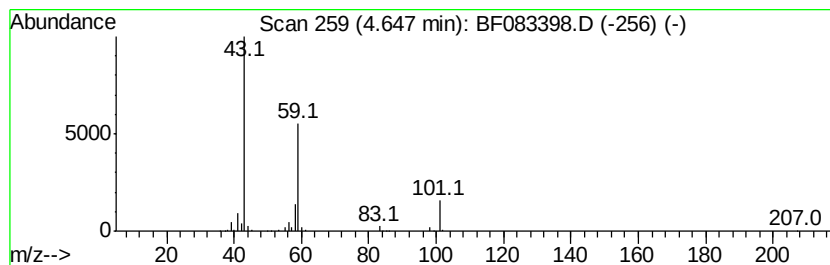

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120115\
Data File : BF083398.D
Acq On : 2 Dec 2015 4:05
Operator : UM/IZ
Sample : G4587-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.32	77.44 ng	4104300	1,4-Dichlorobenzene-d4	6.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
3		2-Cyclohexen-1-one	96	C6H8O	000930-68-7	11
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		5-Aminoindole	132	C8H8N2	005192-03-0	10

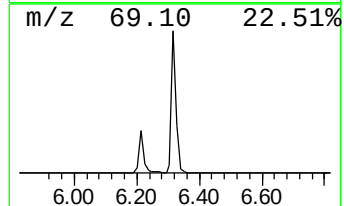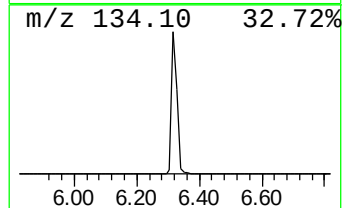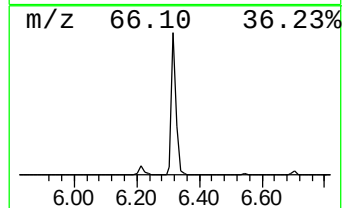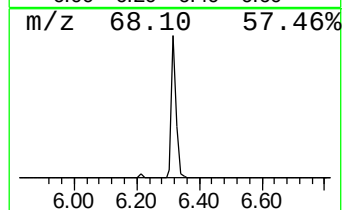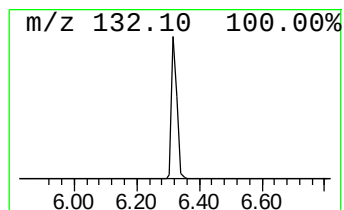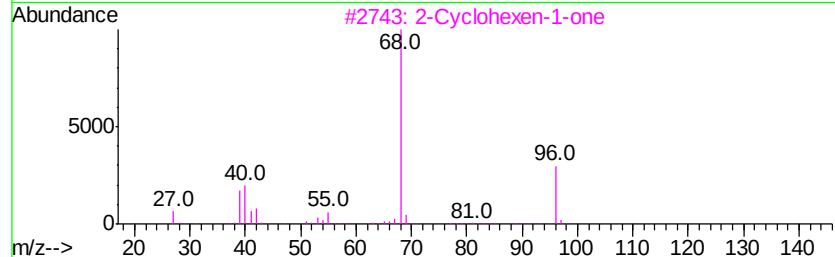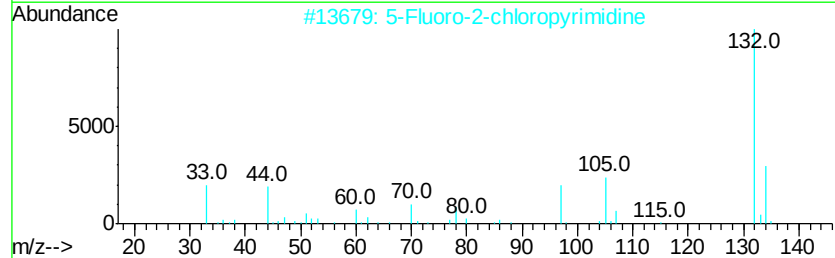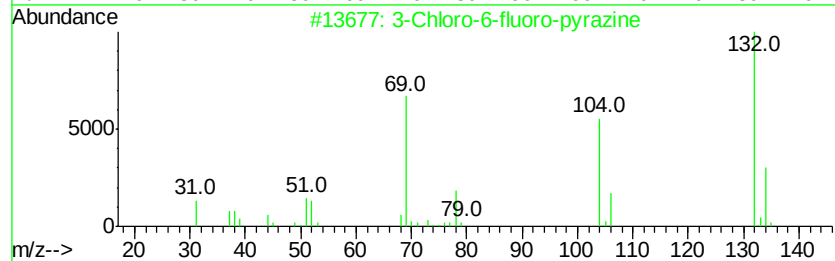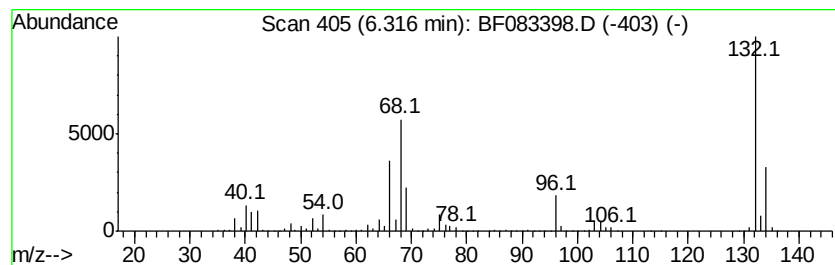

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120115\
Data File : BF083398.D
Acq On : 2 Dec 2015 4:05
Operator : UM/IZ
Sample : G4587-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.65	12.0	ng	635092	1	6.54	1059940	20.0
unknown6.32	6.32	77.4	ng	4104300	1	6.54	1059940	20.0