


Data Path : Z:\HPCHEM1\BNA F\Data\BF120115\
 Data File : BF083376.D
 Acq On : 1 Dec 2015 16:54
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 01:17:16 2015

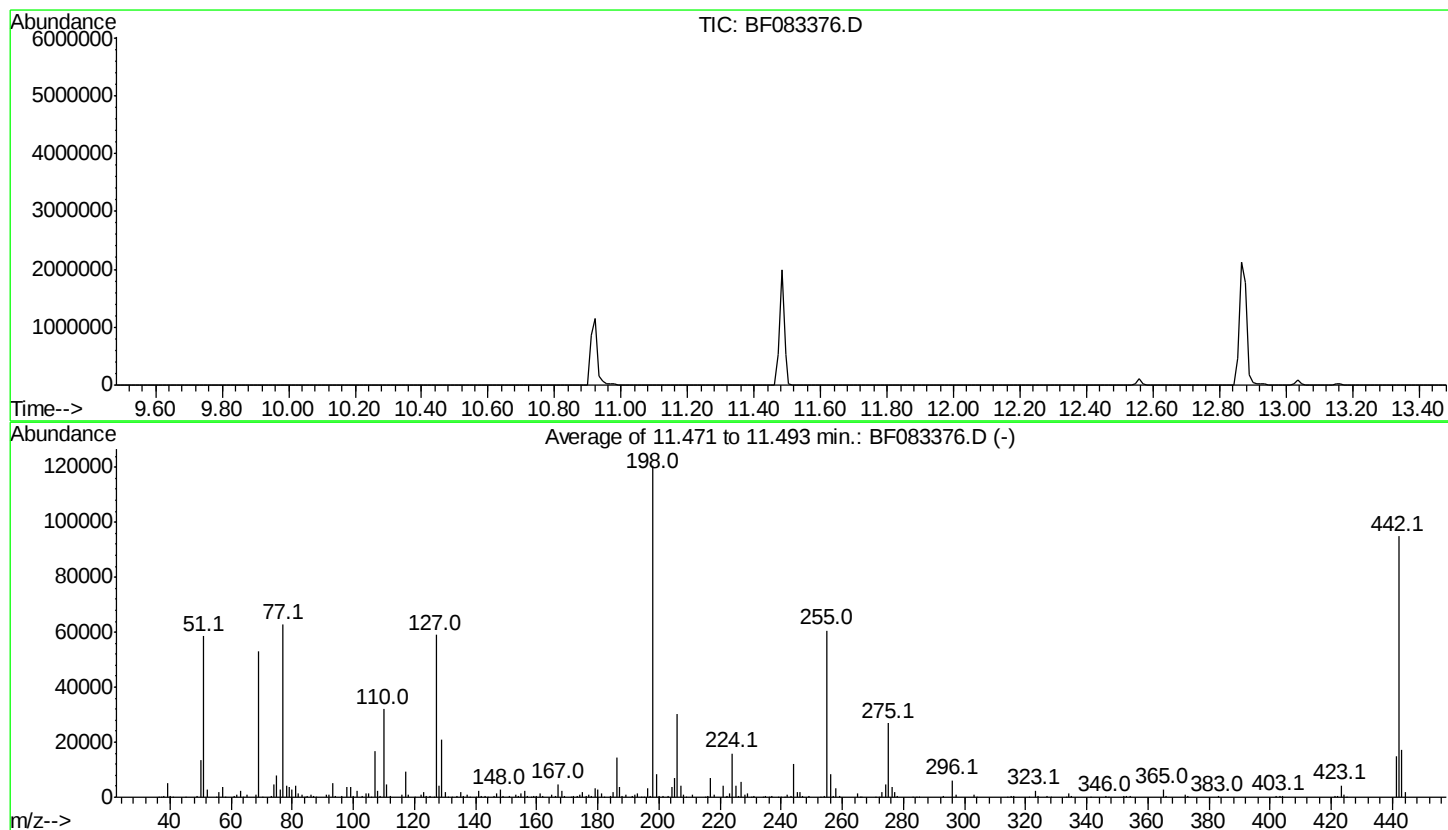

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	58467	PASS
68	69	0.00	2	1.4	725	PASS
69	198	0.00	100	44.2	53293	PASS
70	69	0.00	2	0.4	207	PASS
127	198	10	80	49.0	59013	PASS
197	198	0.00	2	0.6	671	PASS
198	198	100	100	100.0	120549	PASS
199	198	5	9	6.8	8223	PASS
275	198	10	60	22.2	26784	PASS
365	198	1	100	2.5	2966	PASS
441	442	0.01	24	15.9	15082	PASS
442	198	50	100	78.6	94766	PASS
443	442	15	24	18.2	17232	PASS