


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120115\
 Data File : BF083401.D
 Acq On : 2 Dec 2015 5:37
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 01:17:16 2015

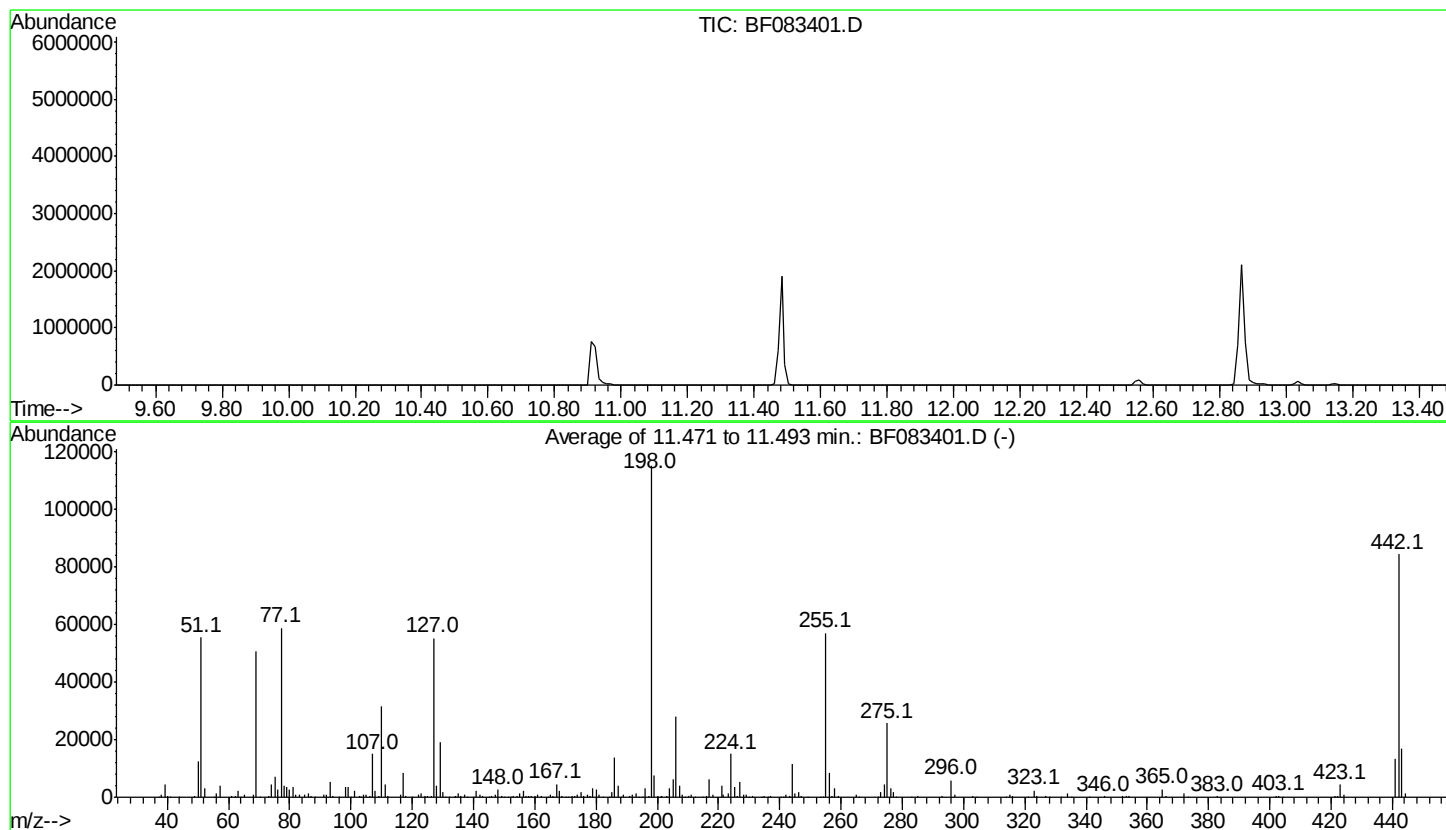

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.1	55474	PASS
68	69	0.00	2	1.6	792	PASS
69	198	0.00	100	44.1	50891	PASS
70	69	0.00	2	0.3	150	PASS
127	198	10	80	47.9	55251	PASS
197	198	0.00	2	0.5	617	PASS
198	198	100	100	100.0	115298	PASS
199	198	5	9	6.6	7627	PASS
275	198	10	60	22.3	25697	PASS
365	198	1	100	2.3	2676	PASS
441	442	0.01	24	15.6	13200	PASS
442	198	50	100	73.2	84409	PASS
443	442	15	24	20.0	16896	PASS