


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120116\
 Data File : BF091370.D
 Acq On : 1 Dec 2016 11:09
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

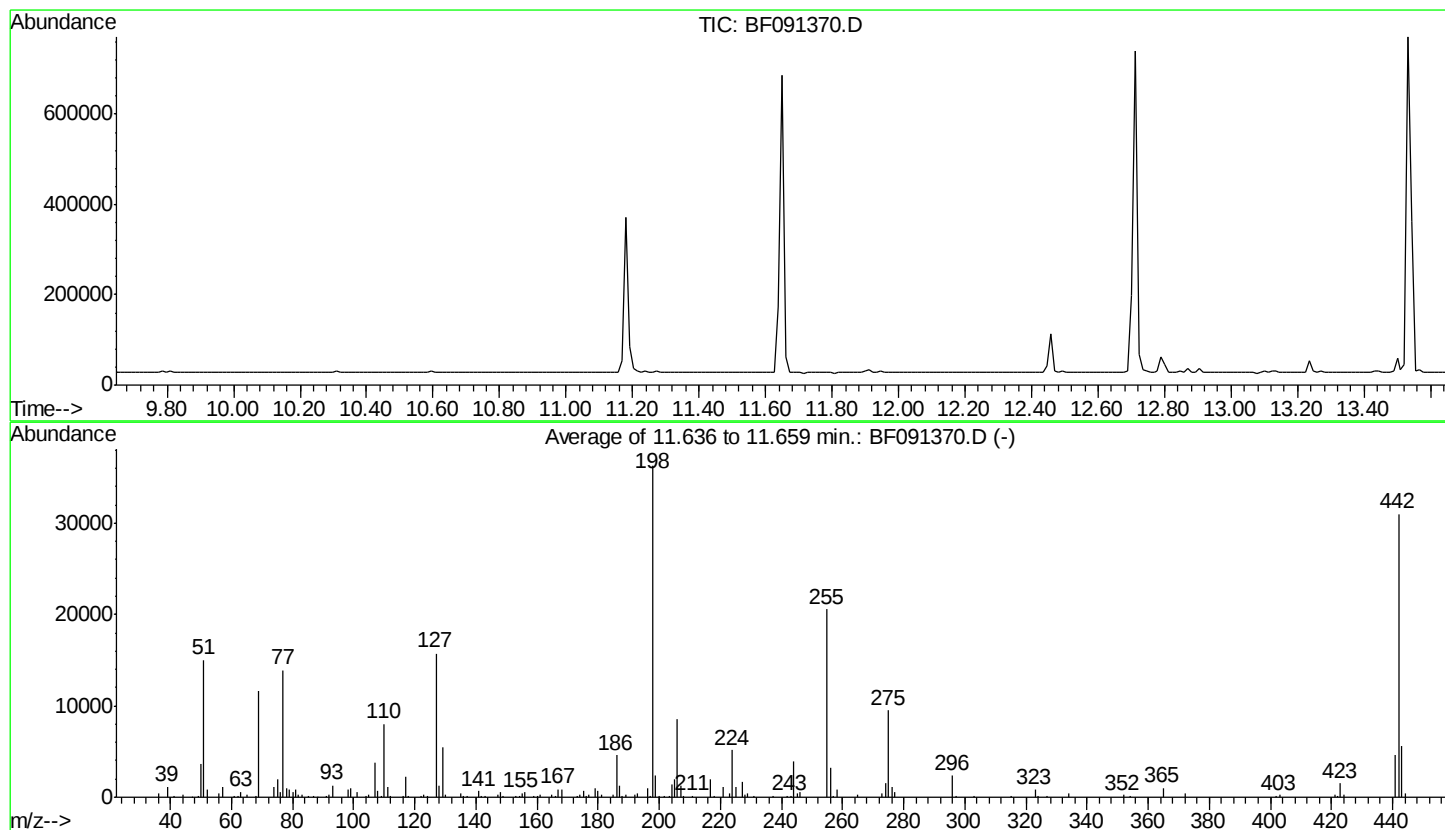

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	15061	PASS
68	69	0.00	2	1.2	145	PASS
69	198	0.00	100	32.1	11641	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	15755	PASS
197	198	0.00	2	0.6	214	PASS
198	198	100	100	100.0	36283	PASS
199	198	5	9	6.7	2432	PASS
275	198	10	60	26.2	9502	PASS
365	198	1	100	2.9	1039	PASS
441	442	0.01	24	14.8	4575	PASS
442	198	50	100	85.4	30995	PASS
443	442	15	24	18.0	5565	PASS