
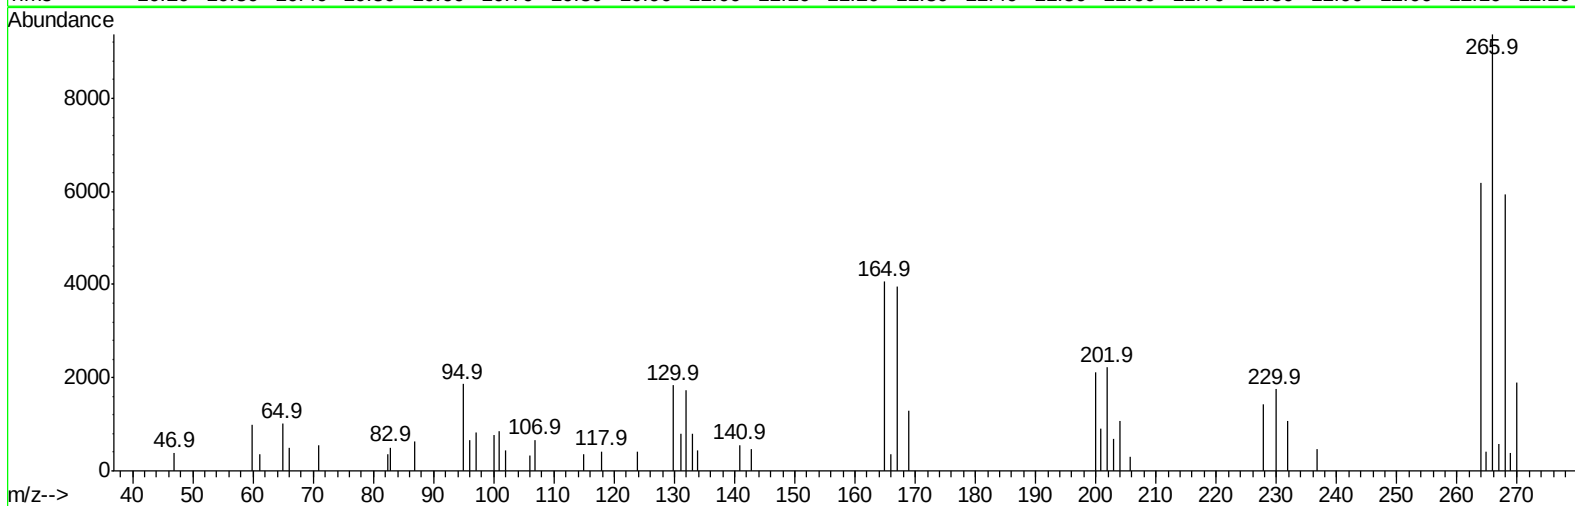


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120117\
Data File : BF101082.D
Acq On : 2 Dec 2017 00:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 04:03:33 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 15:52:19 2017
Response via : Initial Calibration

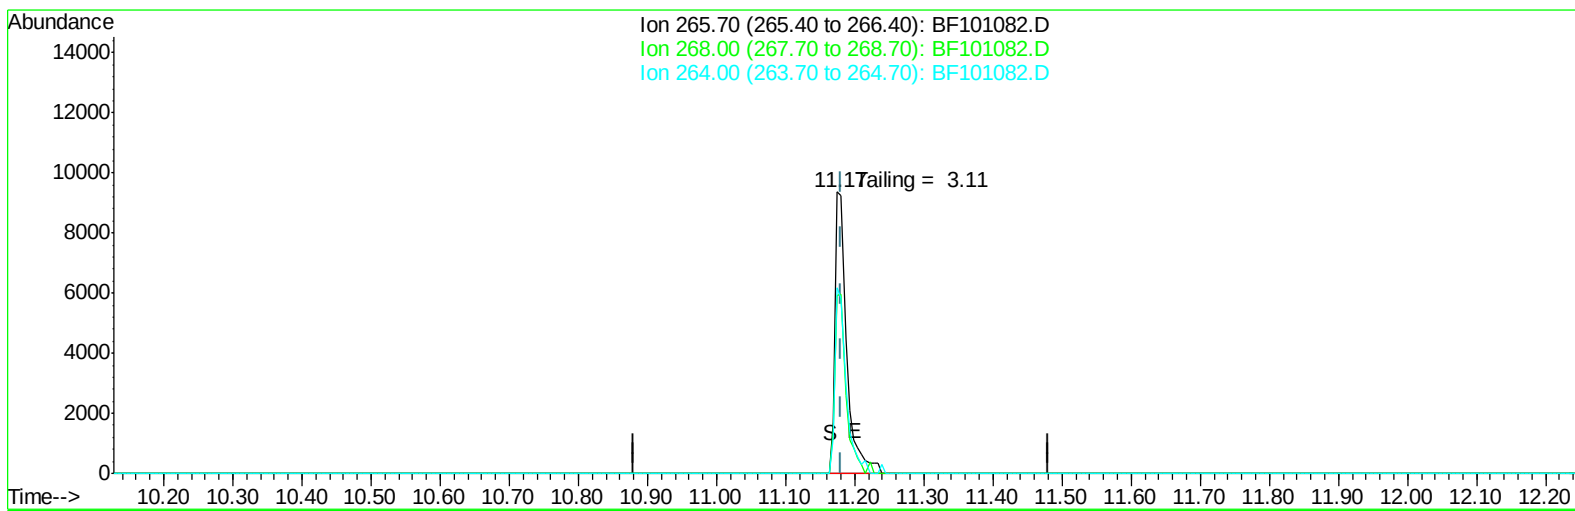

TIC: BF101082.D

(69) Pentachlorophenol (C)



11.175min (-0.006) 0.00ng m

response 10925

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.25
264.00	61.90	65.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120117\
Data File : BF101082.D
Acq On : 2 Dec 2017 00:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 04:03:33 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 15:52:19 2017
Response via : Initial Calibration

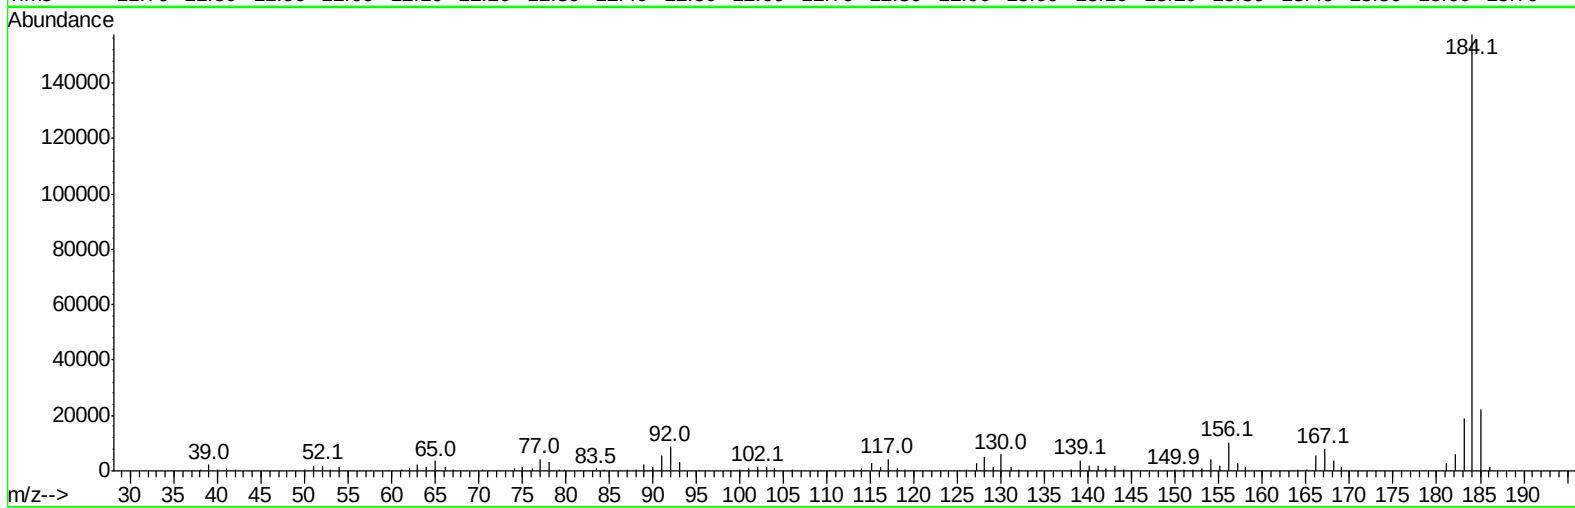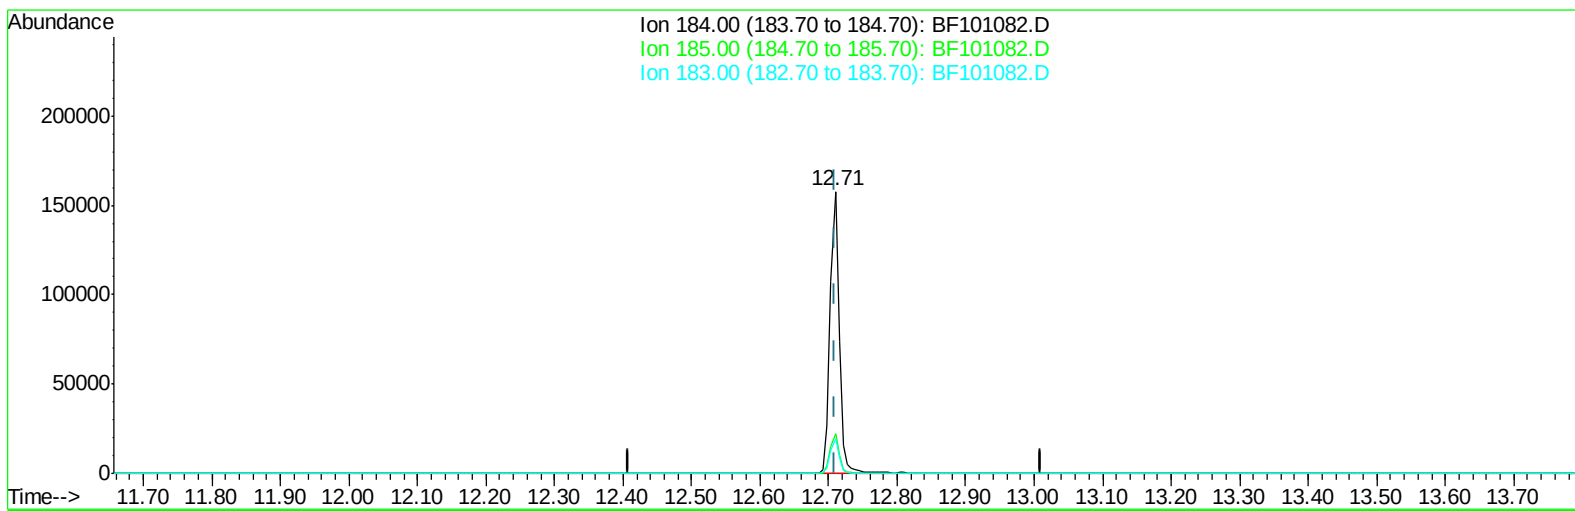

TIC: BF101082.D

(76) Benzidine

12.710min (+0.000) 0.00ng

response 140712

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.18
183.00	11.60	12.09
0.00	0.00	0.00