


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF120117\
 Data File : BF101055.D
 Acq On : 1 Dec 2017 11:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 01 15:52:19 2017

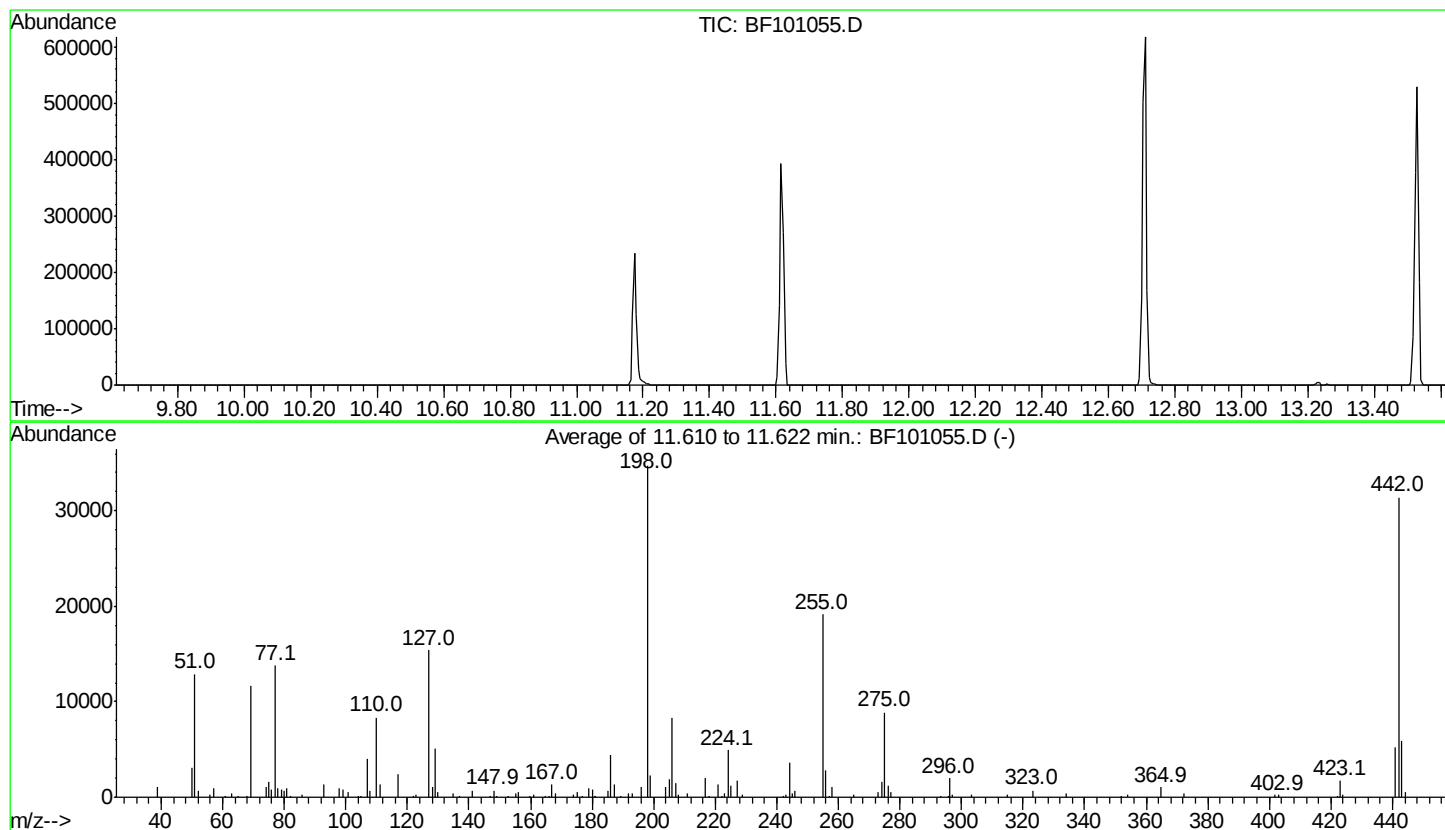

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	12908	PASS
68	69	0.00	2	1.1	123	PASS
69	198	0.00	100	33.7	11704	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	15361	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34730	PASS
199	198	5	9	6.6	2309	PASS
275	198	10	60	25.6	8880	PASS
365	198	1	100	2.9	1015	PASS
441	443	0.01	100	88.8	5281	PASS
442	198	50	100	90.5	31414	PASS
443	442	15	24	18.9	5949	PASS