

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120120\
 Data File : BF122526.D
 Acq On : 1 Dec 2020 17:28
 Operator : JU/CG
 Sample : L4909-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROCK-HILL-SLOPE-EMBANKMENT-

Quant Time: Dec 01 17:53:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 14:38:56 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	193305	20.00	ng	0.00
21) Naphthalene-d8	8.139	136	744270	20.00	ng	0.00
39) Acenaphthene-d10	9.898	164	386514	20.00	ng	0.00
64) Phenanthrene-d10	11.386	188	713298	20.00	ng	0.00
76) Chrysene-d12	14.027	240	563650	20.00	ng	0.00
86) Perylene-d12	15.498	264	483273	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	1454686	115.55	ng	0.00
7) Phenol-d6	6.492	99	1810141	109.91	ng	0.00
23) Nitrobenzene-d5	7.422	82	1147417	94.38	ng	0.00
42) 2,4,6-Tribromophenol	10.686	330	542016	130.66	ng	0.00
45) 2-Fluorobiphenyl	9.222	172	1923214	77.74	ng	0.00
79) Terphenyl-d14	12.974	244	1932049	72.62	ng	0.00
Target Compounds						
10) Phenol	6.498	94	52196	3.22	ng	92
50) Dimethylphthalate	9.610	163	239818	8.73	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120120\
Data File : BF122526.D
Acq On : 1 Dec 2020 17:28
Operator : JU/CG
Sample : L4909-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-

Quant Time: Dec 01 17:53:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration




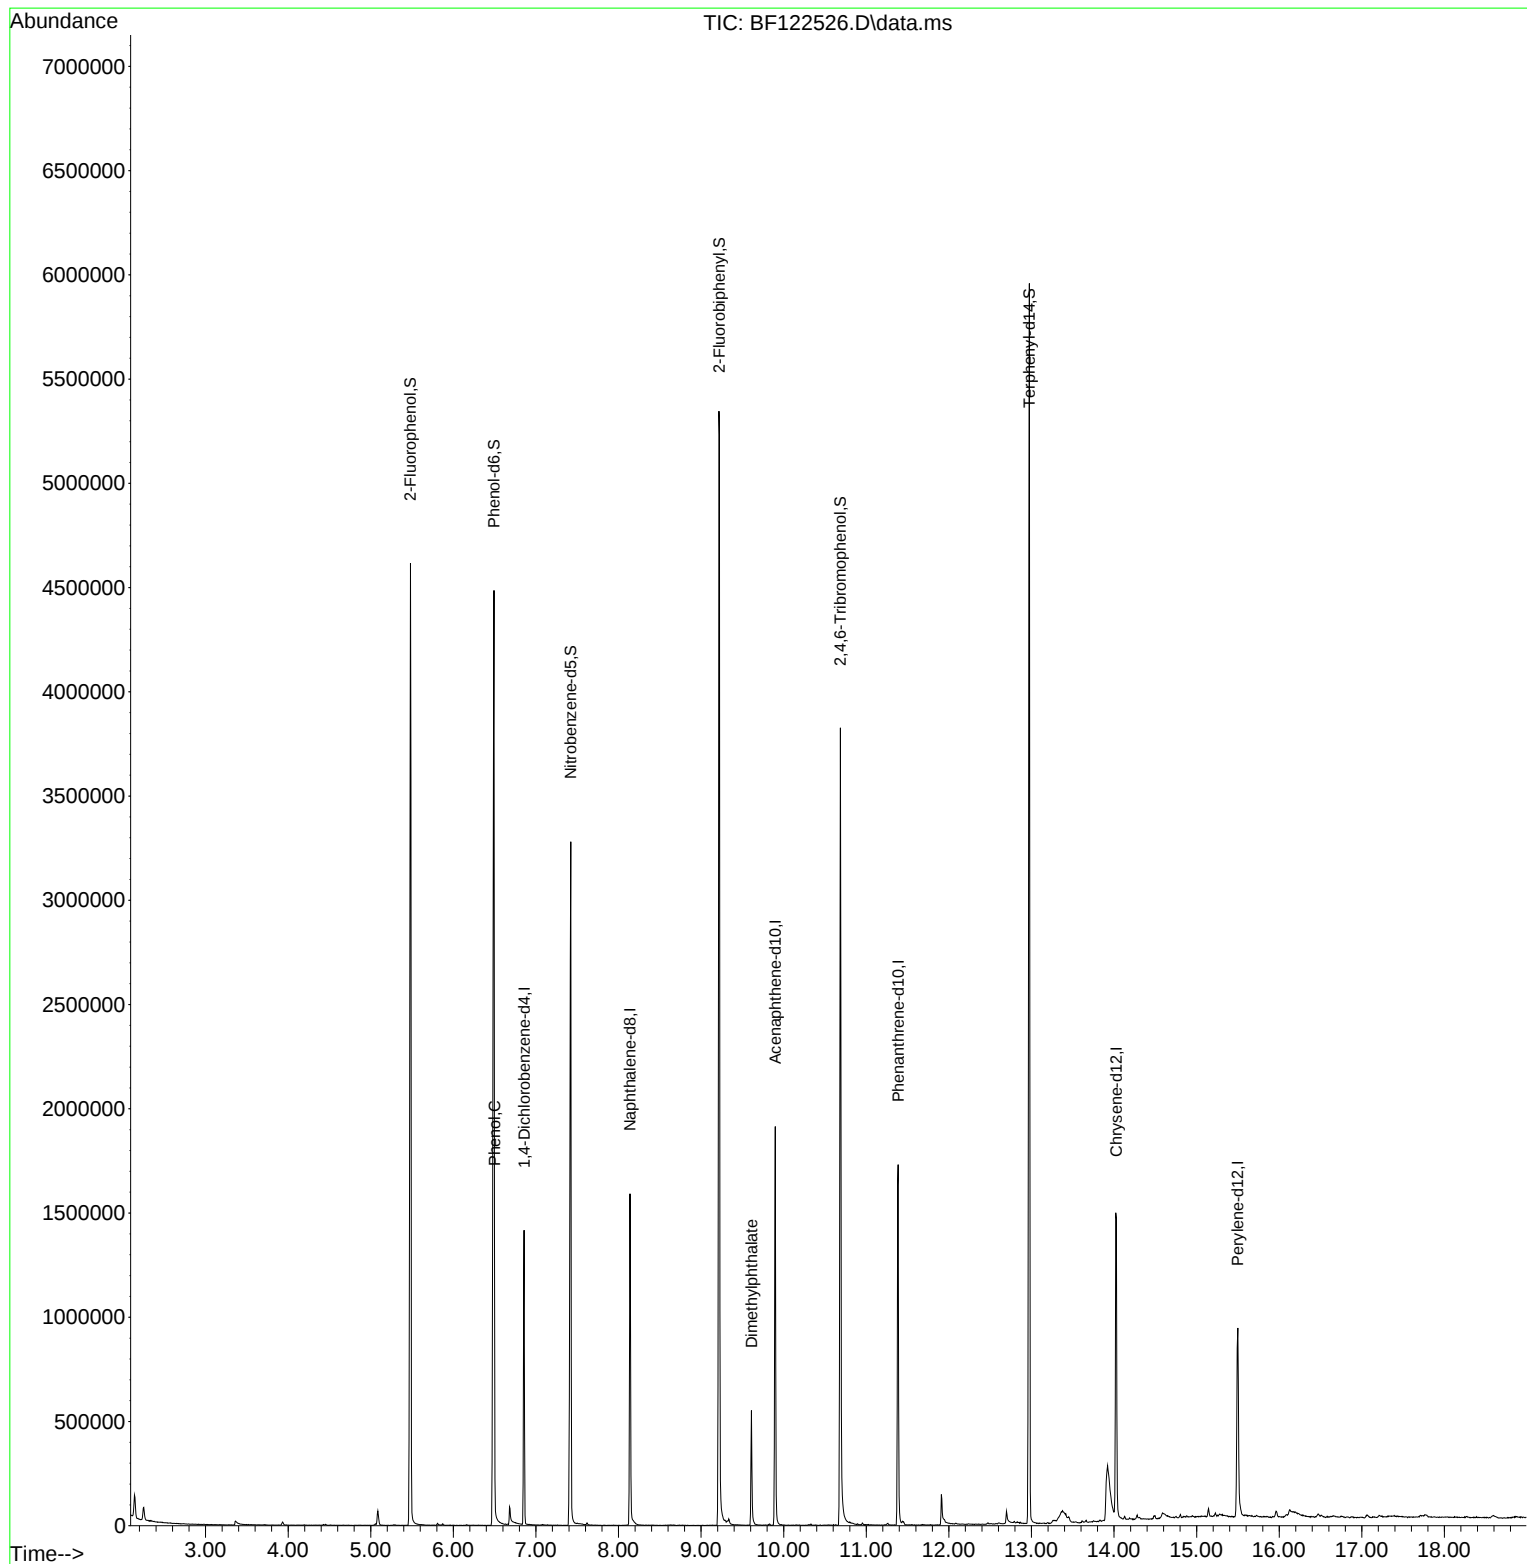




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.857 min Scan# 811
Delta R.T. 0.000 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28




Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-


Tgt Ion:152 Resp: 193305
Ion Ratio Lower Upper
152 100
150 155.6 125.3 187.9
115 59.1 51.9 77.9

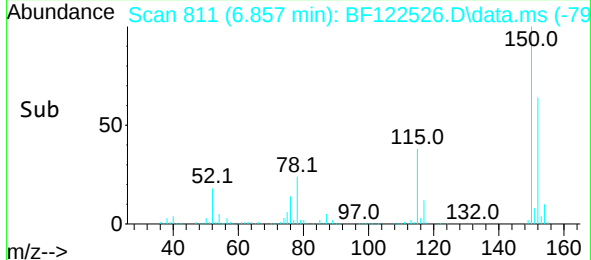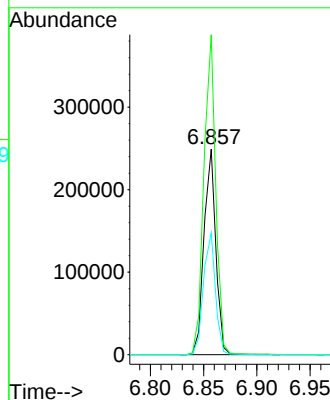

#5
2-Fluorophenol
Concen: 115.55 ng
RT: 5.481 min Scan# 577
Delta R.T. -0.000 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion:112 Resp: 1454686
Ion Ratio Lower Upper
112 100
64 59.0 50.4 75.6
63 30.2 25.8 38.6


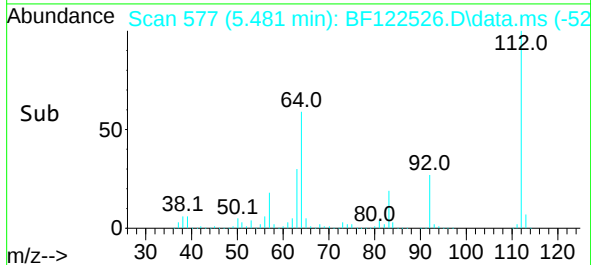
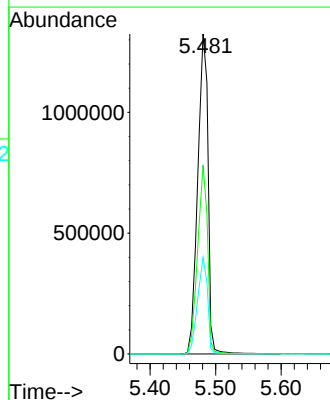
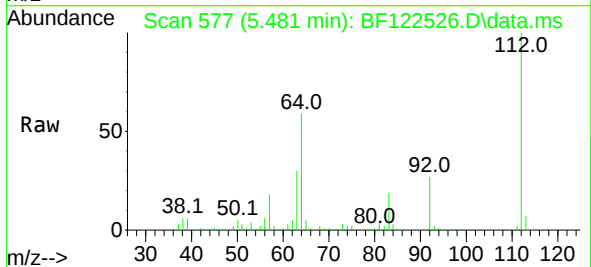


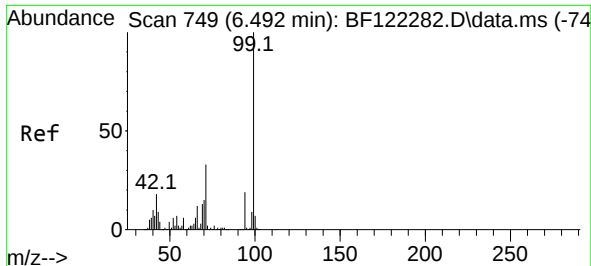

#7
Phenol-d6
Concen: 109.91 ng
RT: 6.492 min Scan# 749
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28




Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-

Tgt Ion: 99 Resp: 1810141
Ion Ratio Lower Upper
99 100
42 18.2 15.9 23.9
71 35.0 27.1 40.7

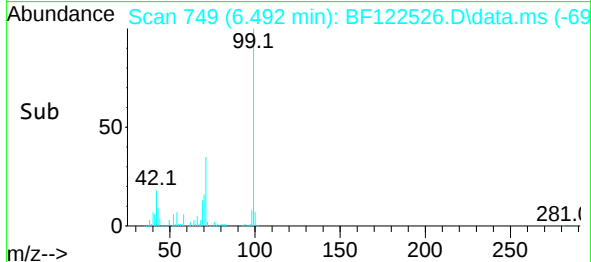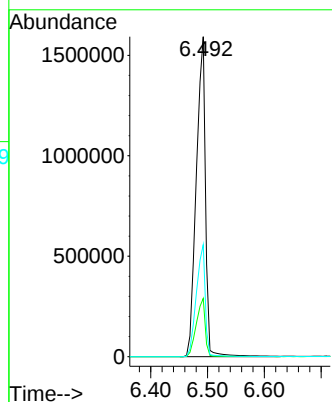

#10
Phenol
Concen: 3.22 ng
RT: 6.498 min Scan# 750
Delta R.T. -0.012 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion: 94 Resp: 52196
Ion Ratio Lower Upper
94 100
65 33.2 17.1 57.1
66 62.0 36.0 76.0

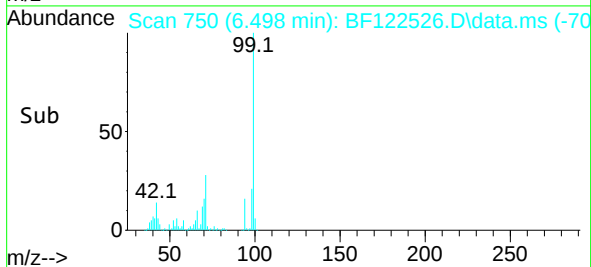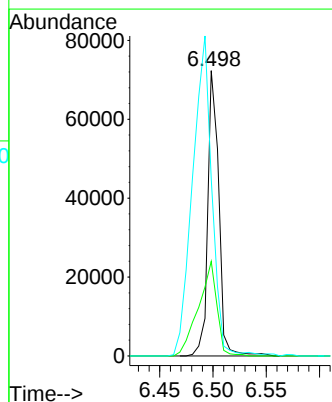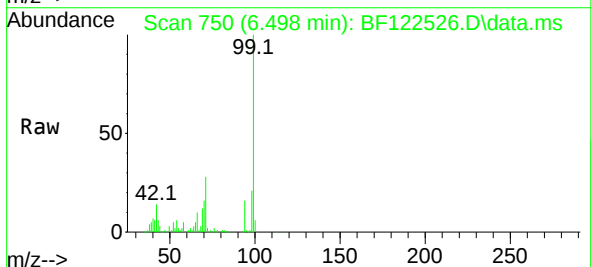







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.139 min Scan# 1029
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-

Tgt Ion:136 Resp: 744270




Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.6	13.0
54	7.8	7.1	10.7
68	6.2	5.0	7.4

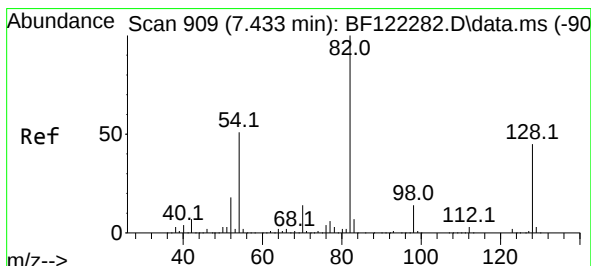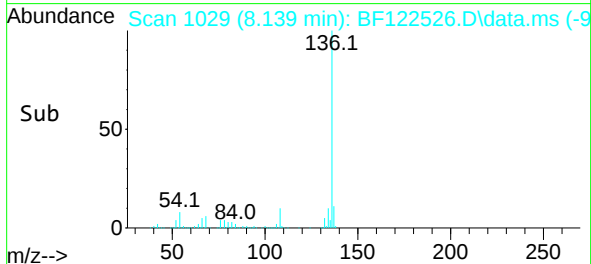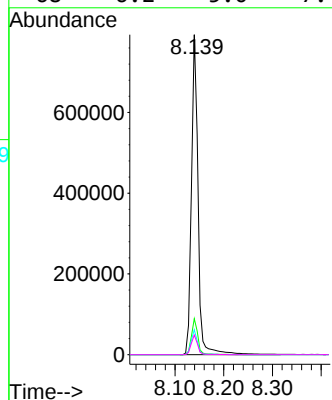


#23
Nitrobenzene-d5
Concen: 94.38 ng
RT: 7.422 min Scan# 907
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion: 82 Resp: 1147417

Ion	Ratio	Lower	Upper
82	100		
128	47.0	35.0	52.4
54	47.7	43.9	65.9


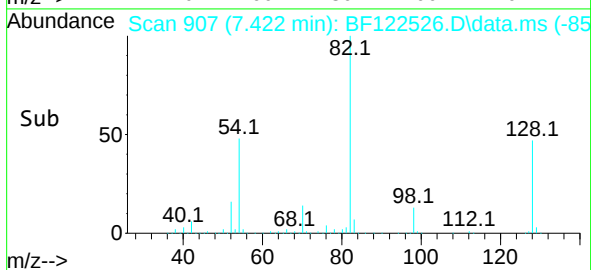
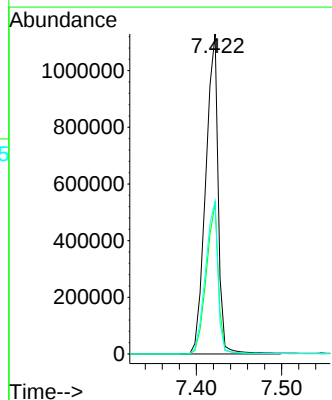
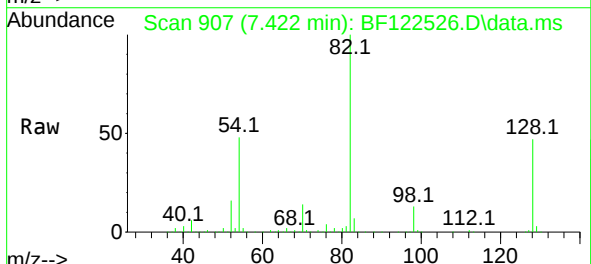




#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.898 min Scan# 1328
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28




Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-


Tgt Ion:164 Resp: 386514
Ion Ratio Lower Upper
164 100
162 104.4 83.2 124.8
160 45.7 37.5 56.3

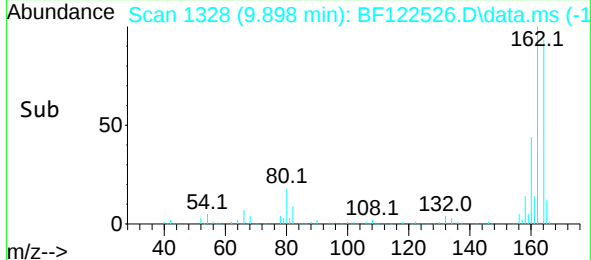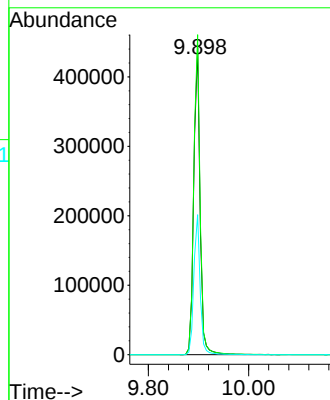

#42
2,4,6-Tribromophenol
Concen: 130.66 ng
RT: 10.686 min Scan# 1462
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion:330 Resp: 542016
Ion Ratio Lower Upper
330 100
332 96.4 77.3 115.9
141 29.0 22.3 33.5


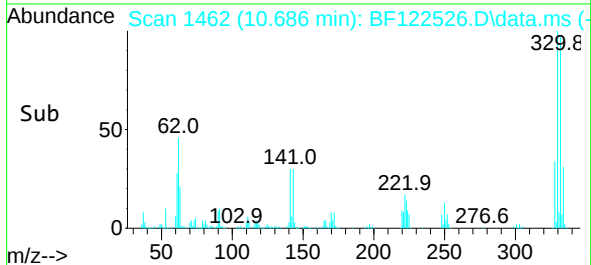
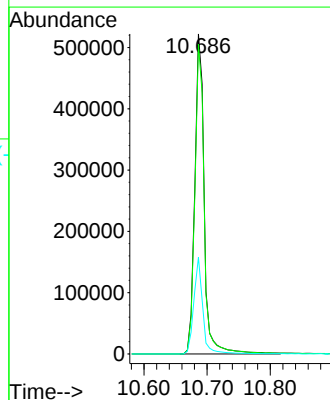
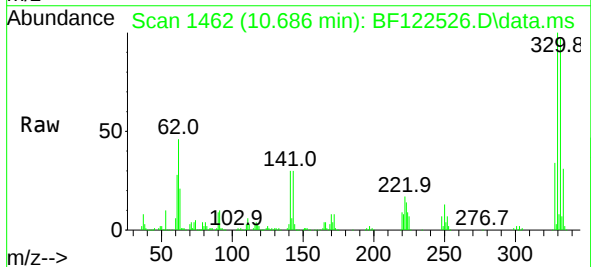




#45
2-Fluorobiphenyl
Concen: 77.74 ng
RT: 9.222 min Scan# 1213
Delta R.T. -0.000 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28




Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-


Tgt Ion:172 Resp: 1923214
Ion Ratio Lower Upper
172 100
171 36.6 29.1 43.7
170 24.6 19.8 29.6

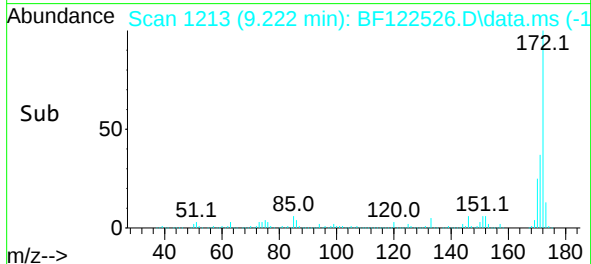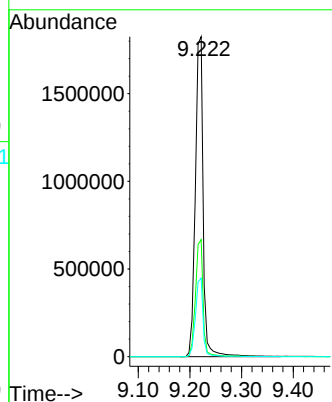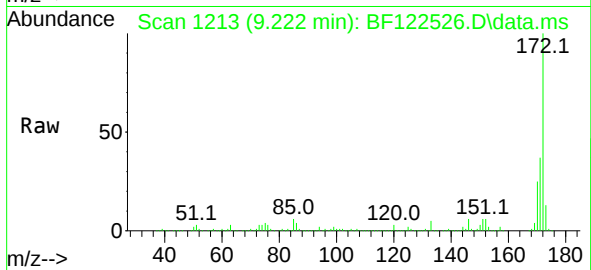

#50
Dimethylphthalate
Concen: 8.73 ng
RT: 9.610 min Scan# 1279
Delta R.T. -0.018 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion:163 Resp: 239818
Ion Ratio Lower Upper
163 100
194 4.0 3.3 4.9
164 9.9 8.2 12.4


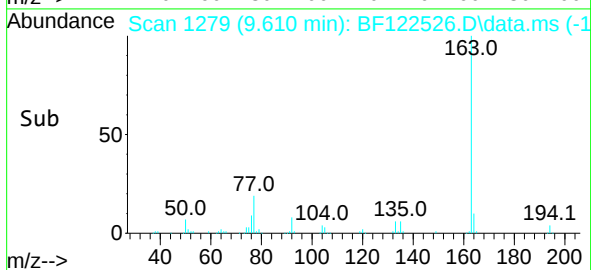
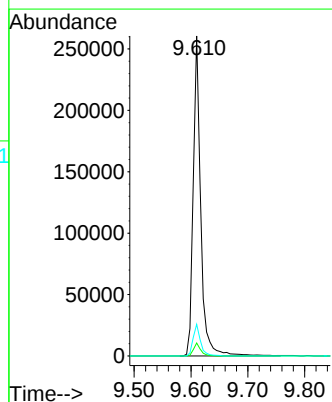
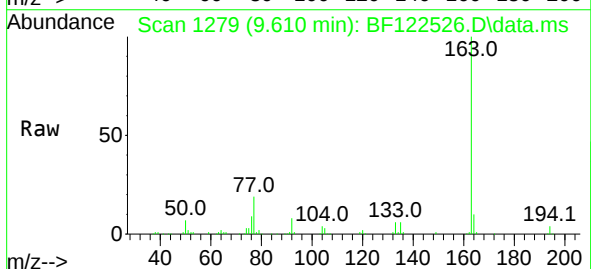


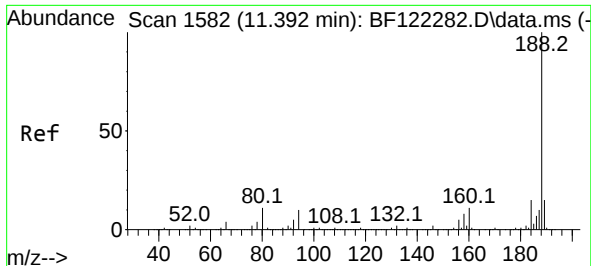

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.386 min Scan# 1581
Delta R.T. -0.000 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28




Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-


Tgt Ion:188 Resp: 713298
Ion Ratio Lower Upper
188 100
94 8.7 8.3 12.5
80 9.3 9.1 13.7

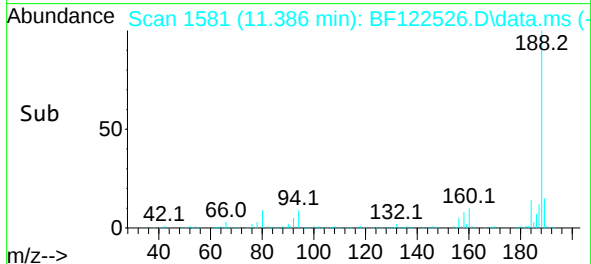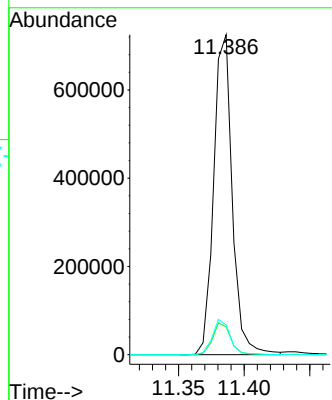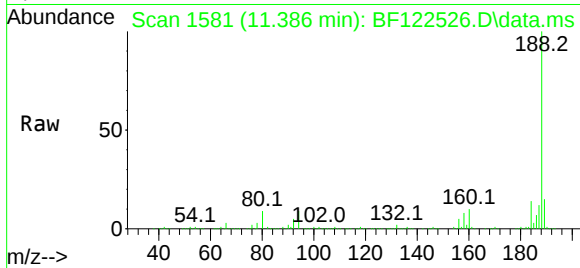

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion:240 Resp: 563650
Ion Ratio Lower Upper
240 100
120 9.7 9.2 13.8
236 25.4 20.9 31.3


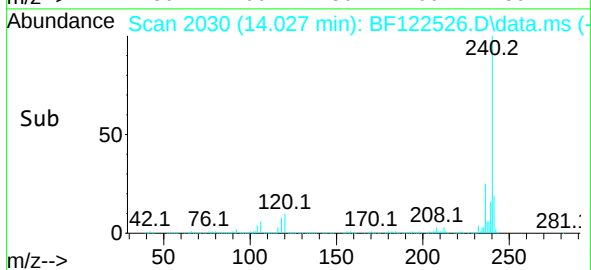
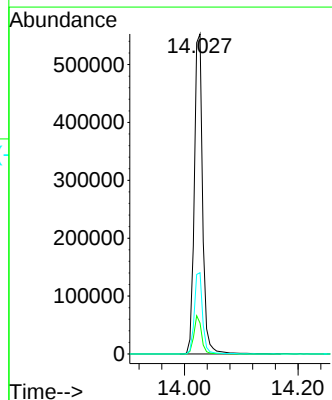
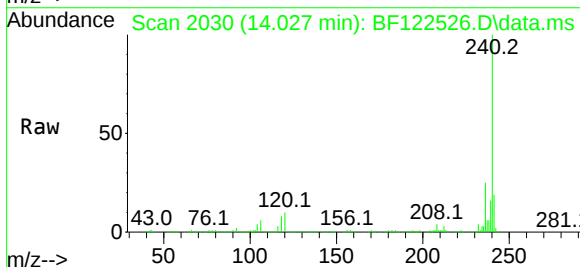


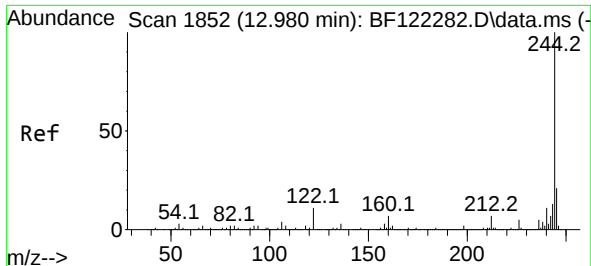

#79
Terphenyl-d14
Concen: 72.62 ng
RT: 12.974 min Scan# 1851
Delta R.T. -0.000 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Instrument :
BNA_F
ClientSampleId :
ROCK-HILL-SLOPE-EMBANKMENT-

Tgt Ion:244 Resp: 1932049
Ion Ratio Lower Upper
244 100
212 7.2 5.4 8.2
122 10.5 8.1 12.1

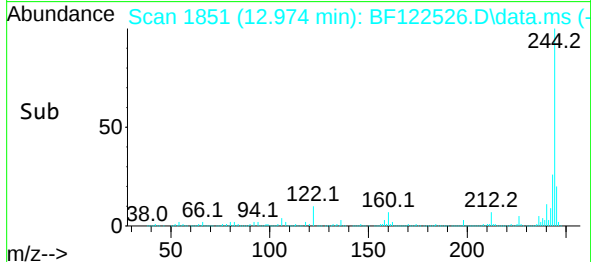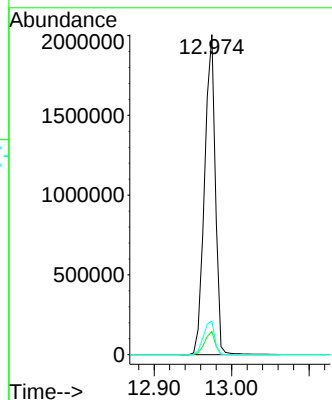

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.498 min Scan# 2280
Delta R.T. -0.006 min
Lab File: BF122526.D
Acq: 1 Dec 2020 17:28

Tgt Ion:264 Resp: 483273
Ion Ratio Lower Upper
264 100
260 23.2 18.7 28.1
265 21.3 17.3 25.9

