
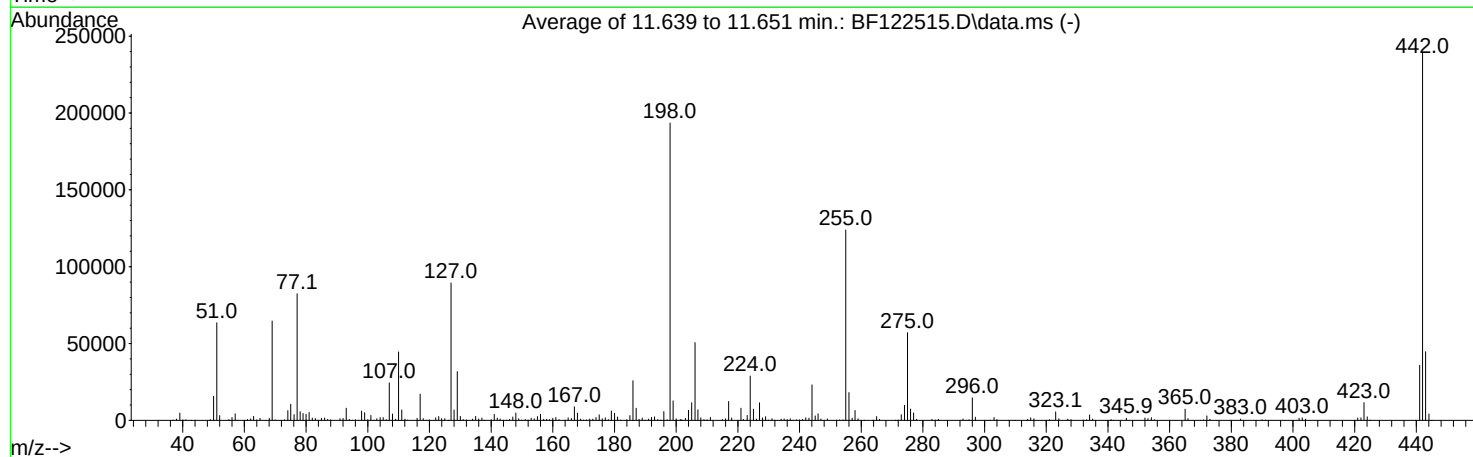


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120120\
 Data File : BF122515.D
 Acq On : 1 Dec 2020 10:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 24 14:38:56 2020

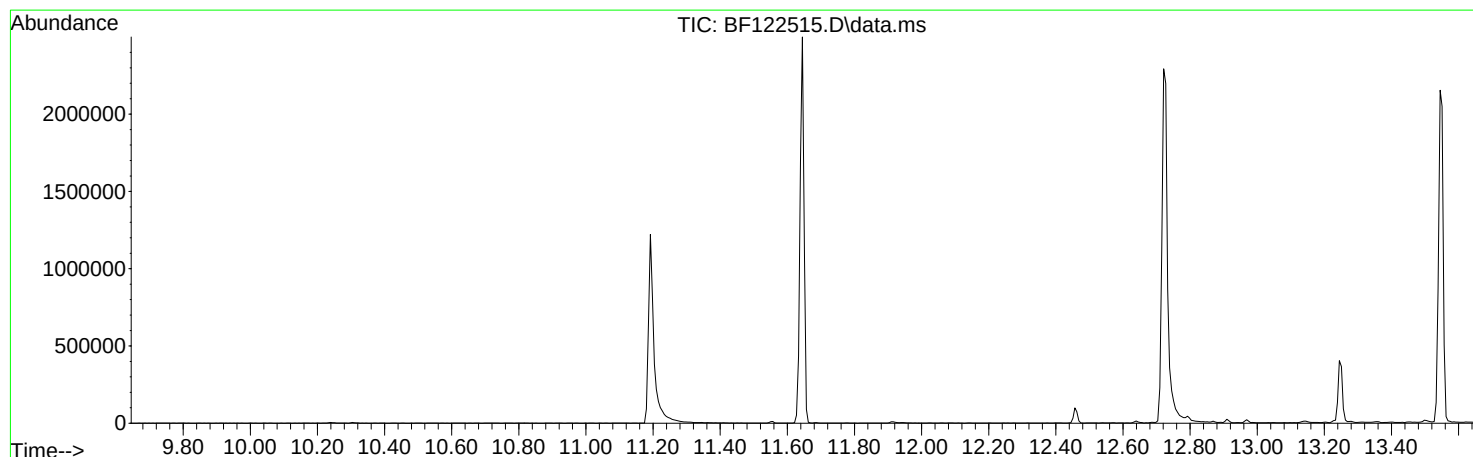

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	63552	PASS
68	69	0.00	2	1.9	1232	PASS
69	198	0.00	100	33.4	64685	PASS
70	69	0.00	2	0.5	352	PASS
127	198	10	80	46.2	89456	PASS
197	198	0.00	2	0.2	441	PASS
198	198	100	100	100.0	193472	PASS
199	198	5	9	6.6	12682	PASS
275	198	10	60	29.5	57088	PASS
365	198	1	100	3.8	7301	PASS
441	198	0.01	100	18.5	35869	PASS
442	442	100	100	100.0	239360	PASS
443	442	15	24	18.7	44709	PASS