
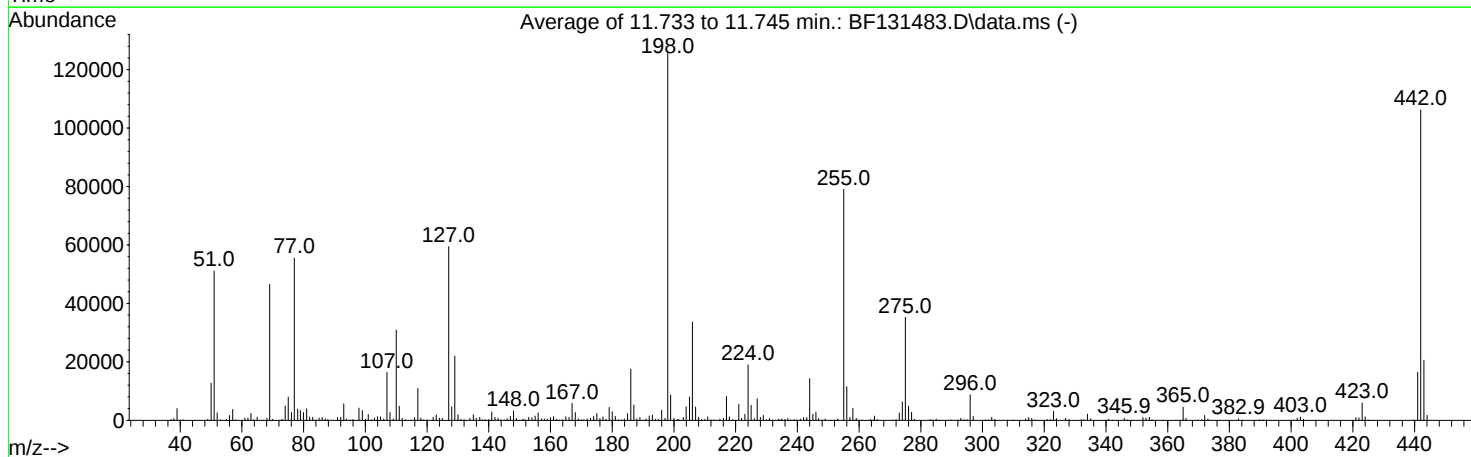


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120122\
Data File : BF131483.D
Acq On : 01 Dec 2022 09:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 01 12:46:17 2022

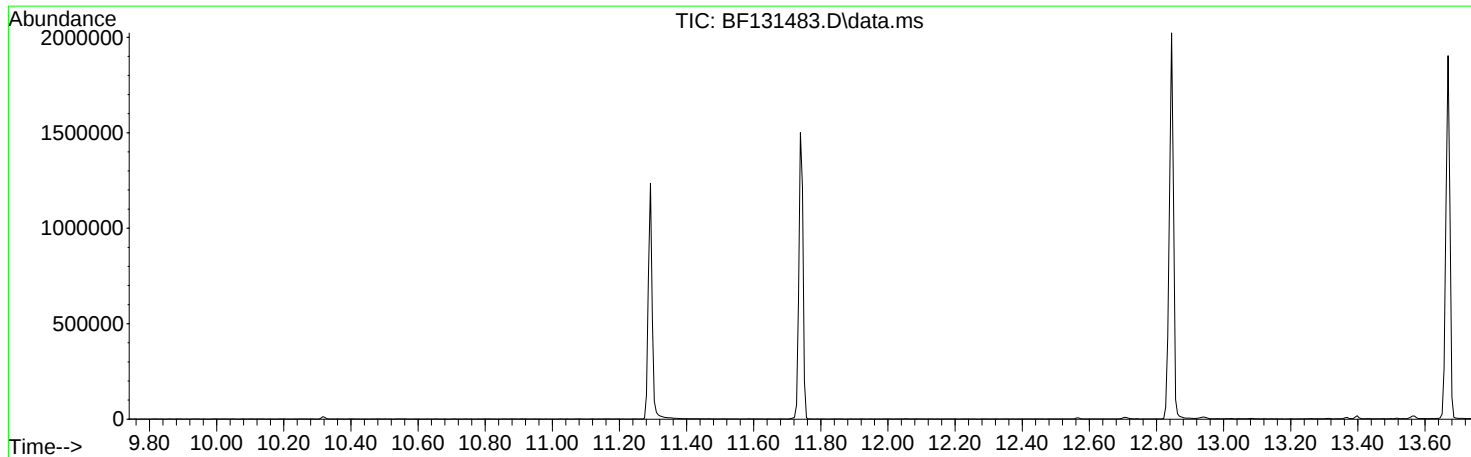




AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	51120	PASS
68	69	0.00	2	1.4	672	PASS
69	198	0.00	100	36.9	46509	PASS
70	69	0.00	2	0.7	344	PASS
127	198	10	80	47.2	59432	PASS
197	198	0.00	2	0.6	695	PASS
198	198	100	100	100.0	125901	PASS
199	198	5	9	6.9	8687	PASS
275	198	10	60	28.0	35226	PASS
365	198	1	100	3.6	4501	PASS
441	198	0.01	100	13.0	16388	PASS
442	442	50	100	100.0	106251	PASS
443	442	15	24	19.3	20489	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120122\
Data File : BF131483.D
Acq On : 01 Dec 2022 09:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 05:40:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 12:46:17 2022
Response via : Initial Calibration

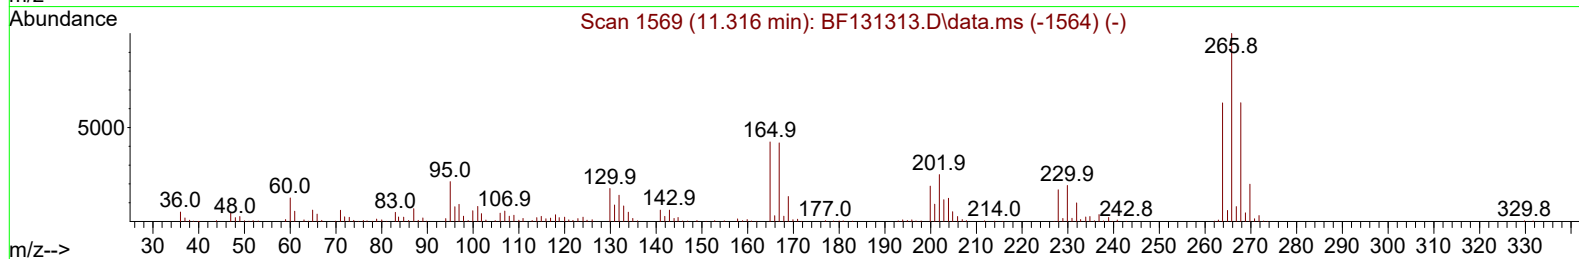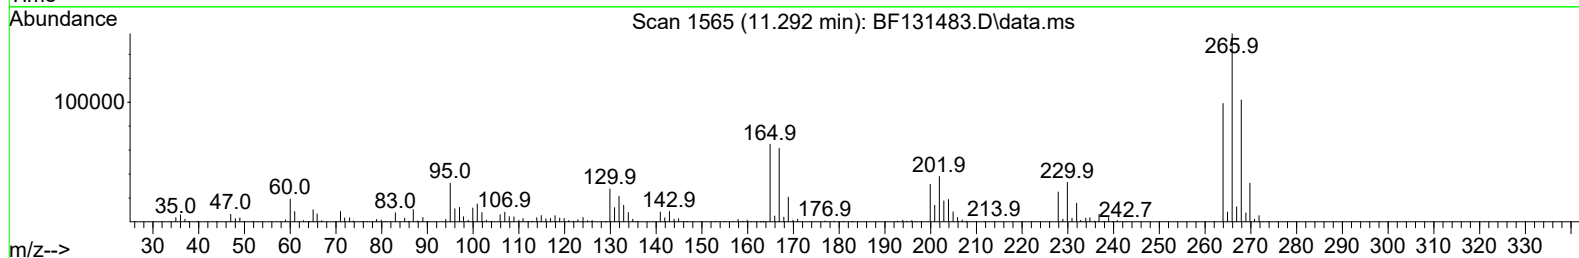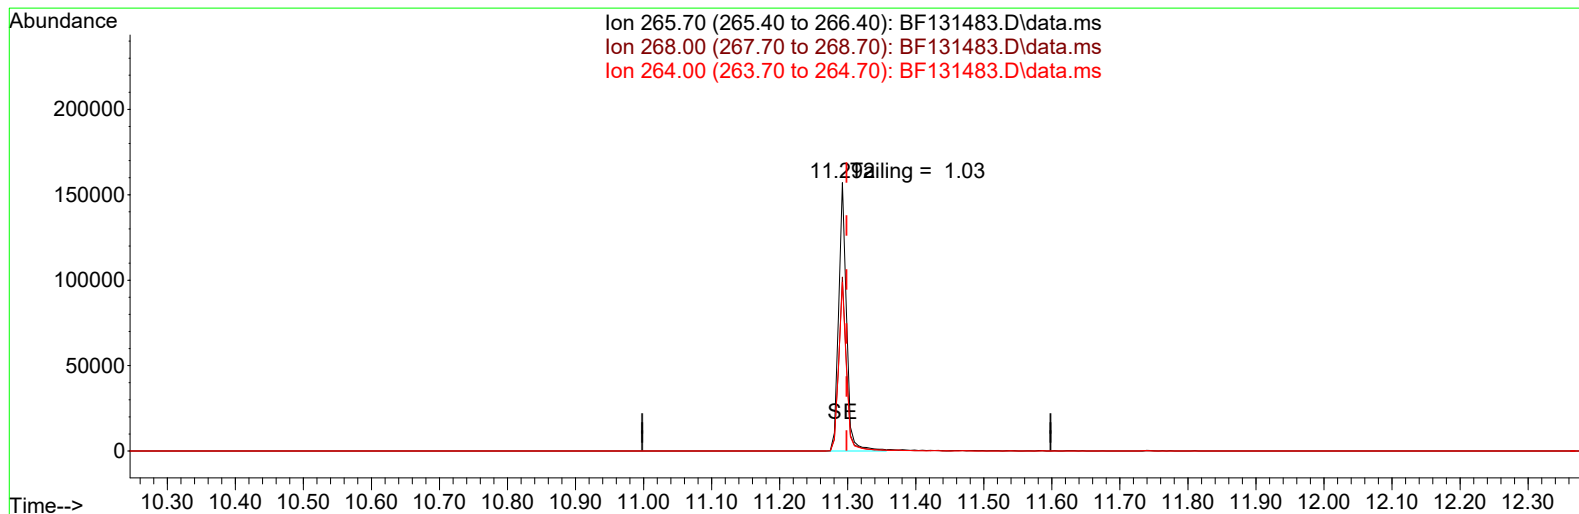

TIC: BF131483.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.006) 29260.26 ng




response 127870

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.79
264.00	63.00	62.90
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120122\  
Data File : BF131483.D  
Acq On    : 01 Dec 2022  09:27  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 05:40:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 12:46:17 2022
Response via : Initial Calibration

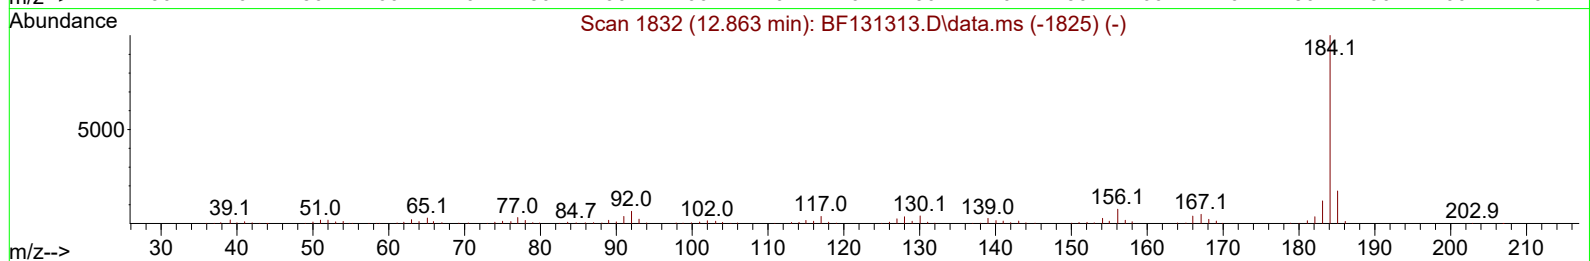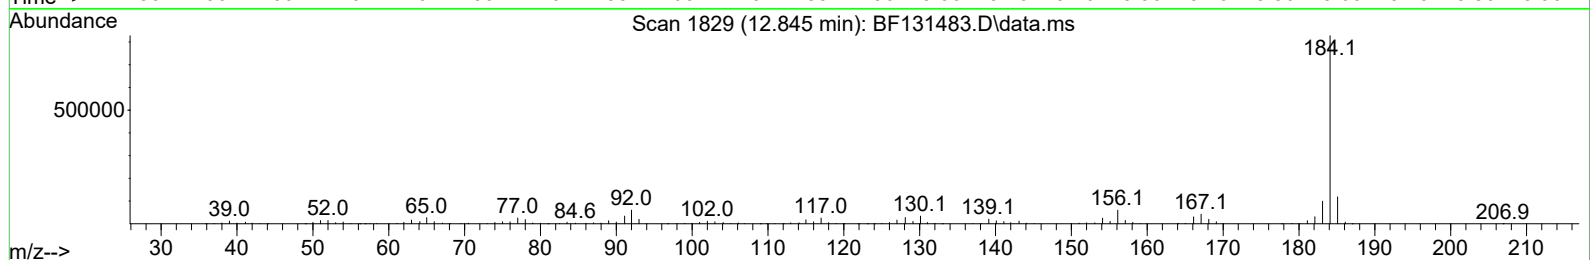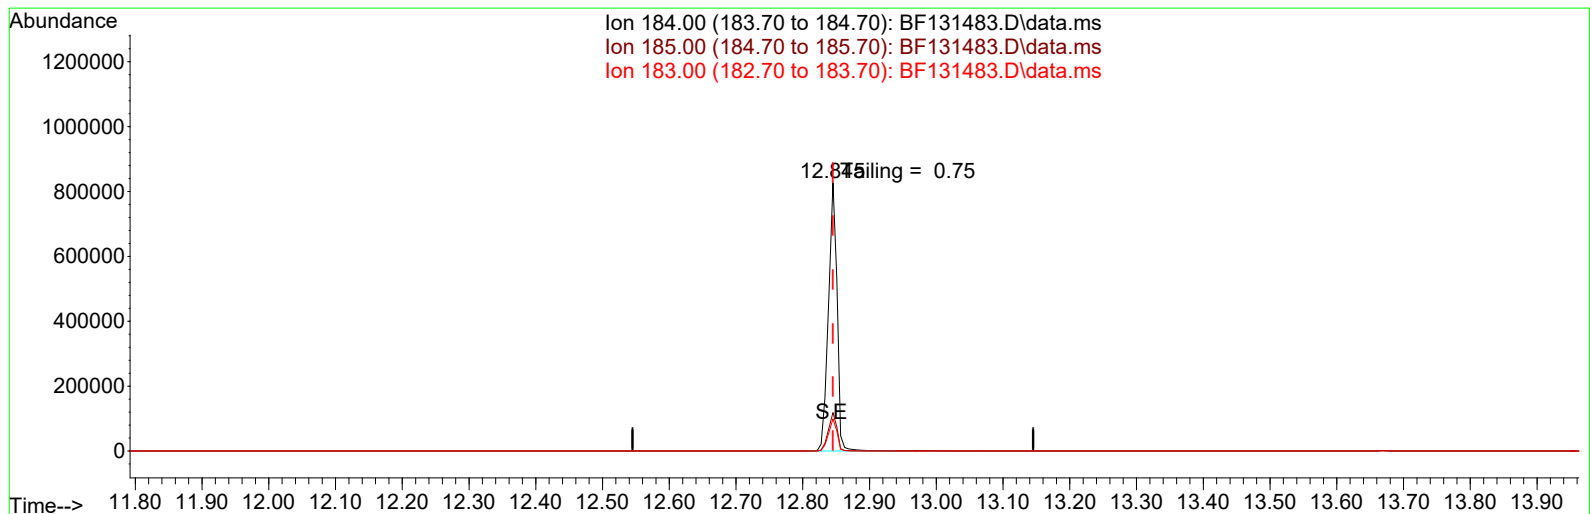

TIC: BF131483.D\data.ms

(77) Benzidine

12.845min (0.000) 0.00 ng

response 748648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.31
183.00	12.00	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2022	BNA_F	<u>BF131483.D</u>
Compound Name	Response	Retention Time
DDT	330789	13.669
DDD	4867	13.398
DDE	254	13.027
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5121	335910	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP