
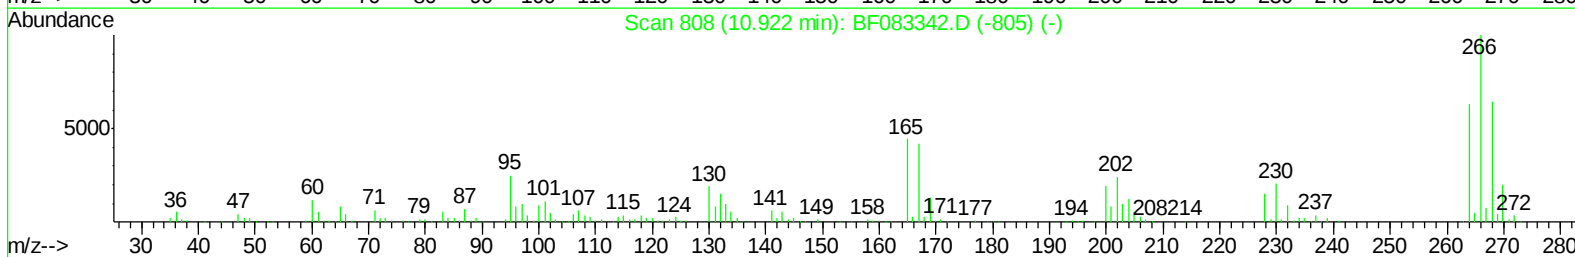
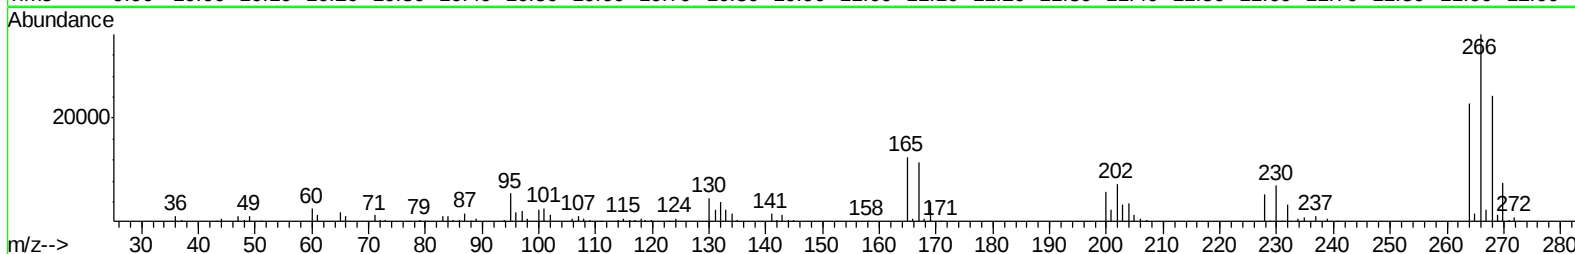


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120215\
Data File : BF083436.D
Acq On : 3 Dec 2015 1:07
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 08:02:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

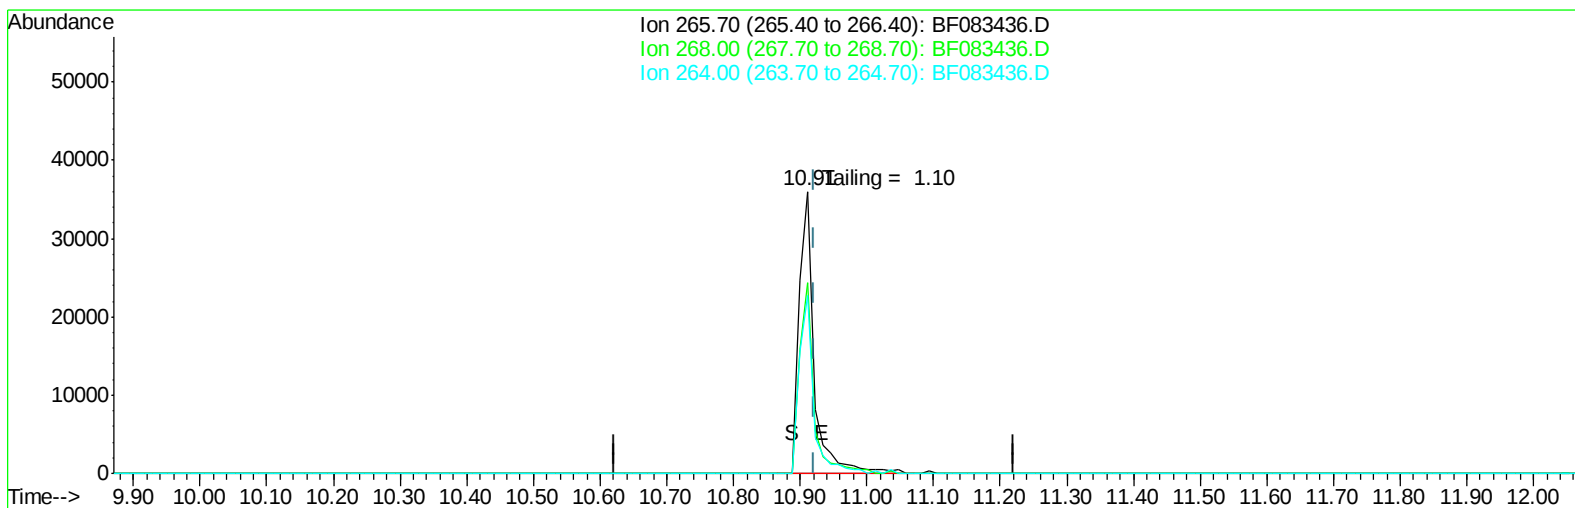

TIC: BF083436.D

(69) Pentachlorophenol (C)




10.911min (-0.011) 0.00ng

response 56054

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	67.59
264.00	63.00	63.03
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120215\
Data File : BF083436.D
Acq On : 3 Dec 2015 1:07
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 08:02:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

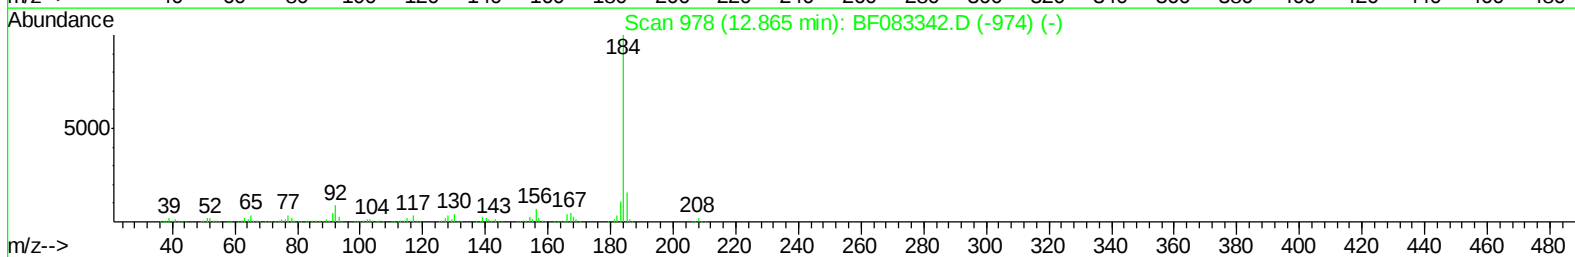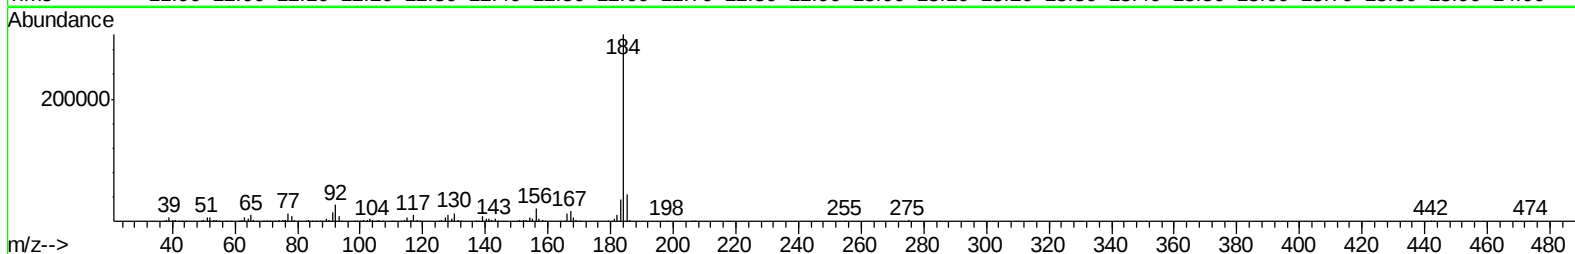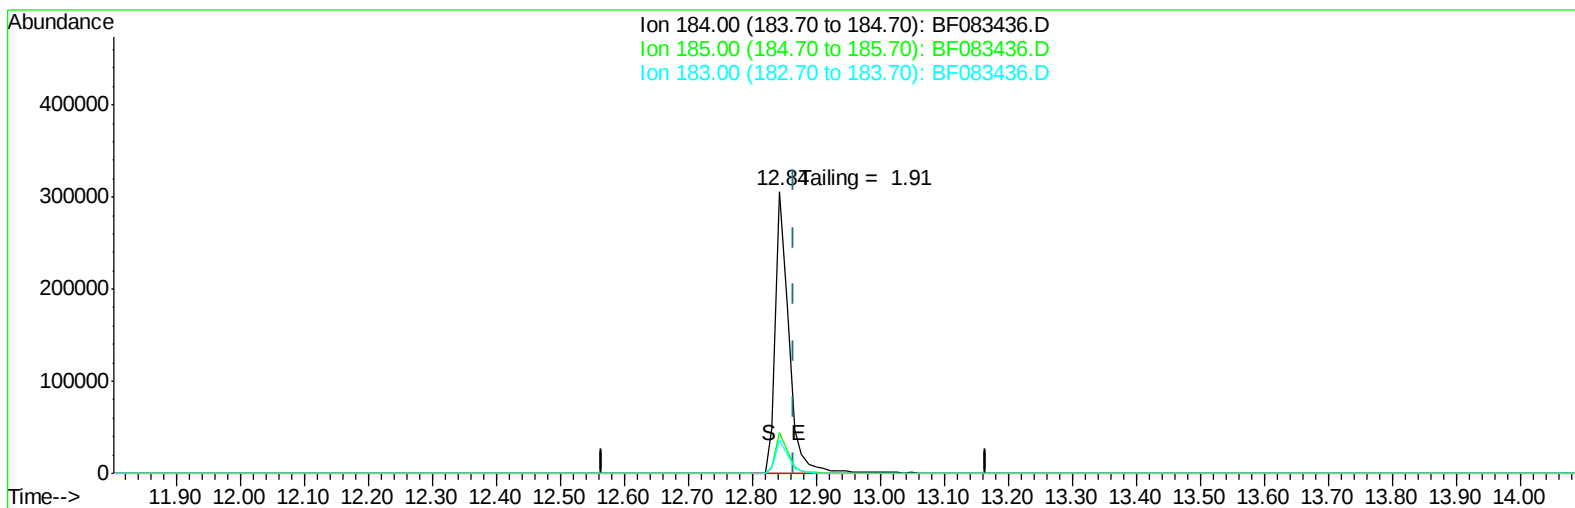

TIC: BF083436.D

(76) Benzidine

12.842min (-0.023) 66379.47ng

response 446828

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.20	11.68
0.00	0.00	0.00