


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120215\
 Data File : BF083436.D
 Acq On : 3 Dec 2015 1:07
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 01:17:16 2015

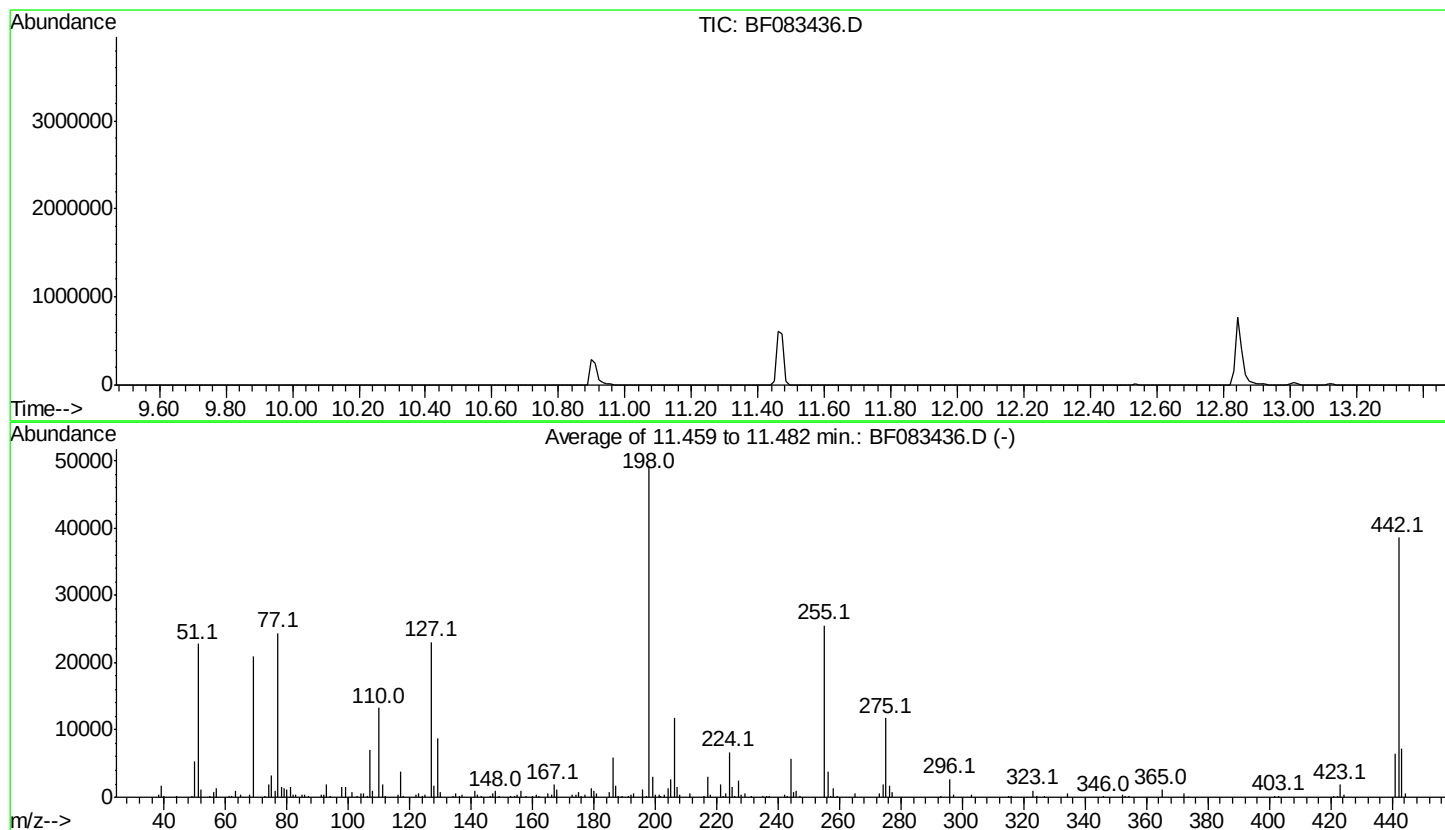

AutoFind: Scans 855, 856, 857; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	22757	PASS
68	69	0.00	2	1.8	372	PASS
69	198	0.00	100	42.4	20892	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	23093	PASS
197	198	0.00	2	0.5	259	PASS
198	198	100	100	100.0	49253	PASS
199	198	5	9	6.1	2986	PASS
275	198	10	60	23.8	11723	PASS
365	198	1	100	2.2	1102	PASS
441	442	0.01	24	16.6	6404	PASS
442	198	50	100	78.2	38515	PASS
443	442	15	24	18.8	7242	PASS