
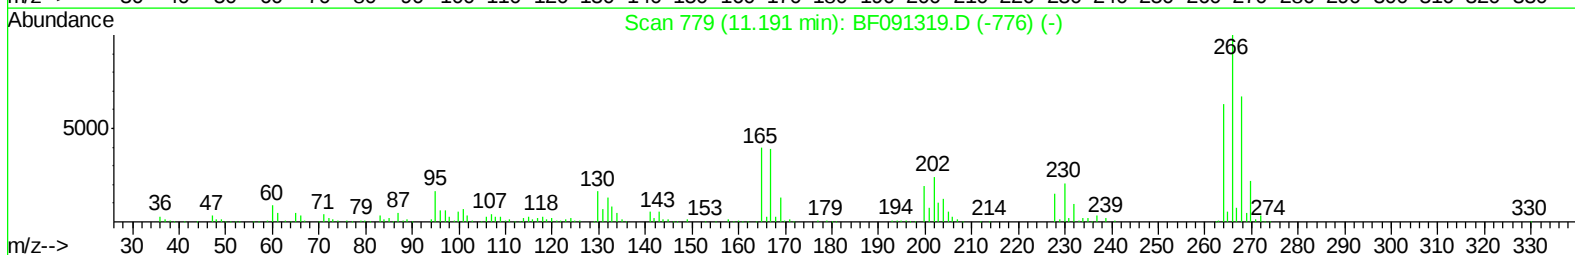
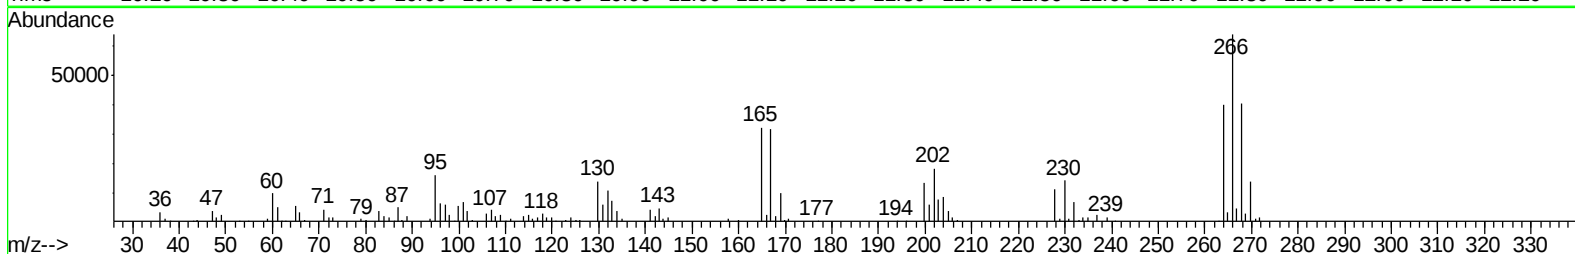


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120216\
Data File : BF091389.D
Acq On : 2 Dec 2016 15:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 05:57:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

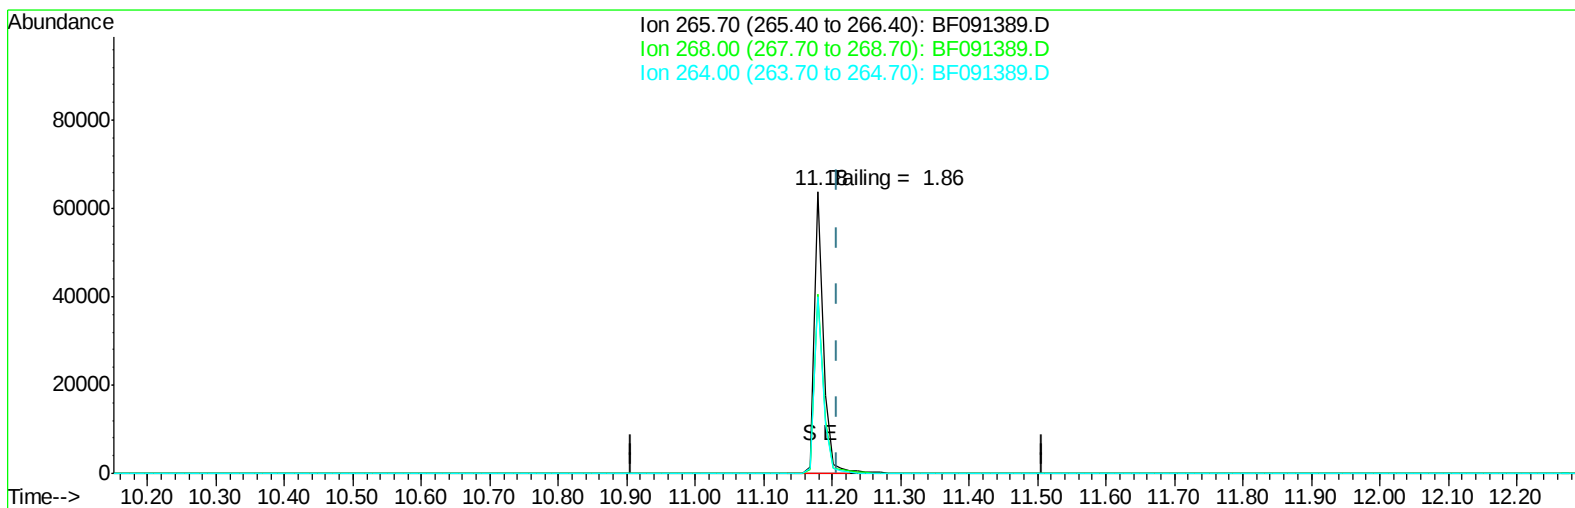

TIC: BF091389.D

(69) Pentachlorophenol (C)




11.179min (-0.028) 0.00ng

response 60530

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	63.55
264.00	60.20	62.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120216\
Data File : BF091389.D
Acq On : 2 Dec 2016 15:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 05:57:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

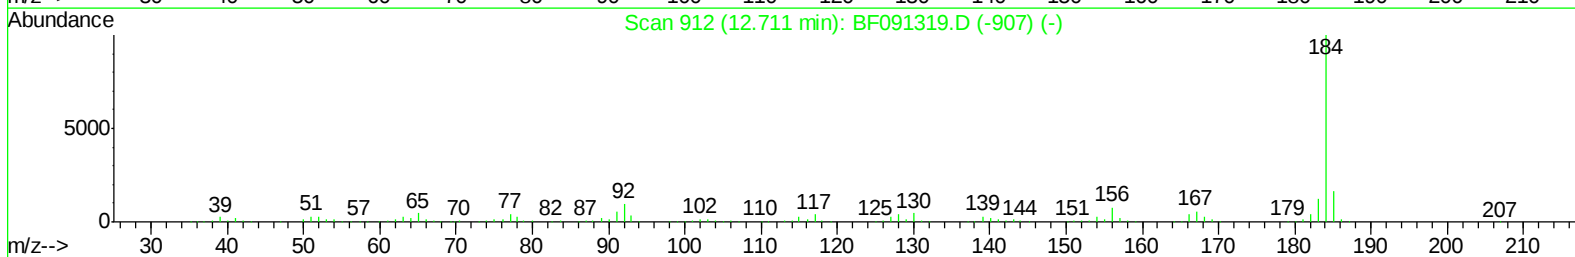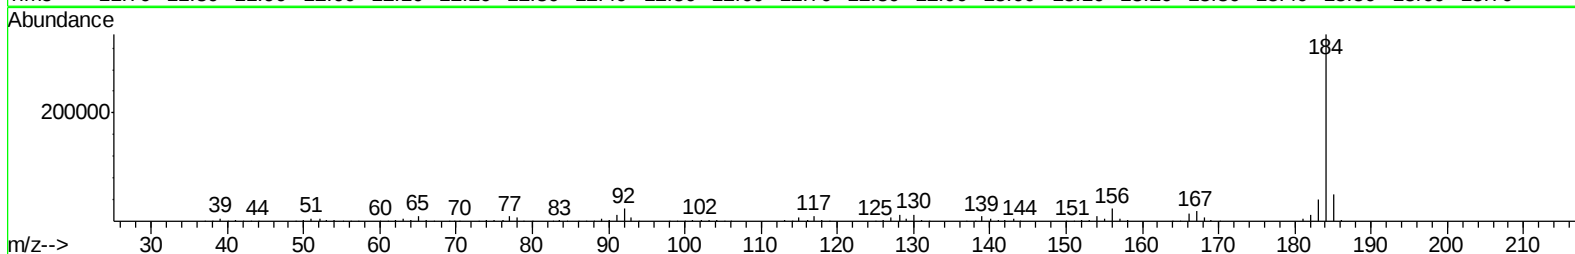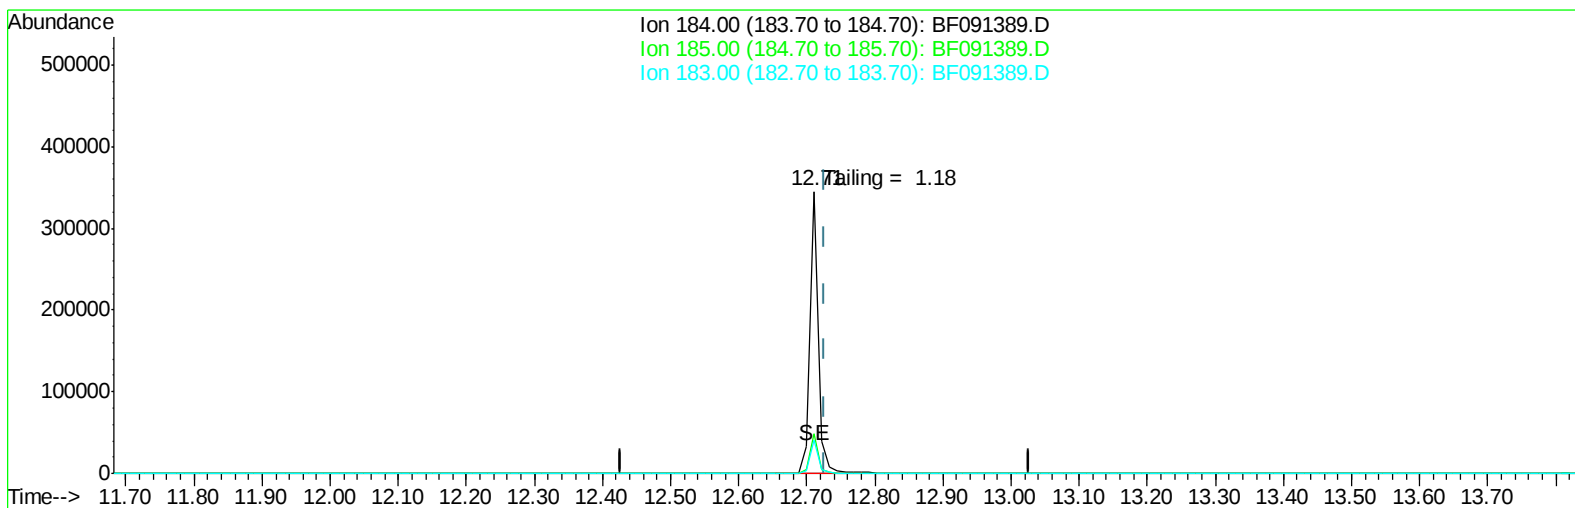

TIC: BF091389.D

(76) Benzidine

12.711min (-0.016) 38664.39ng

response 300787

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.33
183.00	11.10	11.67
0.00	0.00	0.00