


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120216\
 Data File : BF091384.D
 Acq On : 2 Dec 2016 8:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

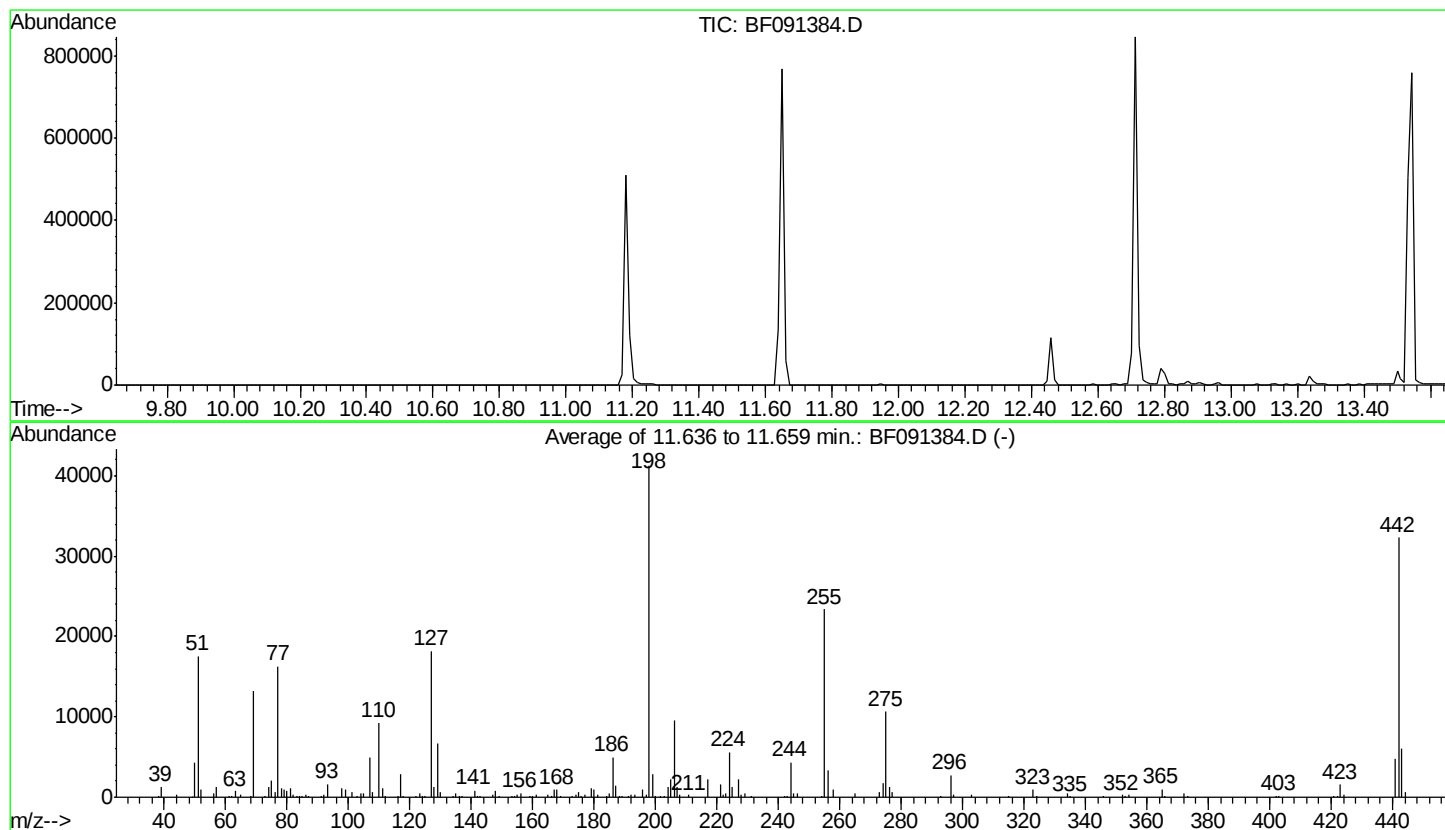

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	17607	PASS
68	69	0.00	2	1.1	144	PASS
69	198	0.00	100	32.2	13306	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	18222	PASS
197	198	0.00	2	0.7	280	PASS
198	198	100	100	100.0	41265	PASS
199	198	5	9	7.1	2923	PASS
275	198	10	60	25.8	10635	PASS
365	198	1	100	2.5	1022	PASS
441	442	0.01	24	15.0	4858	PASS
442	198	50	100	78.3	32305	PASS
443	442	15	24	19.0	6124	PASS