


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120216\
 Data File : BF091389.D
 Acq On : 2 Dec 2016 15:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

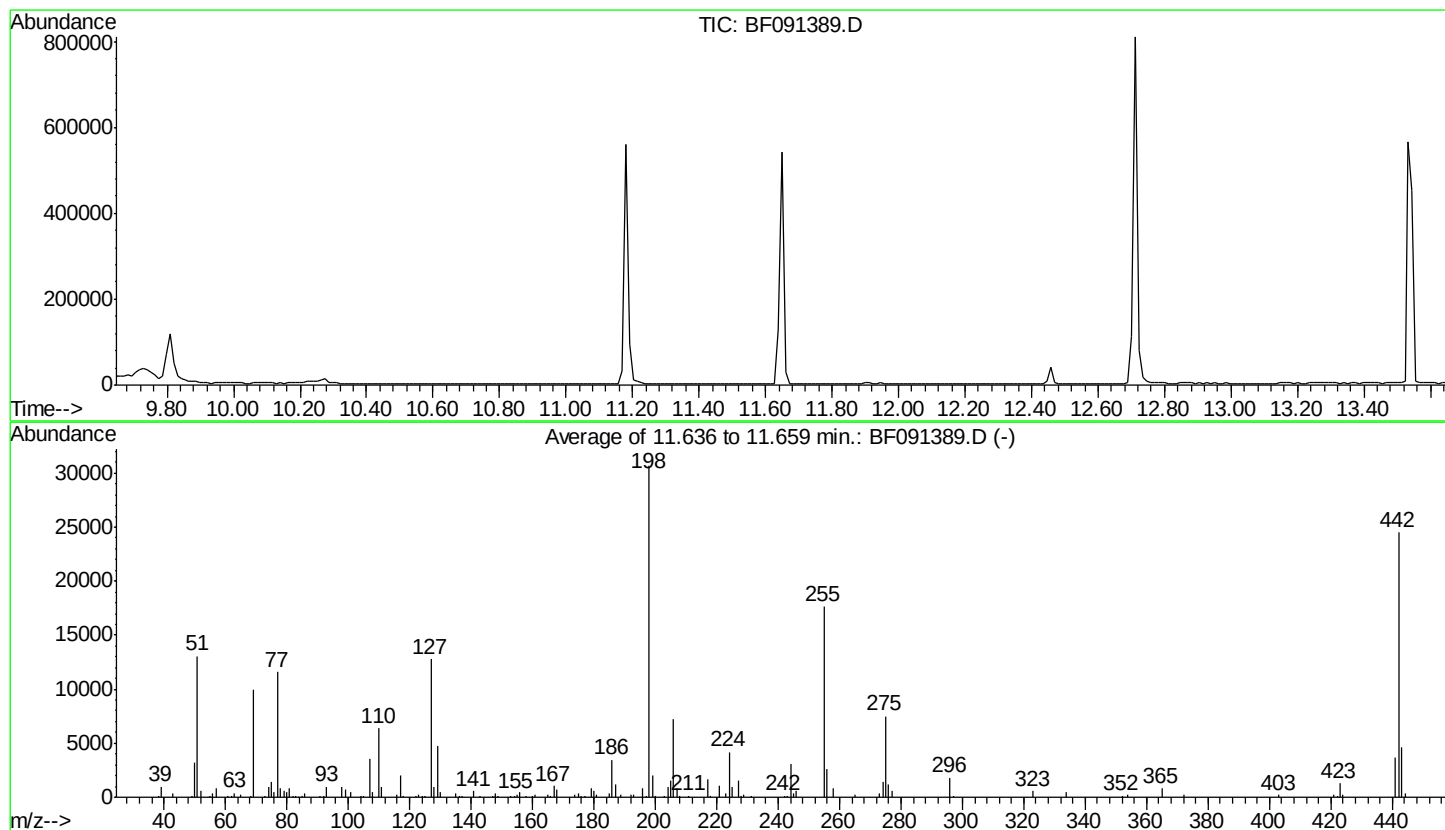

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	13073	PASS
68	69	0.00	2	1.1	106	PASS
69	198	0.00	100	32.6	10003	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	12780	PASS
197	198	0.00	2	0.5	165	PASS
198	198	100	100	100.0	30684	PASS
199	198	5	9	6.4	1962	PASS
275	198	10	60	24.5	7520	PASS
365	198	1	100	2.7	829	PASS
441	442	0.01	24	15.1	3694	PASS
442	198	50	100	79.8	24483	PASS
443	442	15	24	18.8	4599	PASS