
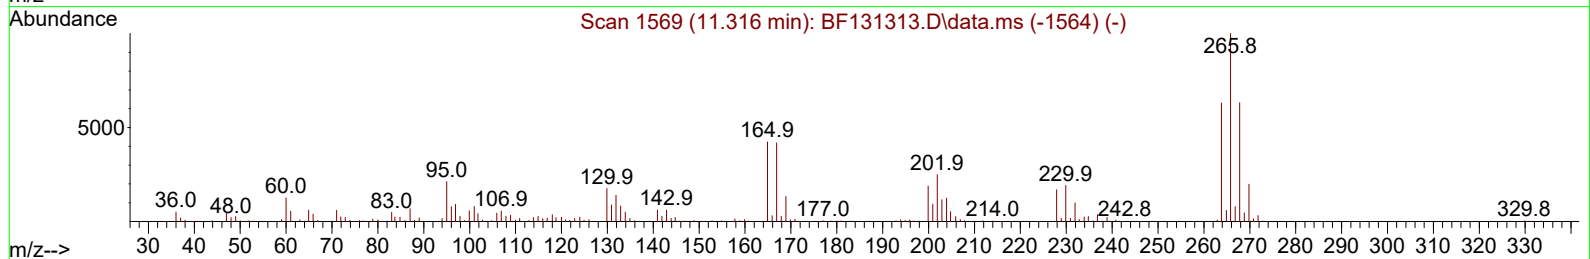
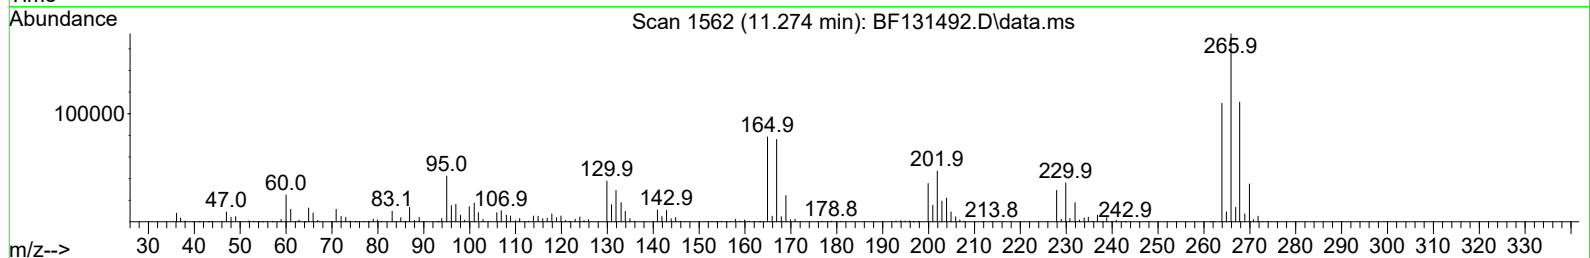


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120222\
 Data File : BF131492.D
 Acq On : 02 Dec 2022 10:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 01:24:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 05 00:00:18 2022
 Response via : Initial Calibration

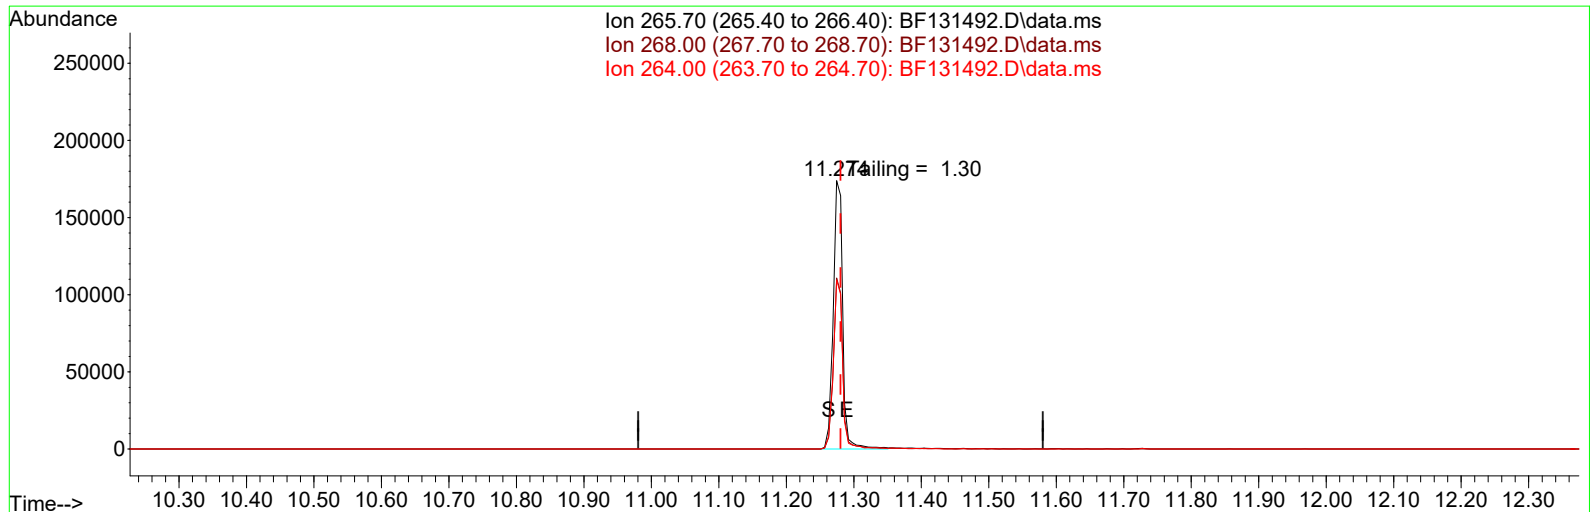

TIC: BF131492.D\data.ms

(70) Pentachlorophenol (C)




11.274min (-0.006) 26262.49 ng

response 170143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.72
264.00	63.00	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120222\
Data File : BF131492.D
Acq On : 02 Dec 2022 10:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 01:24:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 05 00:00:18 2022
Response via : Initial Calibration

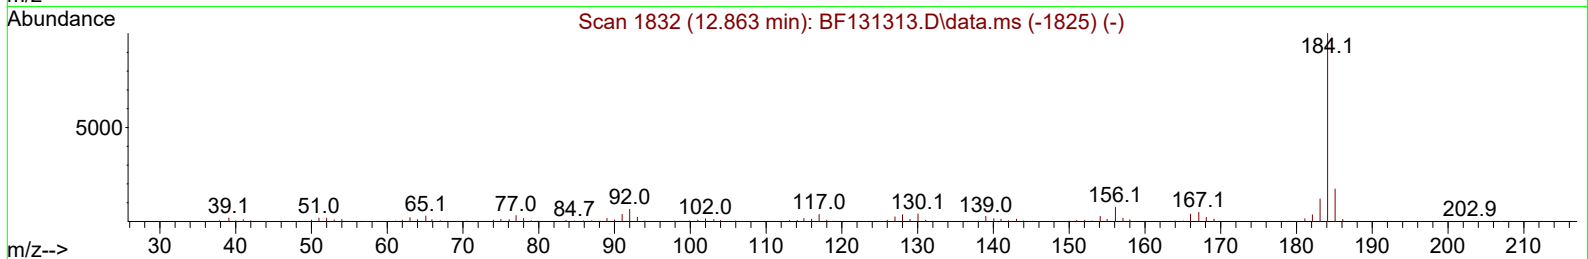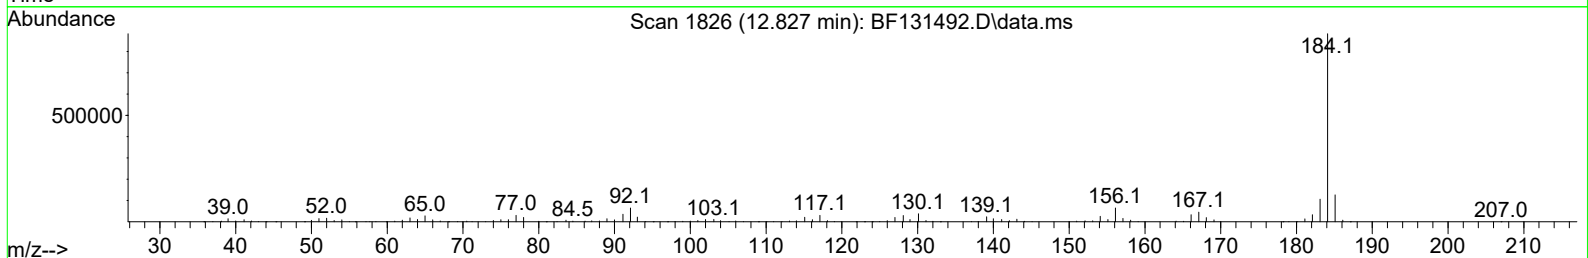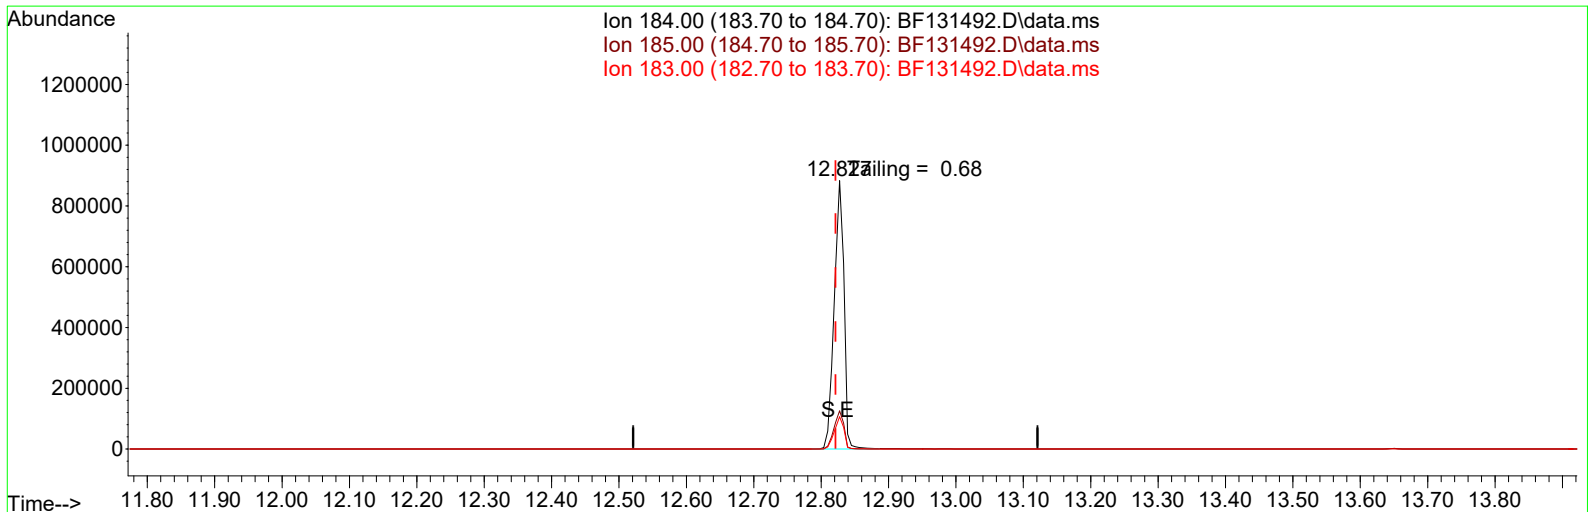

TIC: BF131492.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 0.00 ng

response 887196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.29
183.00	12.00	12.05
0.00	0.00	0.00