
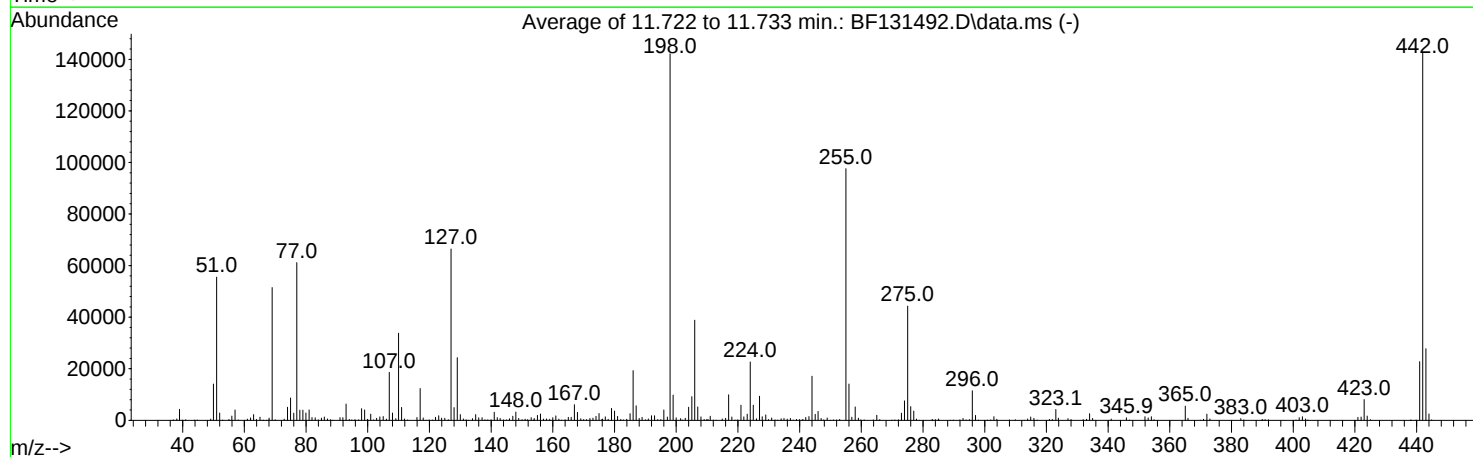


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120222\
 Data File : BF131492.D
 Acq On : 02 Dec 2022 10:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 05 00:00:18 2022

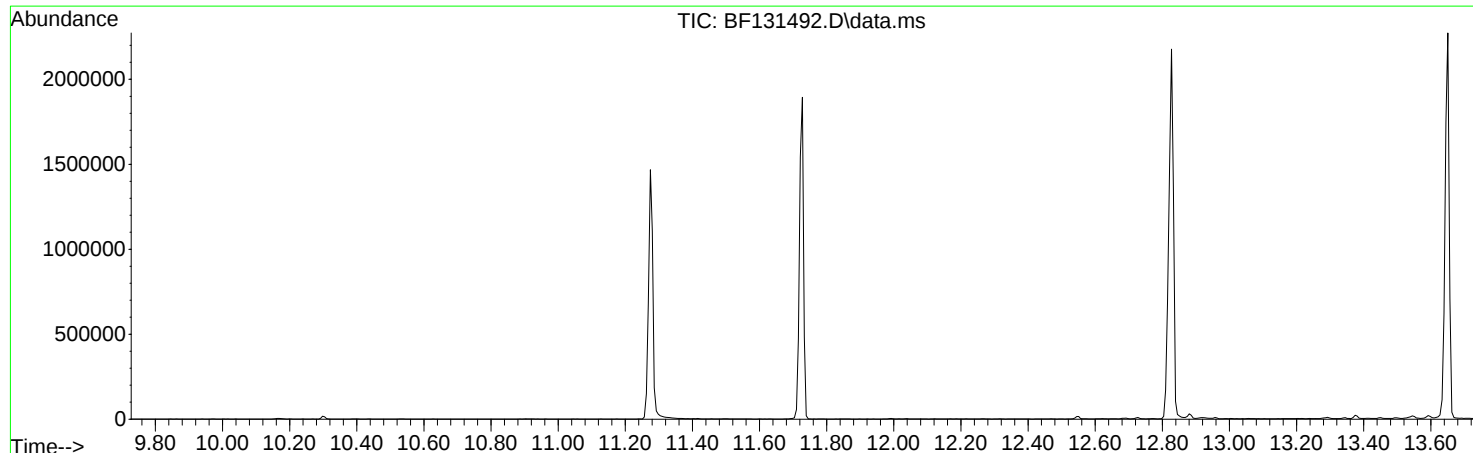




AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	55512	PASS
68	69	0.00	2	1.7	859	PASS
69	198	0.00	100	36.2	51508	PASS
70	69	0.00	2	0.4	221	PASS
127	198	10	80	46.7	66442	PASS
197	198	0.00	2	0.9	1302	PASS
198	198	100	100	100.0	142147	PASS
199	198	5	9	6.9	9795	PASS
275	198	10	60	31.2	44283	PASS
365	198	1	100	3.9	5518	PASS
441	198	0.01	100	16.0	22760	PASS
442	442	50	100	100.0	142680	PASS
443	442	15	24	19.5	27768	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120222\
 Data File : BF131492.D
 Acq On : 02 Dec 2022 10:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 05 01:24:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 05 00:00:18 2022
 Response via : Initial Calibration

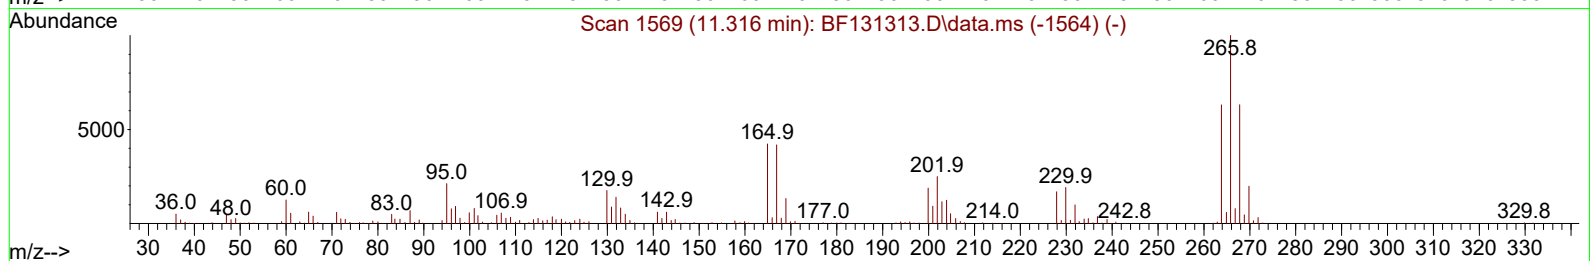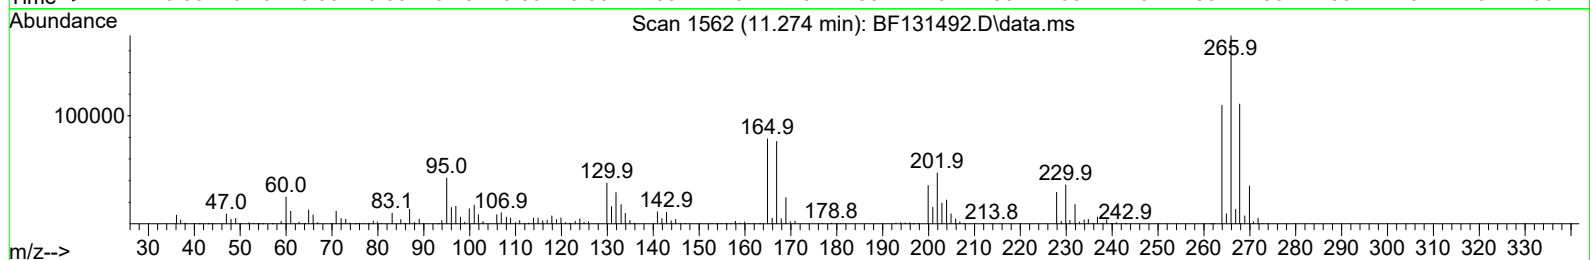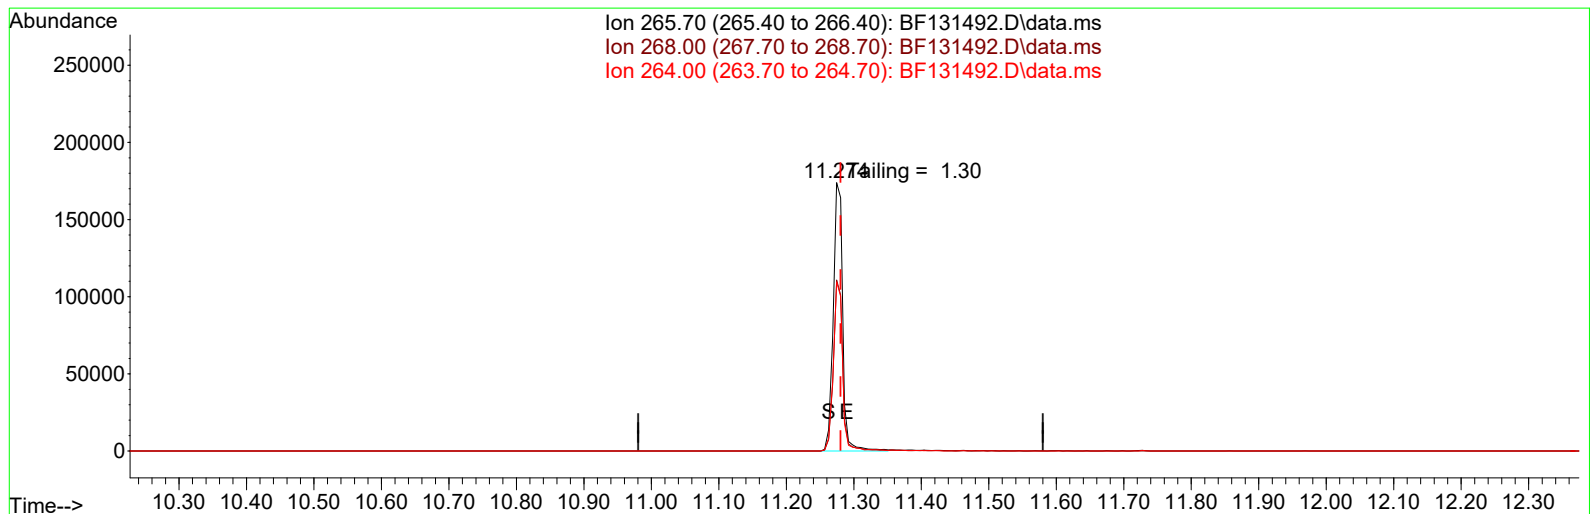

TIC: BF131492.D\data.ms

(70) Pentachlorophenol (C)

11.274min (-0.006) 26262.49 ng




response 170143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.72
264.00	63.00	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120222\
 Data File : BF131492.D
 Acq On : 02 Dec 2022 10:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 05 01:24:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 05 00:00:18 2022
 Response via : Initial Calibration

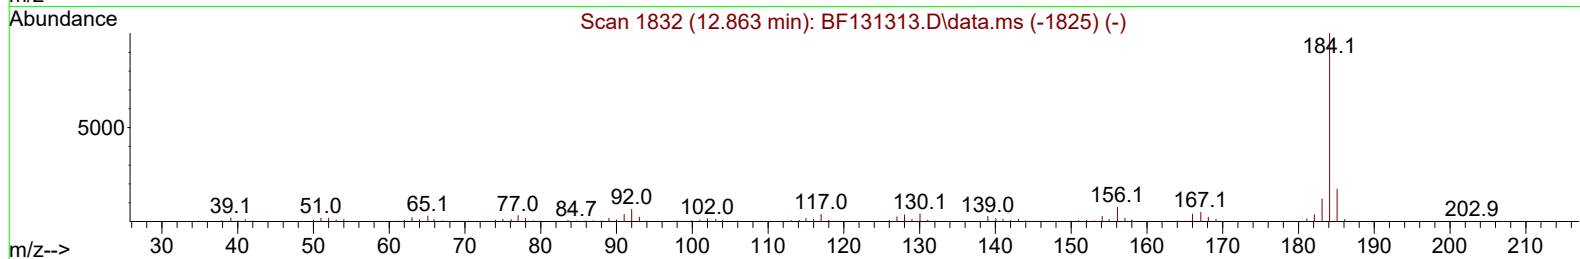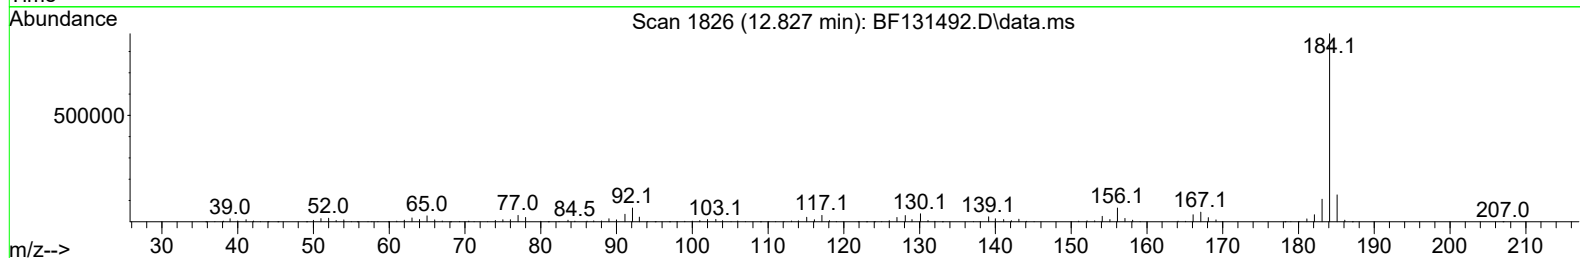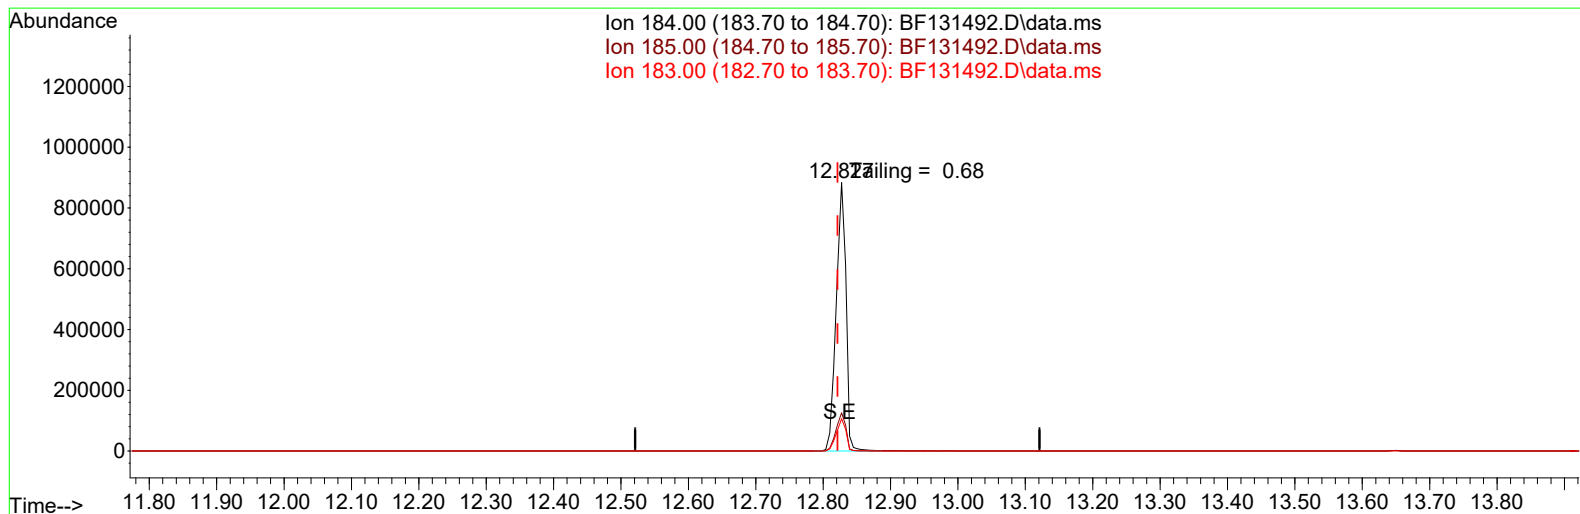

TIC: BF131492.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 0.00 ng

response 887196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.29
183.00	12.00	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/2/2022	BNA_F	<u>BF131492.D</u>
Compound Name	Response	Retention Time
DDT	393312	13.651
DDD	4978	13.38
DDE	228	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5206	398518	1.31

Instrument :
BNA_F
ClientSampleId :
DFTPP