
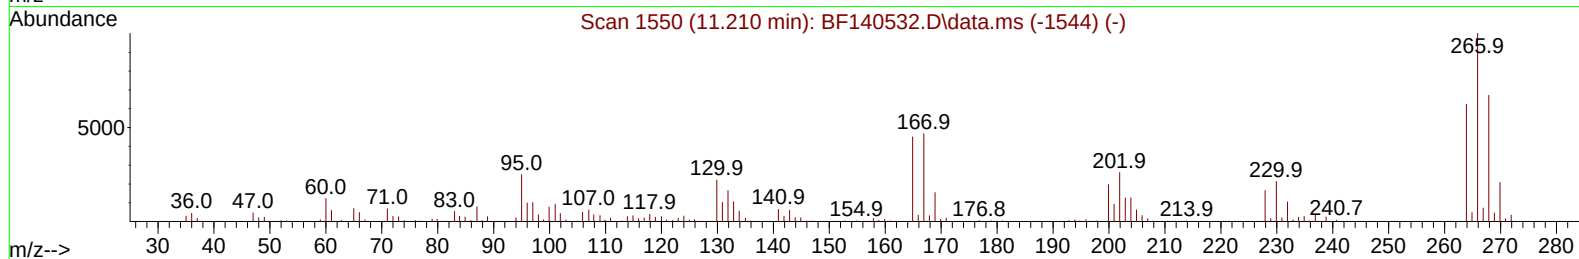
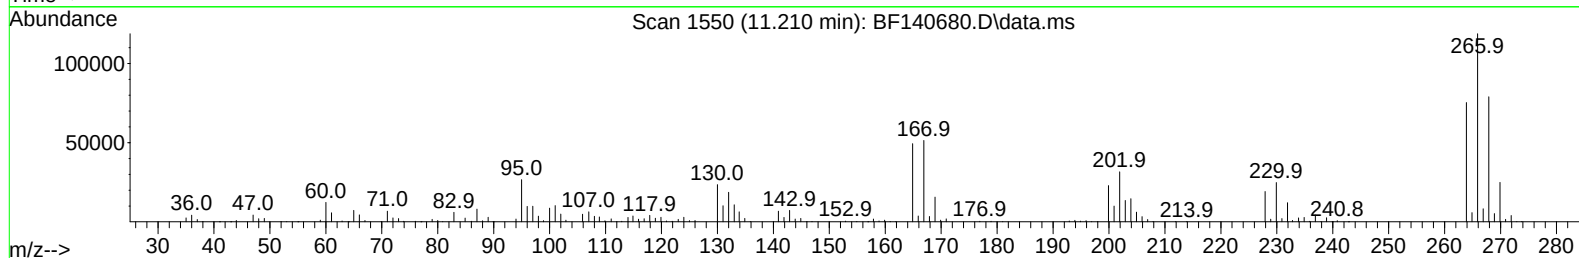


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140680.D
Acq On : 02 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 10:53:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

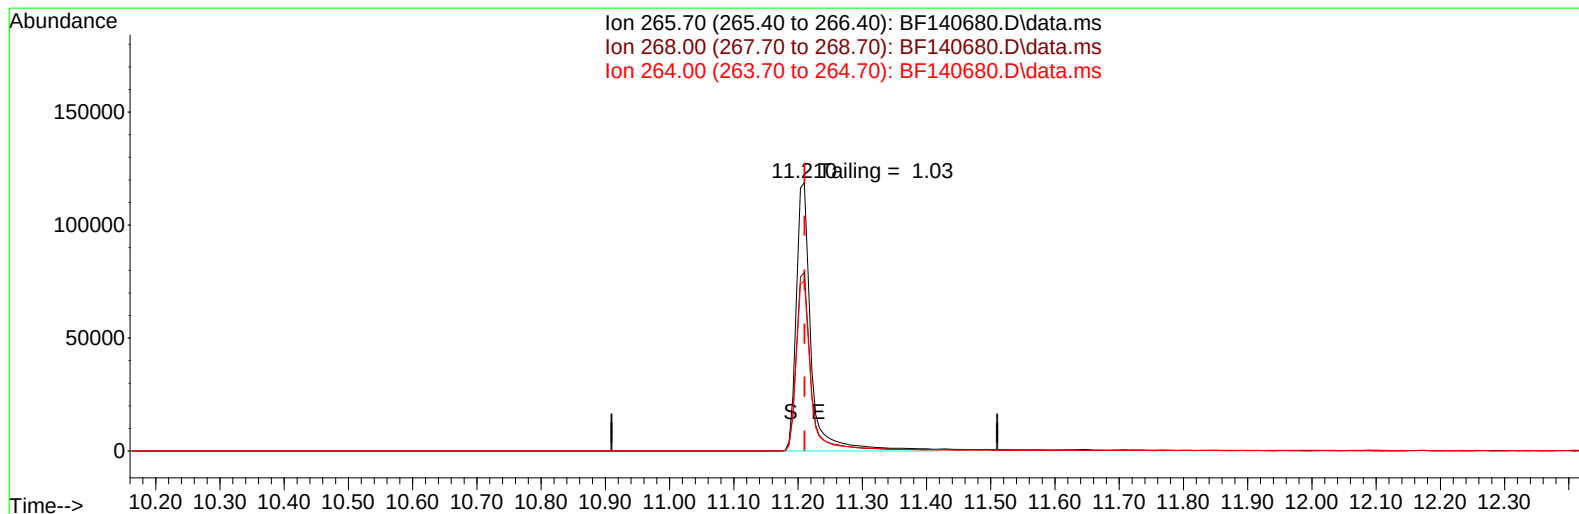

TIC: BF140680.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 19742.67 ng

response 192207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.55
264.00	62.30	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140680.D
Acq On : 02 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 10:53:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

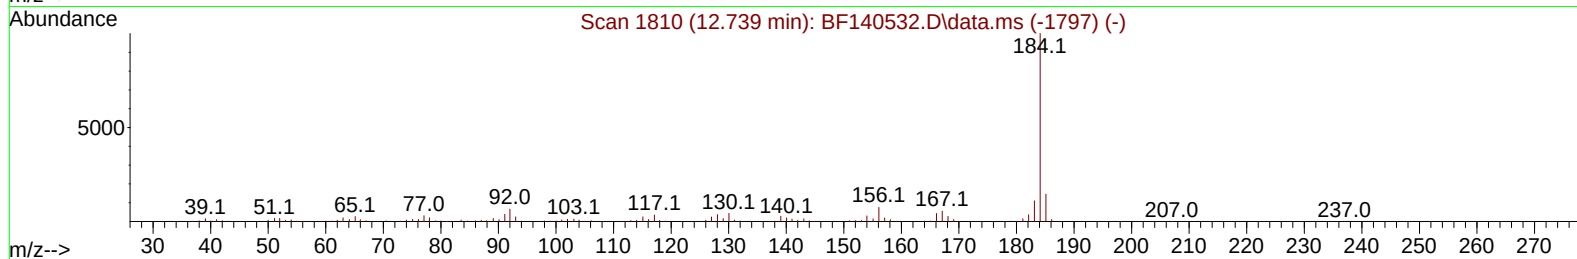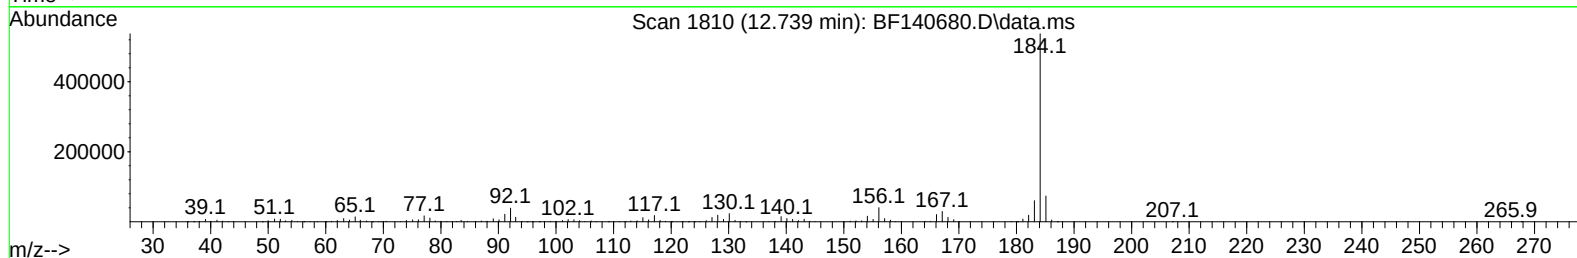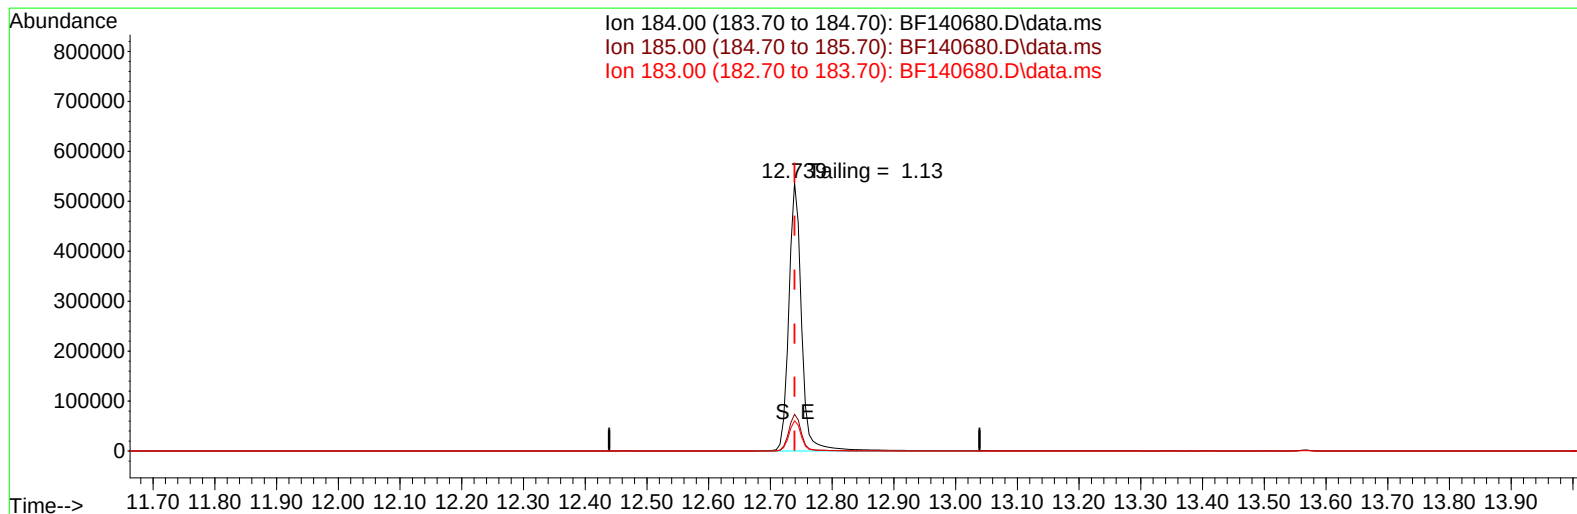

TIC: BF140680.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 18798.86 ng

response 775031

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.73
183.00	11.00	11.31
0.00	0.00	0.00