

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
 Data File : BF140685.D
 Acq On : 02 Dec 2024 12:15
 Operator : RC/JU
 Sample : PB165294BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165294BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	10	20	28	rVB	45396	77962	2.68%	0.470%
2	5.510	575	581	596	rBV	1556113	2131991	73.35%	12.848%
3	6.510	745	751	776	rBV	1569693	2190942	75.38%	13.203%
4	6.869	807	812	821	rBV	374948	457210	15.73%	2.755%
5	7.434	901	908	932	rBV	1028032	1434722	49.36%	8.646%
6	8.151	1024	1030	1045	rBV	432720	589878	20.29%	3.555%
7	9.222	1206	1212	1241	rBV	2099186	2841367	97.76%	17.123%
8	9.904	1322	1328	1348	rBV	517515	693492	23.86%	4.179%
9	10.698	1458	1463	1496	rBV	1168137	1632721	56.17%	9.839%
10	11.398	1576	1582	1606	rBV	542935	752452	25.89%	4.534%
11	12.986	1846	1852	1874	rBV	2155269	2906525	100.00%	17.516%
12	14.057	2029	2034	2049	rBV	337818	502742	17.30%	3.030%
13	15.580	2287	2293	2308	rBV	202140	381972	13.14%	2.302%




Sum of corrected areas: 16593976

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140685.D
Acq On : 02 Dec 2024 12:15
Operator : RC/JU
Sample : PB165294BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165294BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

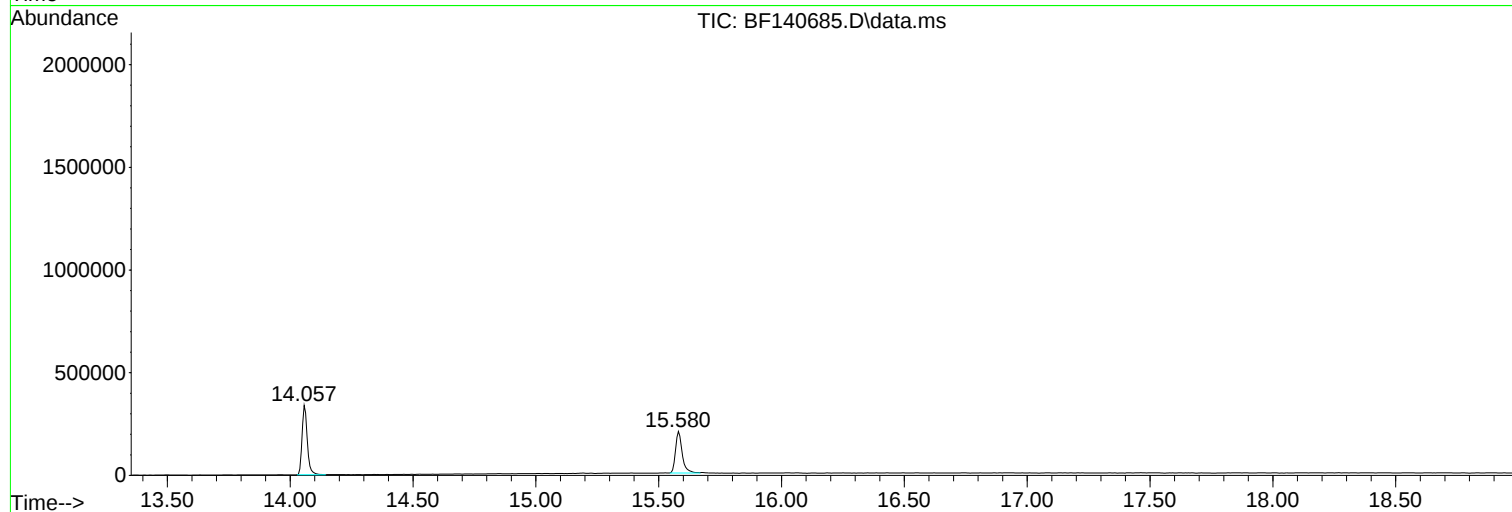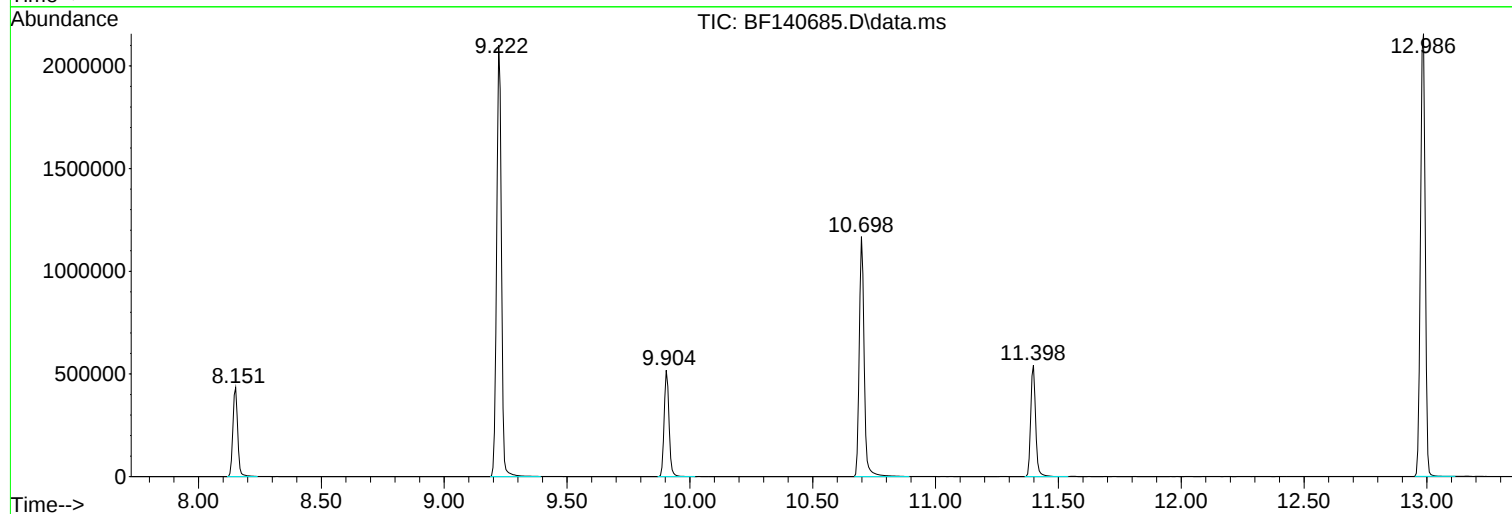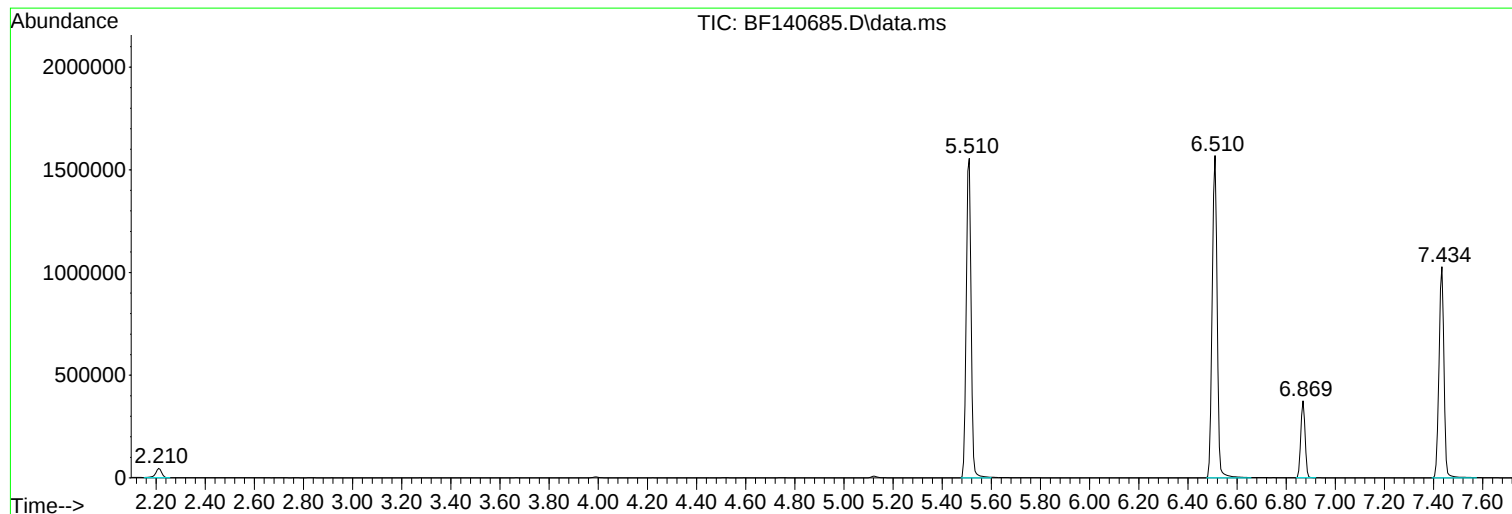

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140685.D
Acq On : 02 Dec 2024 12:15
Operator : RC/JU
Sample : PB165294BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165294BL








Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.210	3.41 ng	77962	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

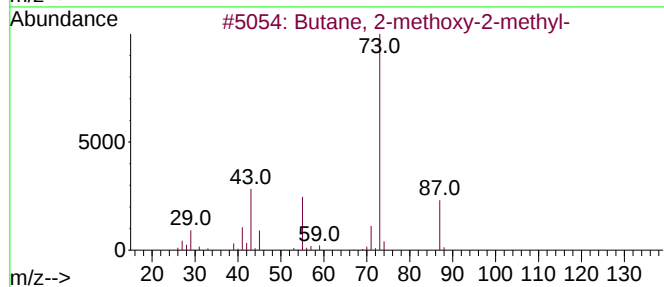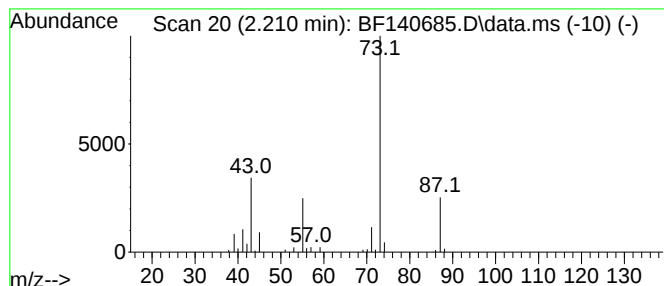

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140685.D
Acq On : 02 Dec 2024 12:15
Operator : RC/JU
Sample : PB165294BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165294BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.210	3.4	ng	77962	1	6.869	457210	20.0