

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120315\
 Data File : BF083486.D
 Acq On : 4 Dec 2015 4:28
 Operator : UM/IZ
 Sample : G4588-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-14

Quant Time: Dec 04 06:21:01 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 01:17:16 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.52	152	171652	20.00	ng	-0.02
21) Naphthalene-d8	7.81	136	636381	20.00	ng	-0.02
38) Acenaphthene-d10	9.56	164	309561	20.00	ng	-0.02
63) Phenanthrene-d10	11.09	188	437851	20.00	ng	-0.03
75) Chrysene-d12	14.71	240	346818	20.00	ng	-0.06
86) Perylene-d12	16.77	264	281915	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	810166	70.82	ng	-0.01
7) Phenol-d6	6.20	99	710607	45.38	ng	-0.02
23) Nitrobenzene-d5	7.10	82	1299005	89.73	ng	-0.02
41) 2,4,6-Tribromophenol	10.35	330	323924	104.24	ng	-0.03
44) 2-Fluorobiphenyl	8.90	172	1888815	86.95	ng	-0.02
78) Terphenyl-d14	13.19	244	1303778	89.65	ng	-0.03
Target Compounds						Qvalue
9) Benzaldehyde	6.30	77	35707	2.86	ng	# 74
19) n-Nitroso-di-n-propylamine	7.10	70	184018	16.44	ng	# 82
25) Isophorone	7.10	82	977631	34.86	ng	# 70
49) Dimethylphthalate	9.30	163	59344	2.36	ng	97
50) 2,6-Dinitrotoluene	9.56	165	38935	7.25	ng	# 19
56) 2,4-Dinitrotoluene	9.56	165	38935	5.71	ng	# 7
66) 4-Bromophenyl-phenylether	10.35	248	22858	4.77	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120315\
Data File : BF083486.D
Acq On : 4 Dec 2015 4:28
Operator : UM/IZ
Sample : G4588-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-14

Quant Time: Dec 04 06:21:01 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

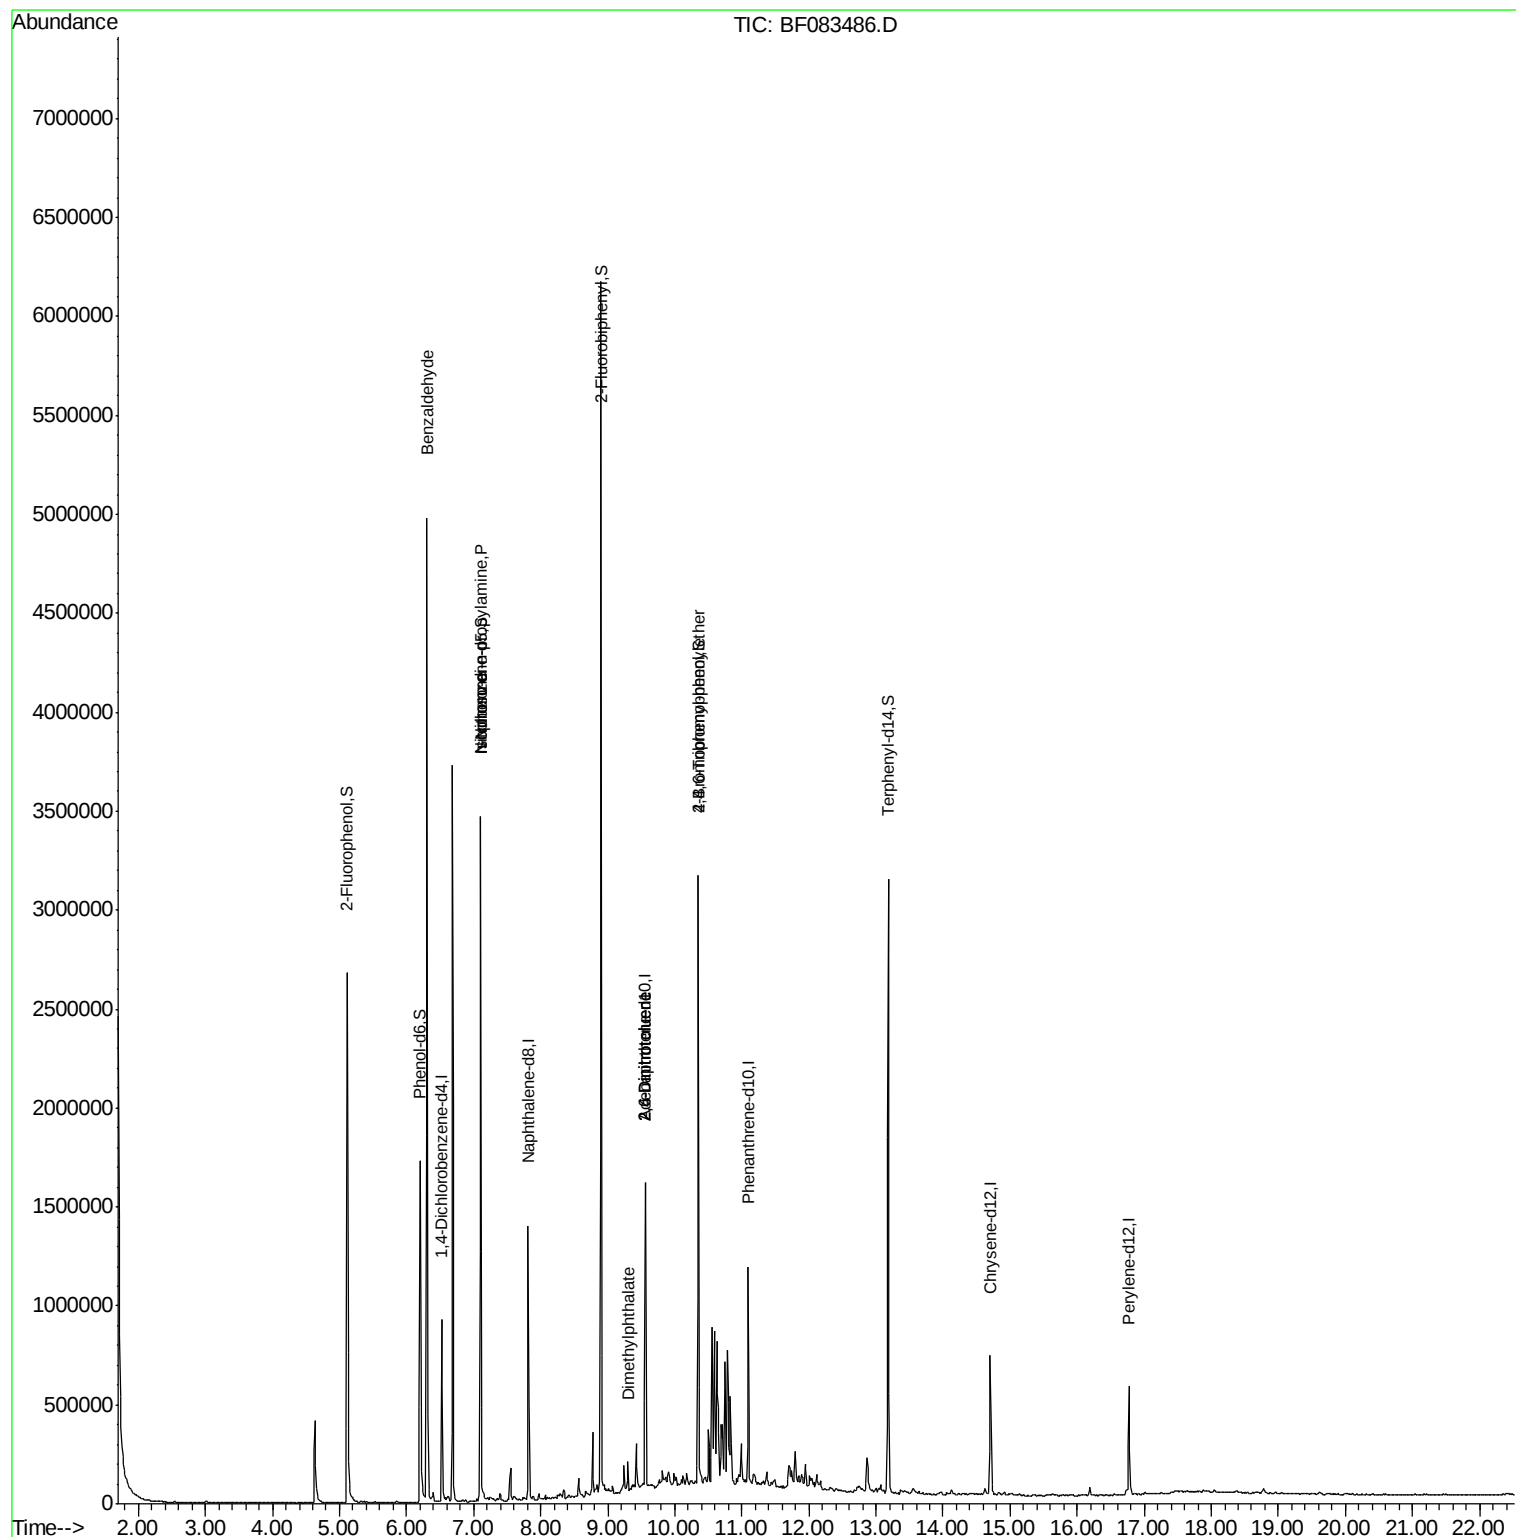



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.52 min Scan# 423

Delta R.T. -0.02 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Instrument :

BNA_F

ClientSampleId :

MW-14


Tgt Ion:152 Resp: 171652

Ion Ratio Lower Upper

152 100

150 157.9 129.8 194.8




115 72.6 59.2 88.8



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

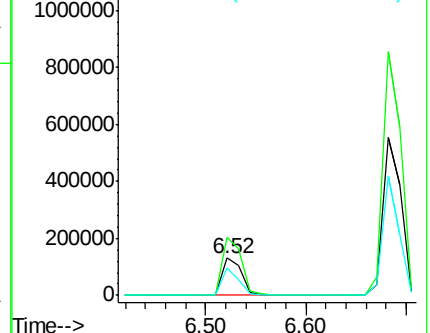

#5

2-Fluorophenol

Concen: 70.82 ng

RT: 5.12 min Scan# 300

Delta R.T. -0.01 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28


Tgt Ion:112 Resp: 810166

Ion Ratio Lower Upper

112 100

64 67.1 55.6 83.4



63 33.8 28.2 42.2




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

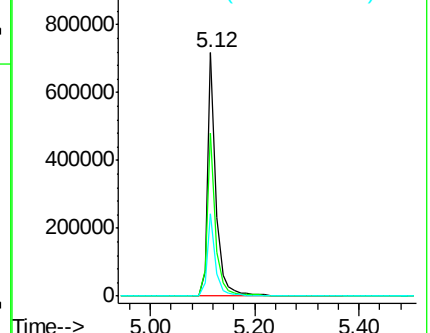

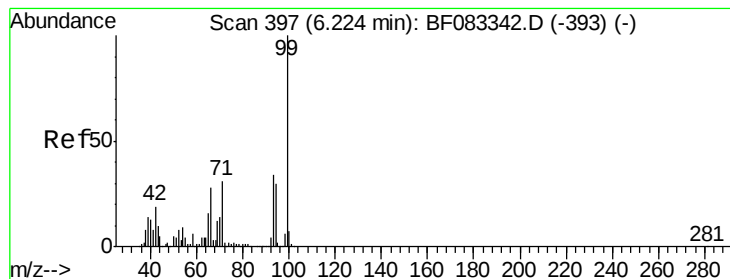

#7

Phenol-d6

Concen: 45.38 ng

RT: 6.20 min Scan# 395

Delta R.T. -0.02 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Instrument :

BNA_F

ClientSampleId :

MW-14





Tgt Ion: 99 Resp: 710607

Ion Ratio Lower Upper

99 100

42 18.2 14.9 22.3

71 30.2 24.7 37.1

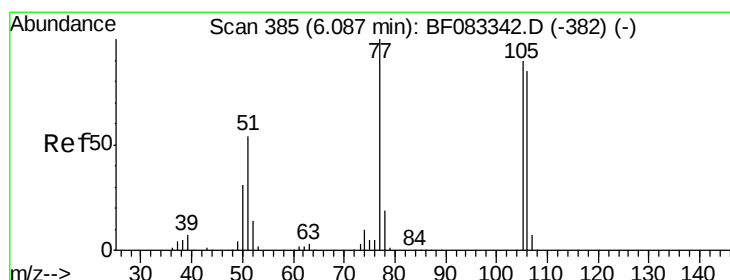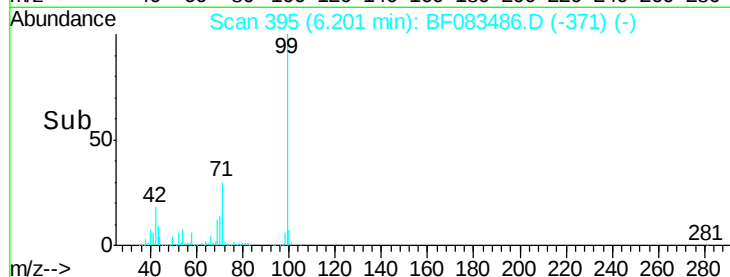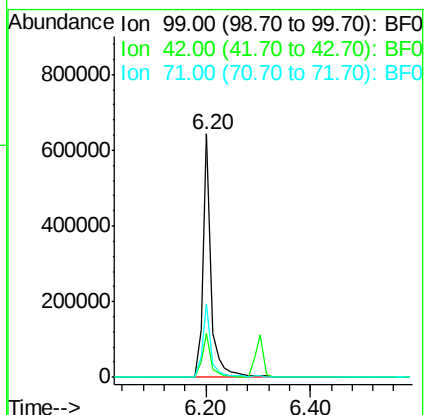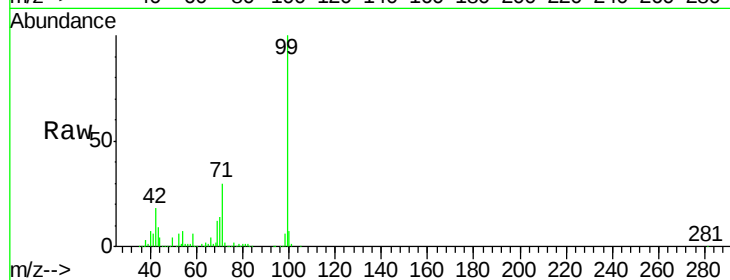

#9

Benzaldehyde

Concen: 2.86 ng

RT: 6.30 min Scan# 404

Delta R.T. 0.22 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28




Tgt Ion: 77 Resp: 35707




Ion Ratio Lower Upper

77 100

105 67.1 70.0 110.0#

106 60.2 65.0 105.0#

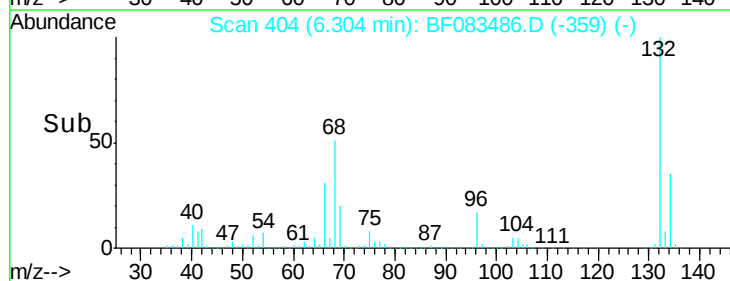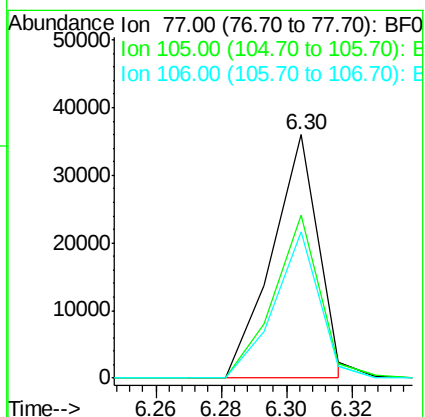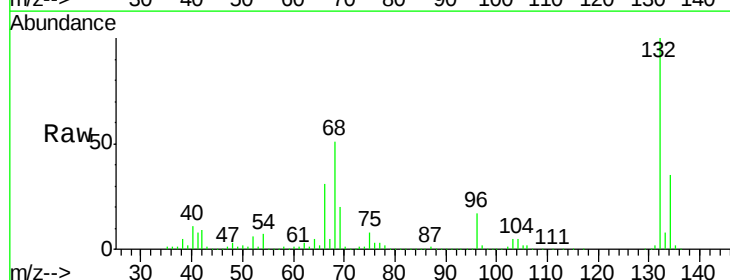

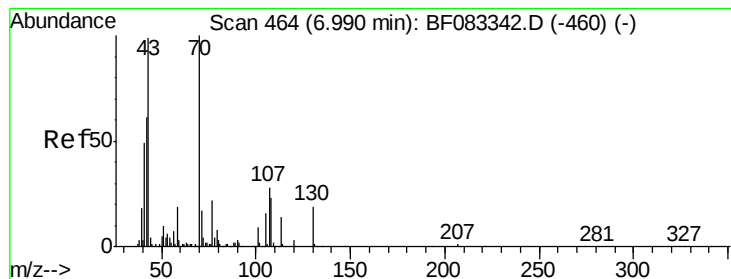

#19

n-Nitroso-di-n-propylamine

Concen: 16.44 ng

RT: 7.10 min Scan# 474

Delta R.T. 0.11 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Instrument :

BNA_F

ClientSampled :

MW-14

Tgt Ion: 70 Resp: 184018





Ion Ratio Lower Upper

70 100

42 52.3 48.8 73.2

101 0.0 7.1 10.7#

130 1.7 15.0 22.6#

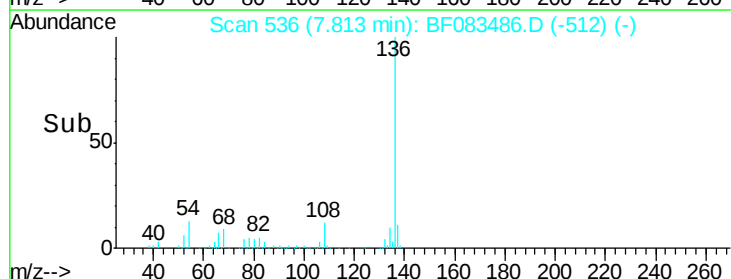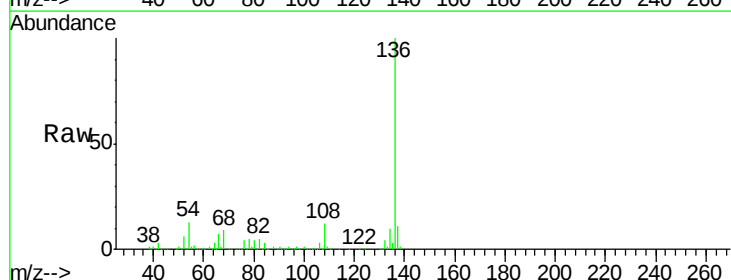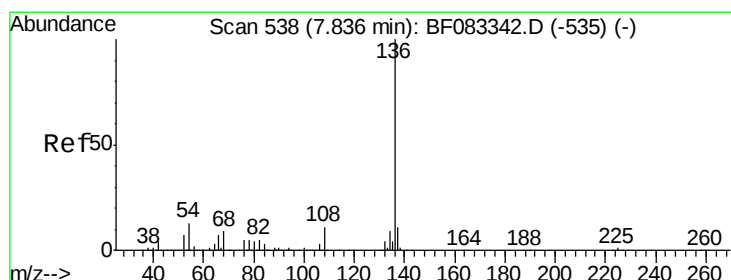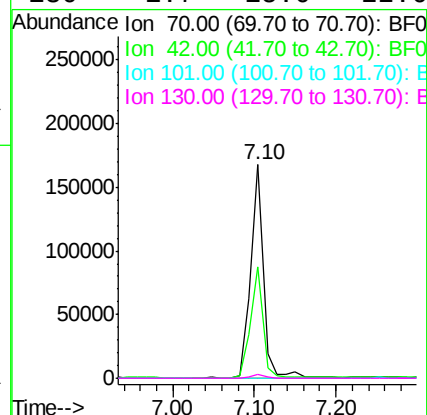

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.81 min Scan# 536

Delta R.T. -0.02 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Tgt Ion:136 Resp: 636381


Ion Ratio Lower Upper


136 100

137 11.3 9.0 13.4

54 12.6 10.1 15.1

68 8.6 7.1 10.7

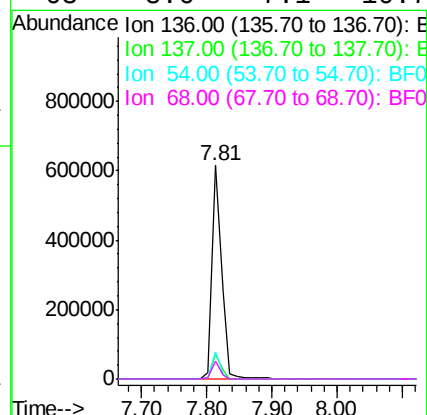

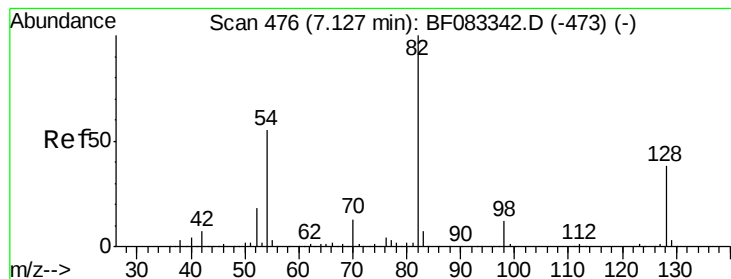

#23

Nitrobenzene-d5

Concen: 89.73 ng

RT: 7.10 min Scan# 474

Delta R.T. -0.02 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Instrument :

BNA_F

ClientSampleId :

MW-14


Tgt Ion: 82 Resp: 1299005

Ion Ratio Lower Upper

82 100

128 37.9 30.6 46.0




54 55.3 43.8 65.6



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

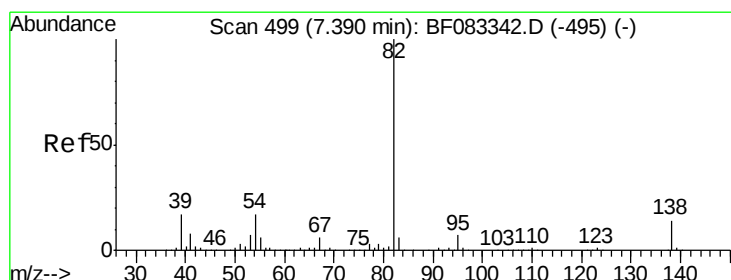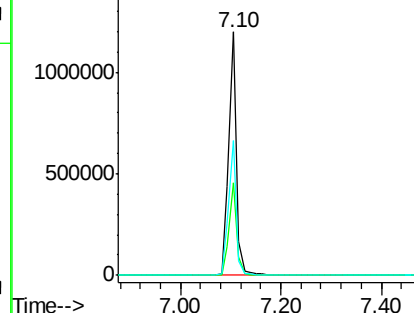

#25

Isophorone

Concen: 34.86 ng

RT: 7.10 min Scan# 474

Delta R.T. -0.29 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28


Tgt Ion: 82 Resp: 977631

Ion Ratio Lower Upper

82 100

95 0.0 5.3 7.9#



138 0.0 11.6 17.4#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0

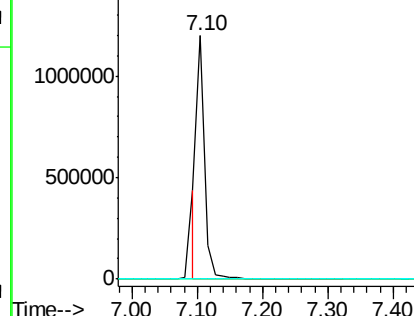



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.56 min Scan# 689

Delta R.T. -0.02 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Instrument :

BNA_F

ClientSampleId :

MW-14


Tgt Ion:164 Resp: 309561

Ion Ratio Lower Upper

164 100

162 101.0 82.6 123.8




160 45.4 35.3 52.9

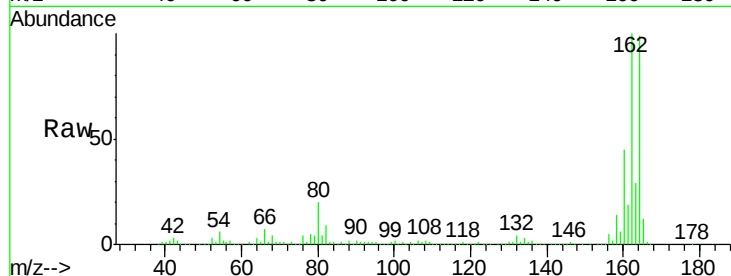

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

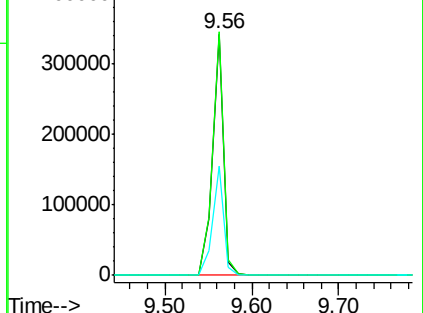

#41

2,4,6-Tribromophenol

Concen: 104.24 ng

RT: 10.35 min Scan# 758

Delta R.T. -0.03 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28


Tgt Ion:330 Resp: 323924

Ion Ratio Lower Upper

330 100

332 98.7 77.8 116.6



141 41.8 29.4 44.0




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

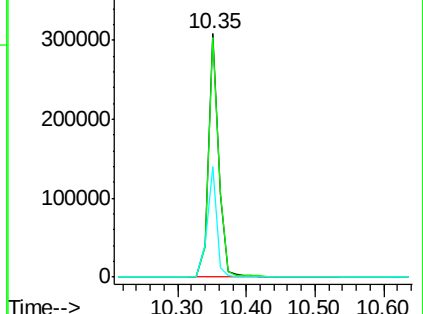







#44
 2-Fluorobiphenyl
 Concen: 86.95 ng
 RT: 8.90 min Scan# 631
 Delta R.T. -0.02 min
 Lab File: BF083486.D
 Acq: 4 Dec 2015 4:28

Instrument :
 BNA_F
 ClientSampleId :
 MW-14

Tgt Ion:172 Resp: 1888815
 Ion Ratio Lower Upper
 172 100
 171 37.1 29.4 44.0
 170 25.5 20.4 30.6




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

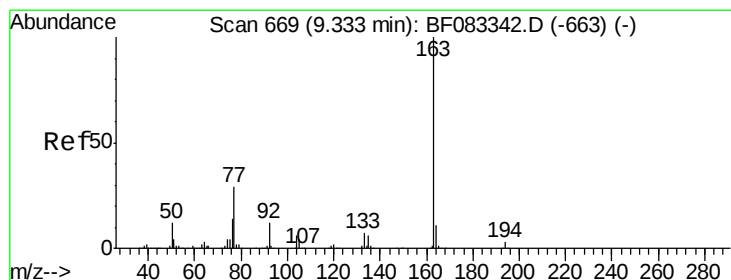
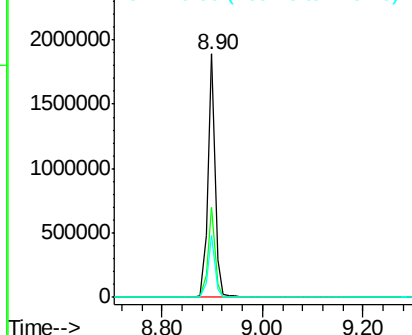



#49
 Dimethylphthalate
 Concen: 2.36 ng
 RT: 9.30 min Scan# 666
 Delta R.T. -0.03 min
 Lab File: BF083486.D
 Acq: 4 Dec 2015 4:28

Tgt Ion:163 Resp: 59344
 Ion Ratio Lower Upper
 163 100
 194 3.5 2.7 4.1
 164 9.7 8.8 13.2



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

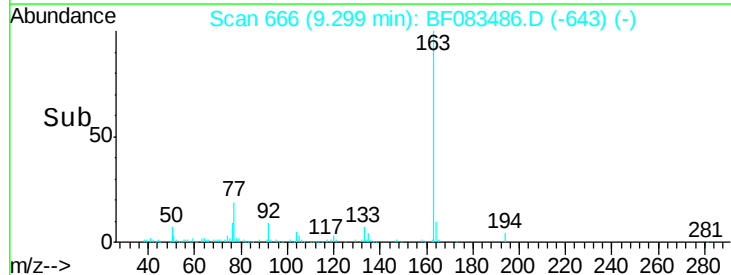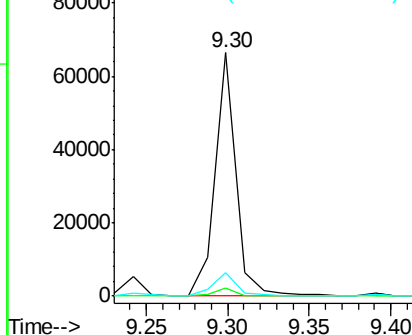

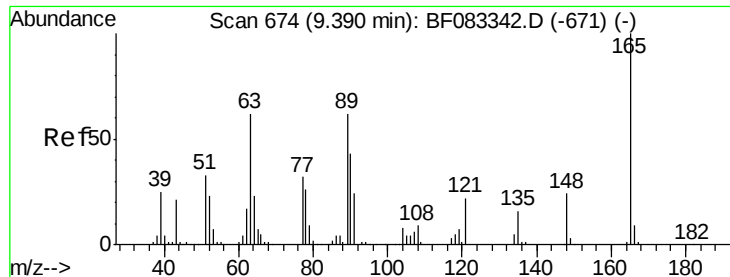

#50

2,6-Dinitrotoluene

Concen: 7.25 ng

RT: 9.56 min Scan# 689

Delta R.T. 0.17 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Instrument :

BNA_F

ClientSampled :

MW-14


Tgt Ion:165 Resp: 38935

Ion Ratio Lower Upper

165 100

63 2.0 56.0 84.0#




89 2.0 49.8 74.8#

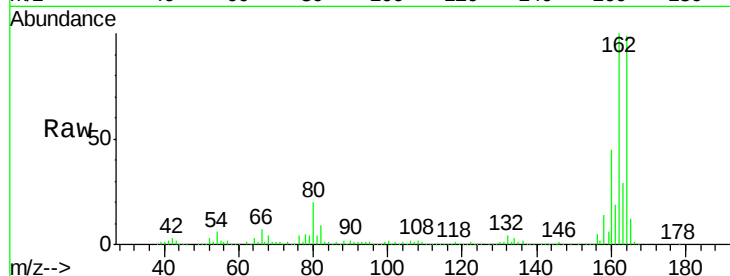

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

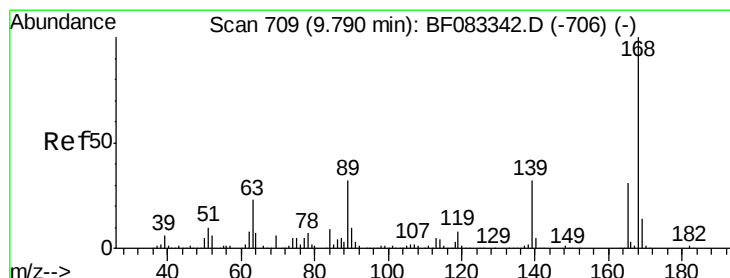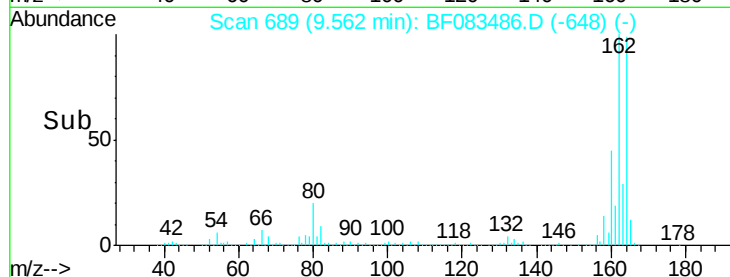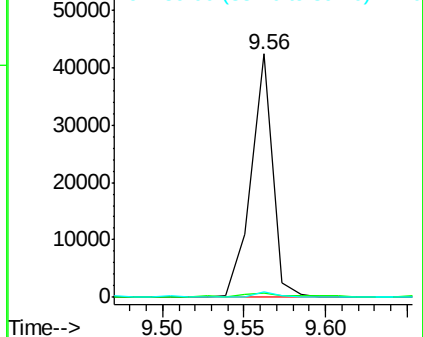

#56

2,4-Dinitrotoluene

Concen: 5.71 ng

RT: 9.56 min Scan# 689

Delta R.T. -0.23 min

Lab File: BF083486.D

Acq: 4 Dec 2015 4:28

Tgt Ion:165 Resp: 38935


Ion Ratio Lower Upper

165 100

63 2.0 65.4 98.0#

89 2.0 81.2 121.8#

182 0.0 1.8 2.8#


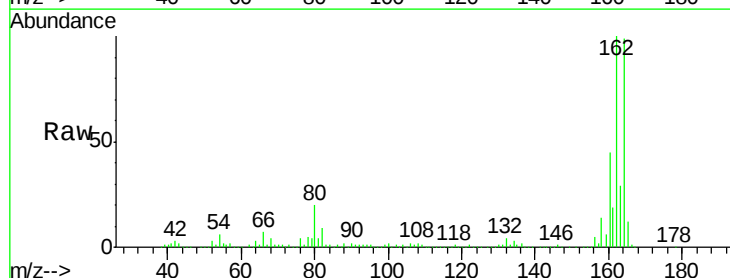



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

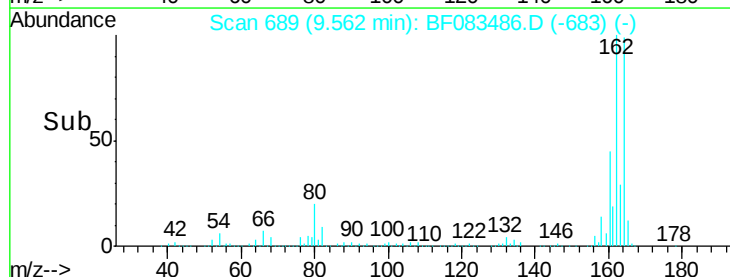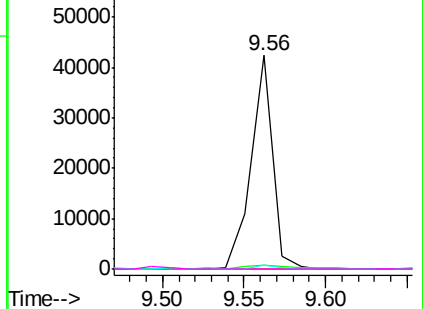


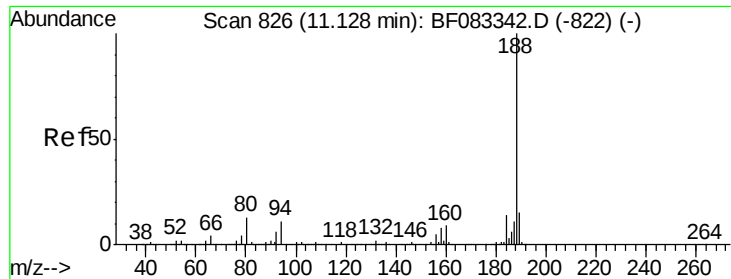




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.09 min Scan# 823
Delta R.T. -0.03 min
Lab File: BF083486.D
Acq: 4 Dec 2015 4:28

Instrument :
BNA_F
ClientSampleId :
MW-14

Tgt Ion:188 Resp: 437851
Ion Ratio Lower Upper
188 100
94 11.7 8.7 13.1
80 13.3 10.3 15.5




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

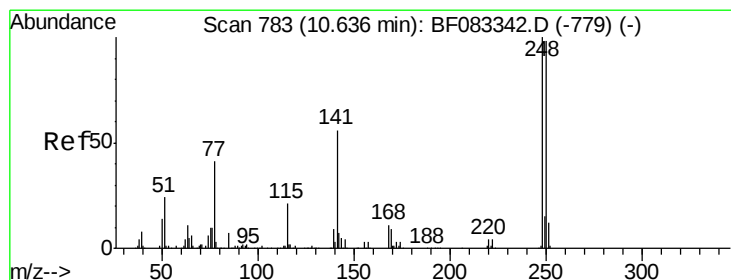
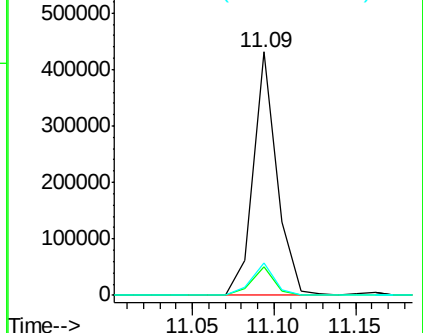



#66
4-Bromophenyl-phenylether
Concen: 4.77 ng
RT: 10.35 min Scan# 758
Delta R.T. -0.29 min
Lab File: BF083486.D
Acq: 4 Dec 2015 4:28

Tgt Ion:248 Resp: 22858
Ion Ratio Lower Upper
248 100
250 206.2 78.6 118.0#
141 600.5 44.4 66.6#



Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E




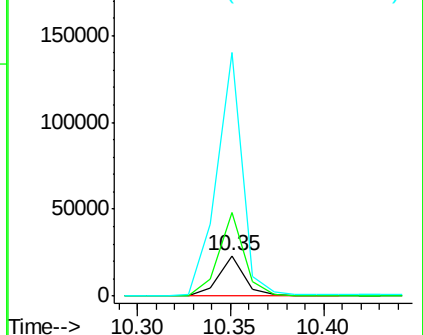


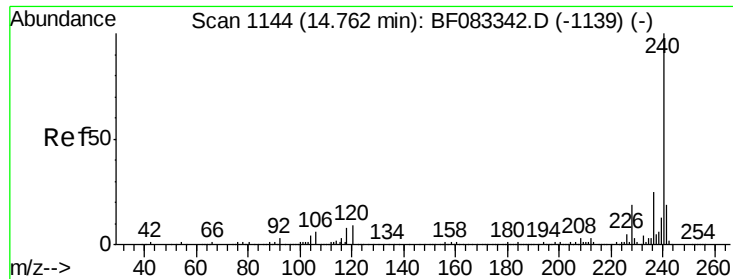

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 14.71 min Scan# 1139
 Delta R.T. -0.06 min
 Lab File: BF083486.D
 Acq: 4 Dec 2015 4:28




Instrument :
 BNA_F
 ClientSampleId :
 MW-14




Tgt Ion:240 Resp: 346818
 Ion Ratio Lower Upper
 240 100
 120 12.9 6.9 10.3#
 236 25.9 19.8 29.6

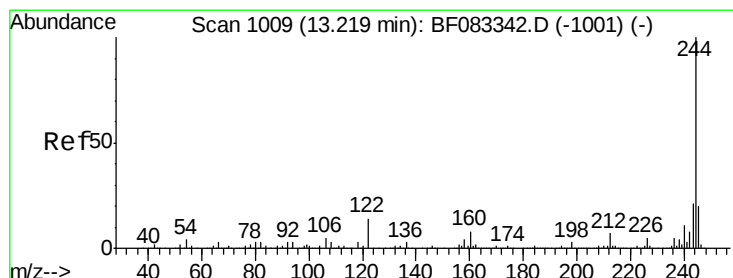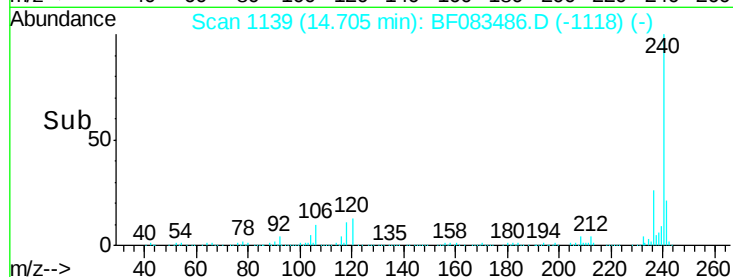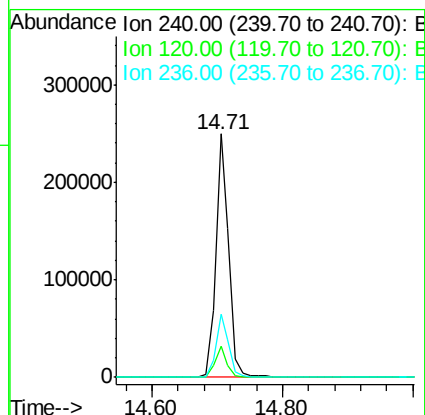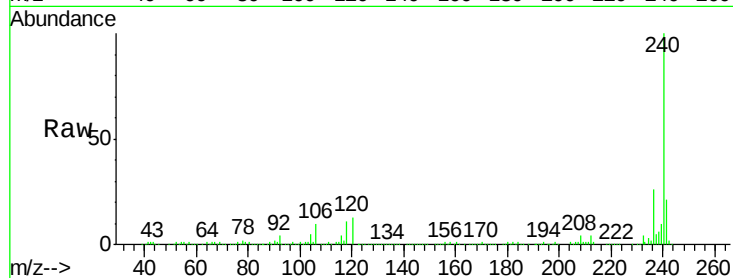

#78
 Terphenyl-d14
 Concen: 89.65 ng
 RT: 13.19 min Scan# 1006
 Delta R.T. -0.03 min
 Lab File: BF083486.D
 Acq: 4 Dec 2015 4:28

Tgt Ion:244 Resp: 1303778
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.8 8.8
 122 11.2 11.0 16.4

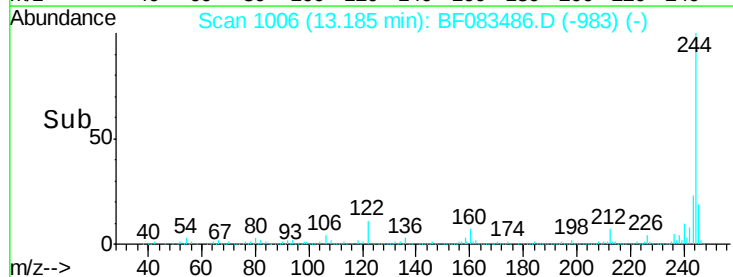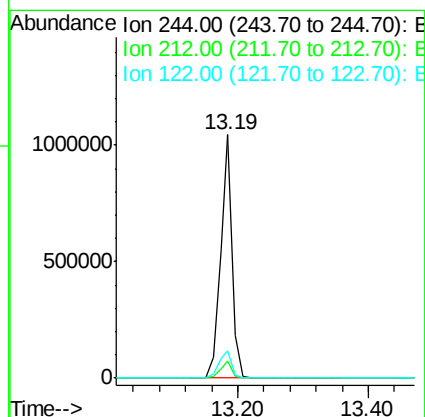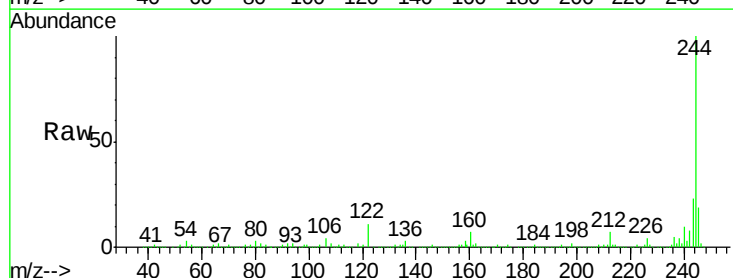

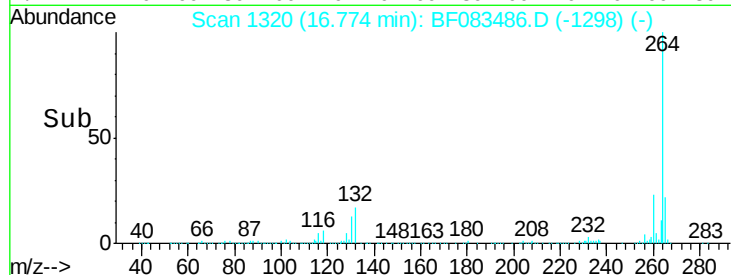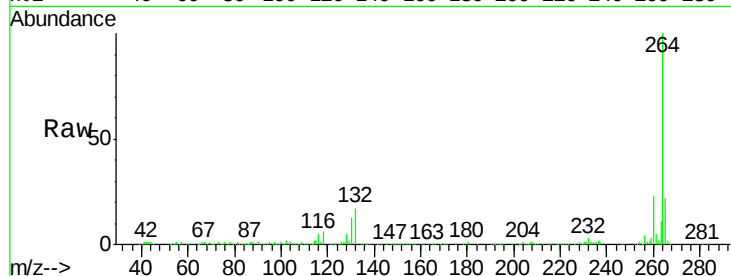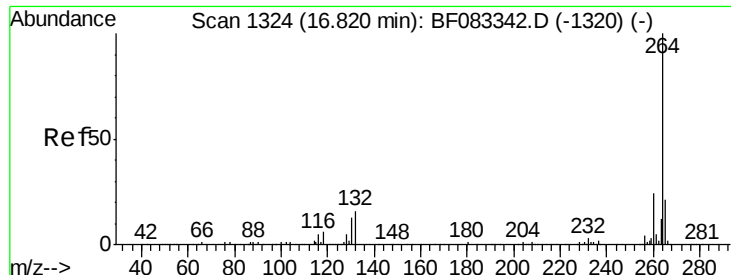

#86
Perylene-d12
Concen: 20.00 ng
RT: 16.77 min Scan# 1320
Delta R.T. -0.05 min
Lab File: BF083486.D
Acq: 4 Dec 2015 4:28

Instrument :
BNA_F
ClientSampleId :
MW-14

Tgt Ion:	264	Resp:	281915
Ion Ratio	Lower	Upper	
264	100		
260	22.5	19.0	28.4
265	21.6	16.8	25.2

