
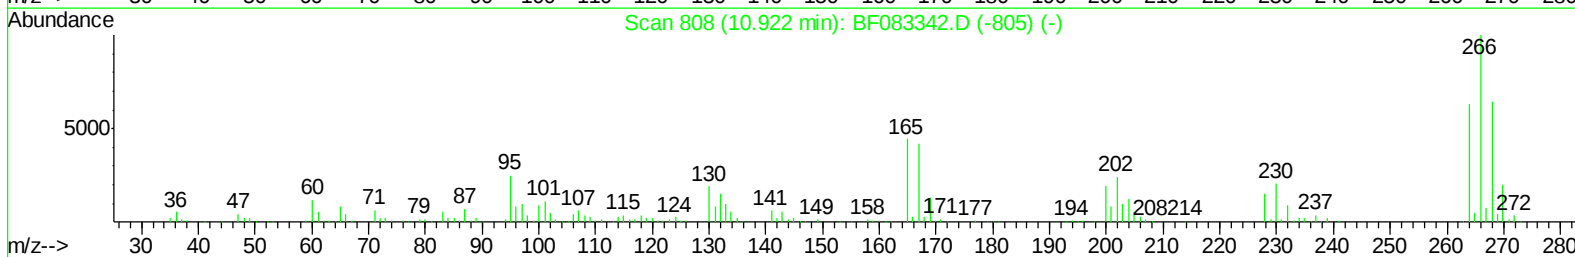
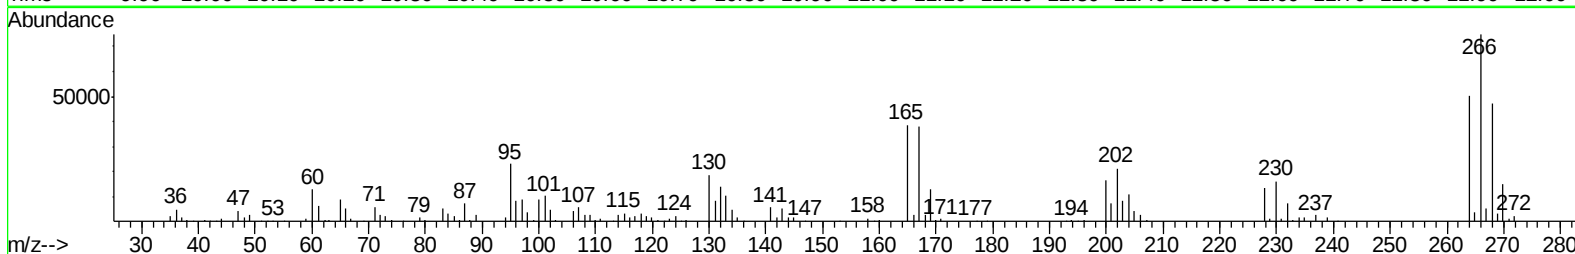


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120315\
Data File : BF083458.D
Acq On : 3 Dec 2015 13:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:37:13 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

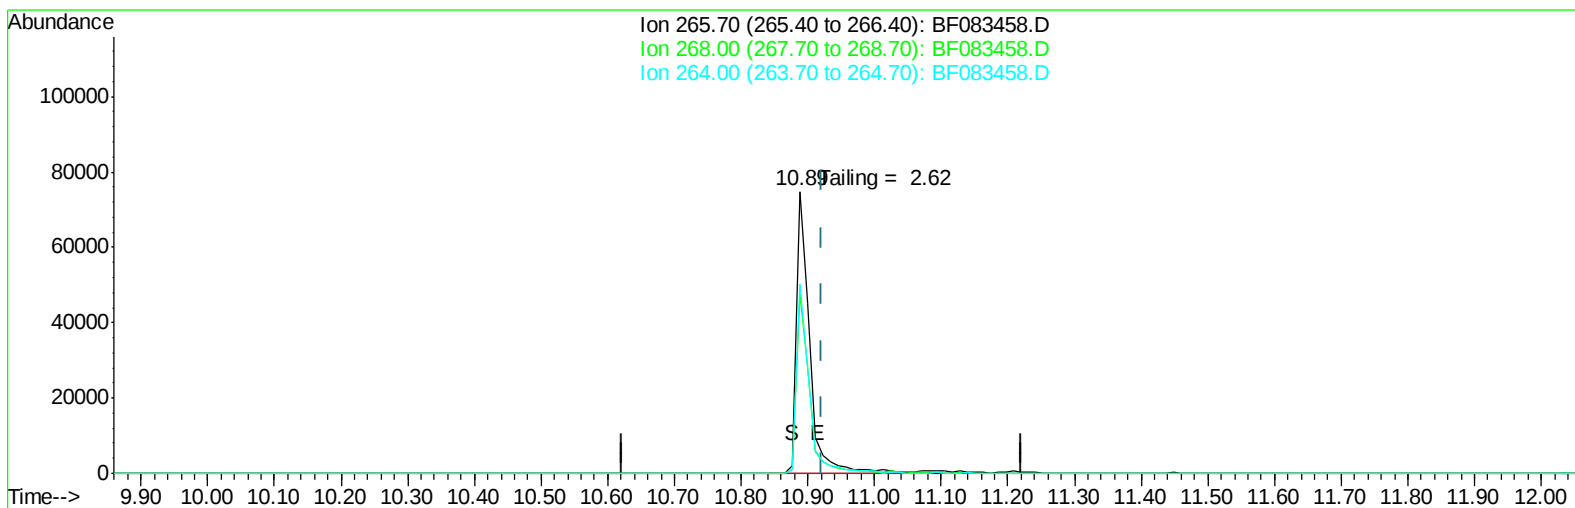

TIC: BF083458.D

(69) Pentachlorophenol (C)




10.888min (-0.034) 0.00ng

response 102843

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.50
264.00	63.00	67.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120315\
 Data File : BF083458.D
 Acq On : 3 Dec 2015 13:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:37:13 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 01:17:16 2015
 Response via : Initial Calibration

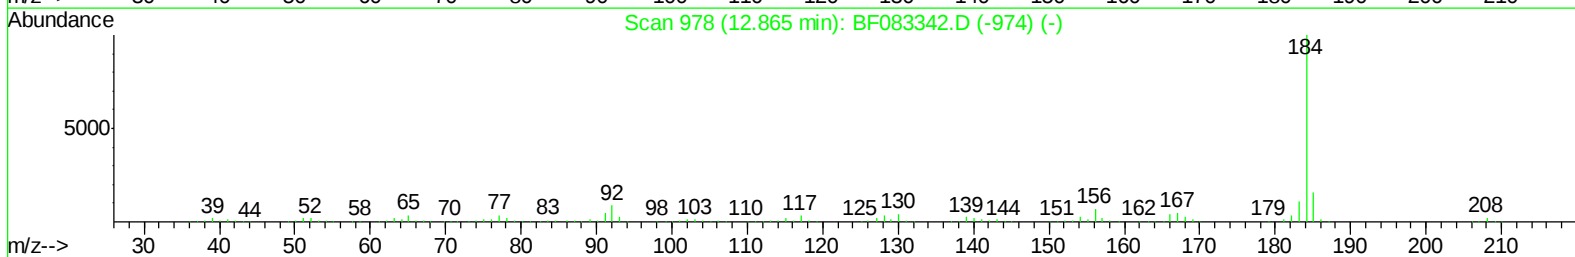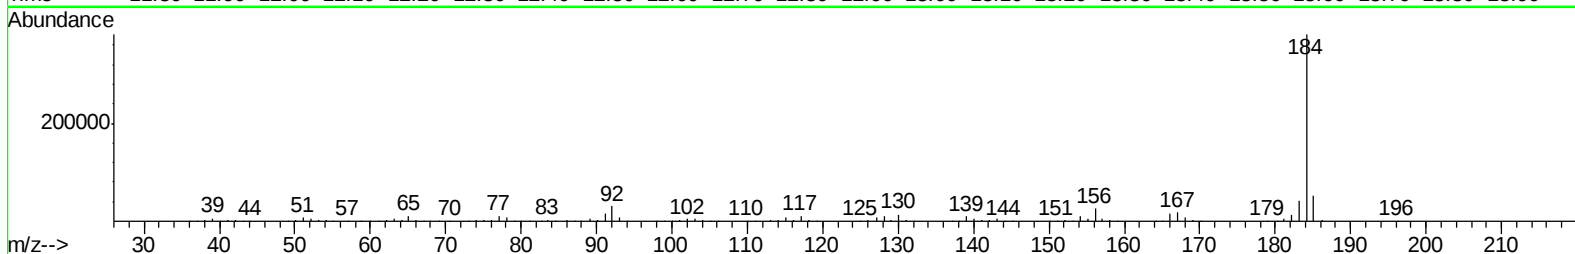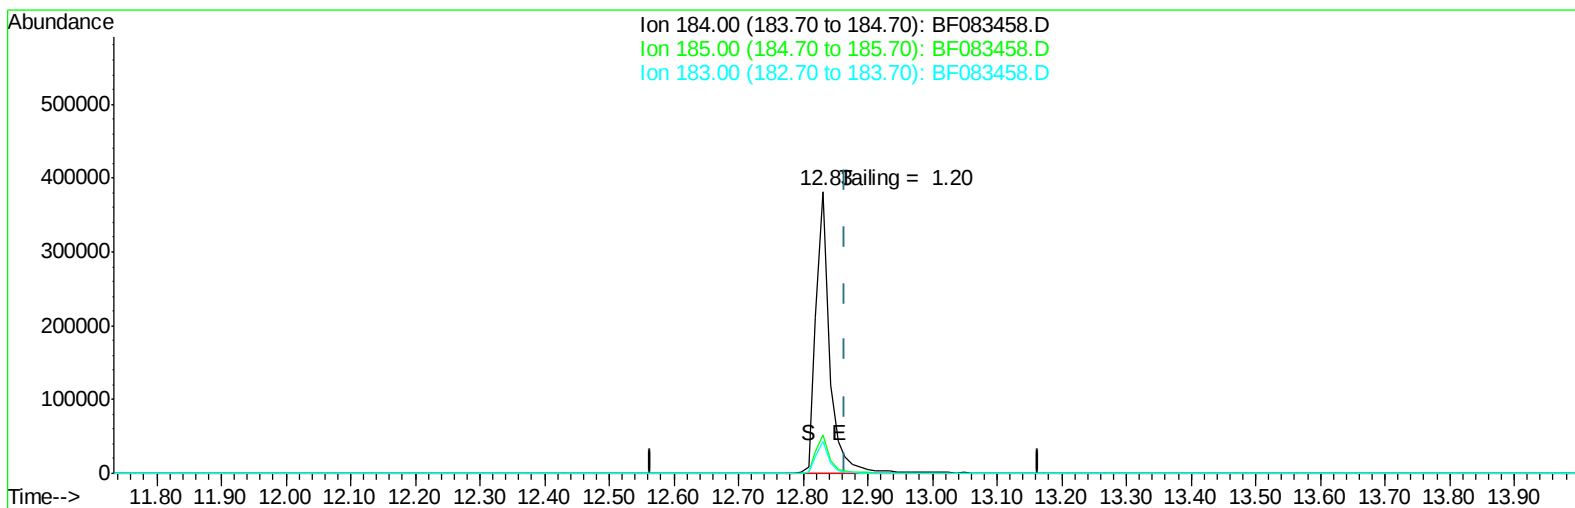

TIC: BF083458.D

(76) Benzidine

12.831min (-0.034) 45825.43ng

response 574628

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.77
183.00	11.20	11.20
0.00	0.00	0.00