

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120315\
Data File : BF083495.D
Acq On : 4 Dec 2015 9:04
Operator : UM/IZ
Sample : G4588-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.624	256	257	274	rVB	287665	569984	10.63%	1.571%
2	5.116	297	300	318	rBV	2374869	2887051	53.84%	7.957%
3	6.202	392	395	400	rBV	2103739	2210424	41.23%	6.093%
4	6.305	402	404	406	rBV	4566433	4656234	86.84%	12.834%
5	6.522	421	423	426	rBV	855173	992494	18.51%	2.736%
6	6.682	435	437	440	rBV	3599241	3763111	70.18%	10.372%
7	7.105	471	474	476	rBV	3318139	3312016	61.77%	9.129%
8	7.813	534	536	539	rBV	1191674	1192213	22.24%	3.286%
9	8.899	628	631	633	rBV	5849461	5361802	100.00%	14.779%
10	9.299	663	666	671	rBV	142292	136314	2.54%	0.376%
11	9.562	687	689	691	rBV	1345253	1243644	23.19%	3.428%
12	9.996	724	727	730	rBV3	39002	59119	1.10%	0.163%
13	10.351	755	758	760	rBV	2716478	2786805	51.98%	7.681%
14	11.094	820	823	826	rBV	1054510	1034881	19.30%	2.852%
15	11.402	848	850	855	rVB	124238	148516	2.77%	0.409%
16	12.477	941	944	948	rBV	64970	99211	1.85%	0.273%
17	13.185	1002	1006	1009	rBV	2946705	4155208	77.50%	11.453%
18	14.705	1136	1139	1146	rBV	676133	882827	16.47%	2.433%
19	16.774	1317	1320	1327	rBV	462218	699345	13.04%	1.928%
20	17.574	1385	1390	1396	rBV5	21667	89757	1.67%	0.247%


Sum of corrected areas: 36280956

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120315\
Data File : BF083495.D
Acq On : 4 Dec 2015 9:04
Operator : UM/IZ
Sample : G4588-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

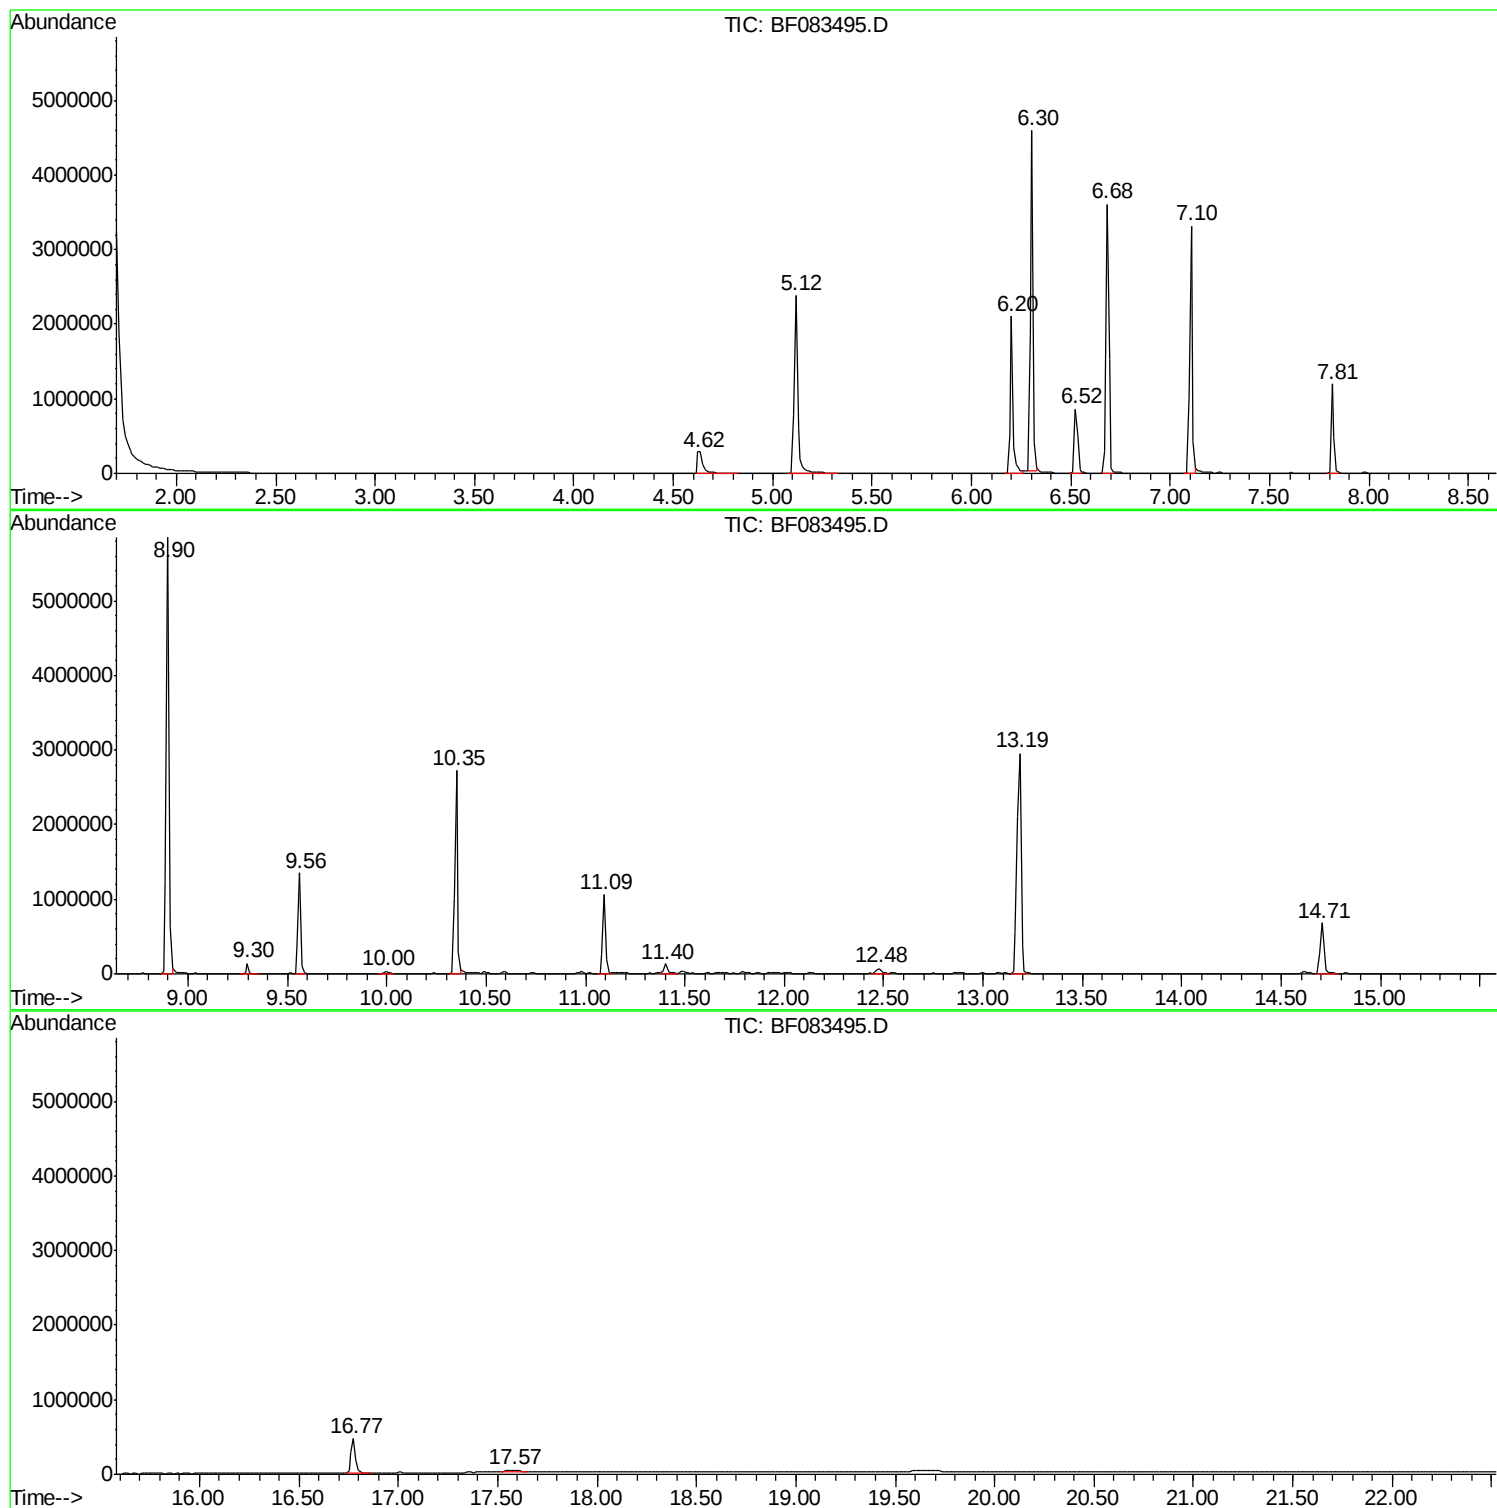

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120315\
Data_File : BF083495.D
Acq_On : 4 Dec 2015 9:044
Operator : UM/IZZ
Sample : G4588-111
Misc :
ALS_Vial : 36 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
MW-13

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
