


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120315\
 Data File : BF083483.D
 Acq On : 4 Dec 2015 2:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 01:17:16 2015

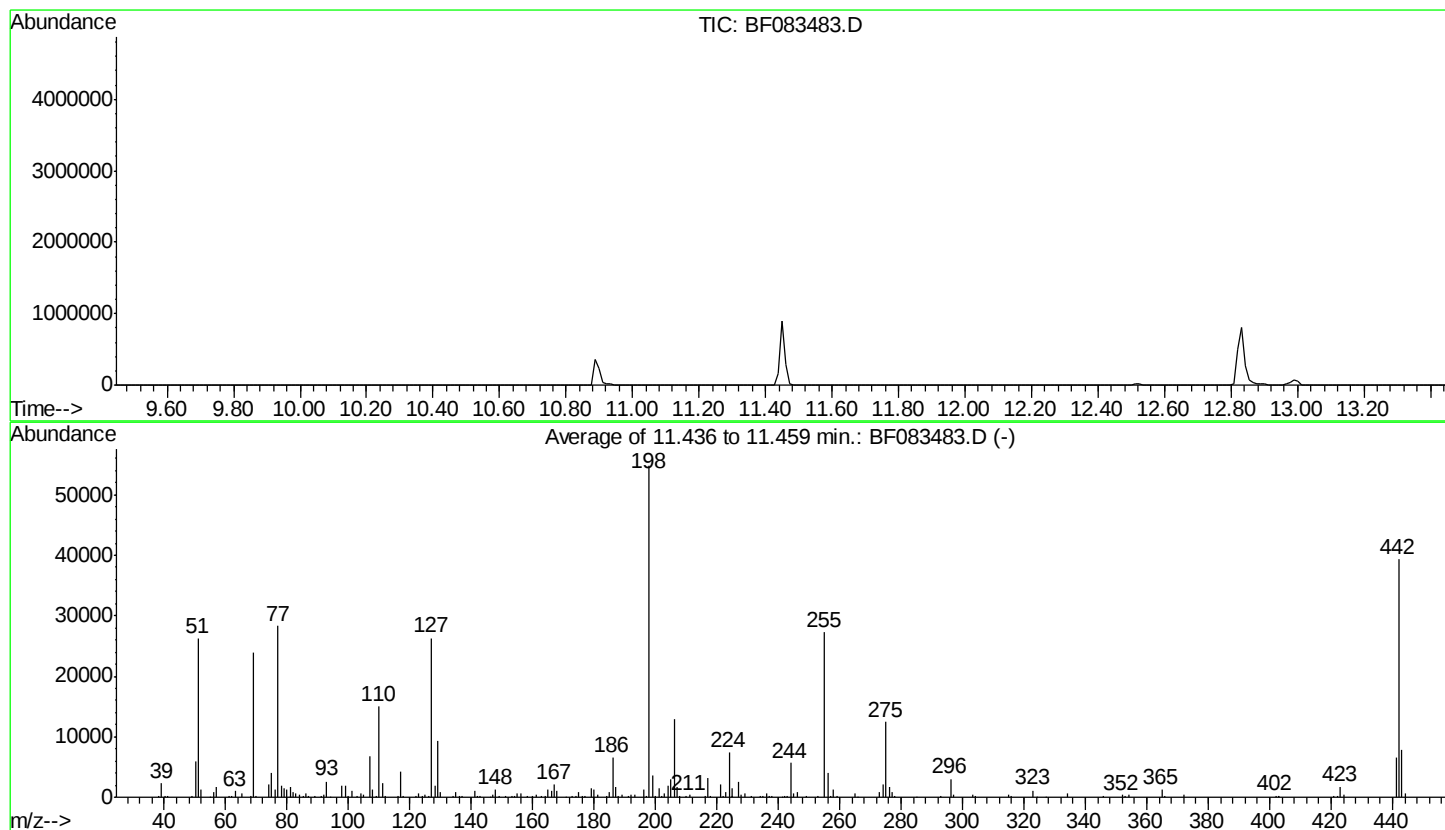

AutoFind: Scans 853, 854, 855; Background Corrected with Scan 850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	26200	PASS
68	69	0.00	2	1.0	228	PASS
69	198	0.00	100	43.4	23817	PASS
70	69	0.00	2	0.5	120	PASS
127	198	10	80	48.0	26303	PASS
197	198	0.00	2	0.4	236	PASS
198	198	100	100	100.0	54820	PASS
199	198	5	9	6.7	3656	PASS
275	198	10	60	22.7	12471	PASS
365	198	1	100	2.2	1181	PASS
441	442	0.01	24	16.9	6633	PASS
442	198	50	100	71.7	39322	PASS
443	442	15	24	20.1	7923	PASS