
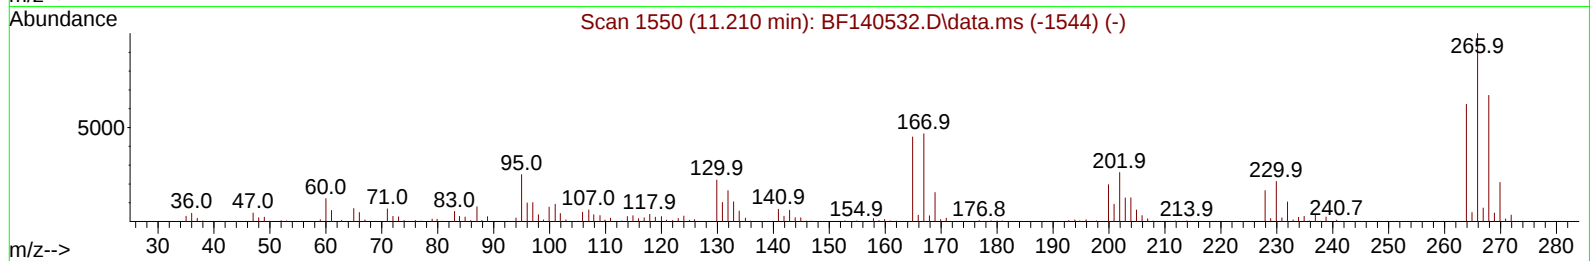
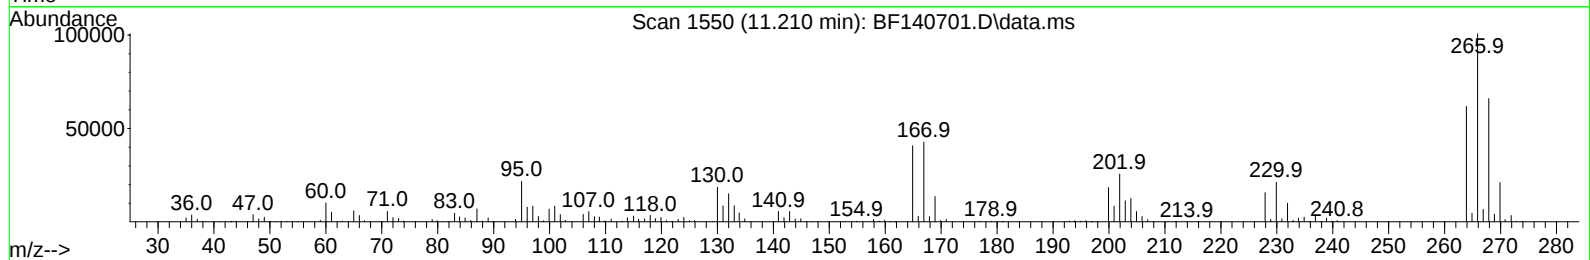


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120324\
Data File : BF140701.D
Acq On : 03 Dec 2024 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 12:35:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

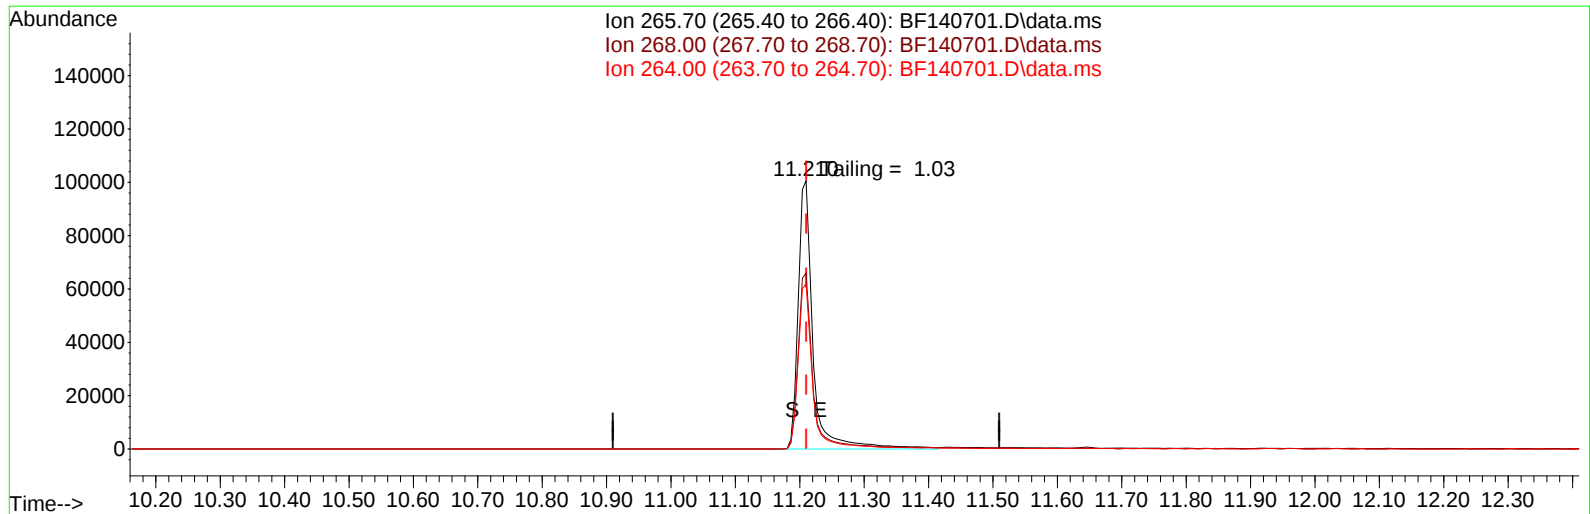

TIC: BF140701.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 13968.96 ng

response 162096

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	65.61
264.00	62.30	61.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120324\
Data File : BF140701.D
Acq On : 03 Dec 2024 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 12:35:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

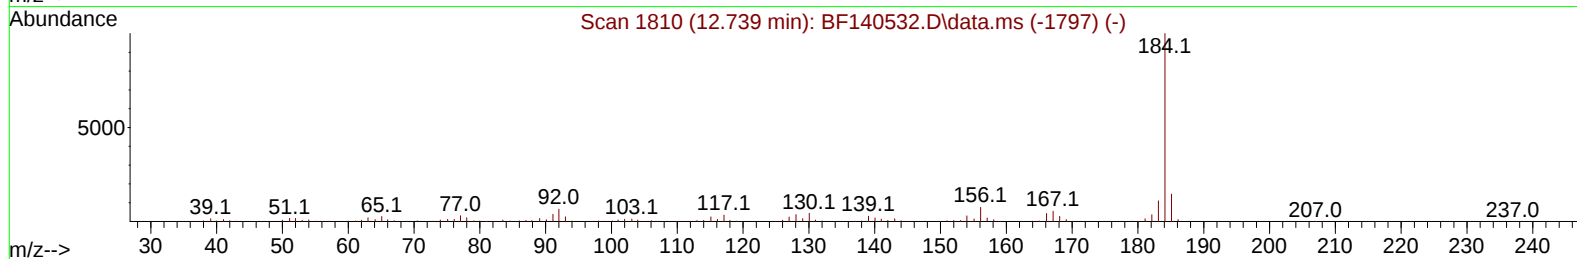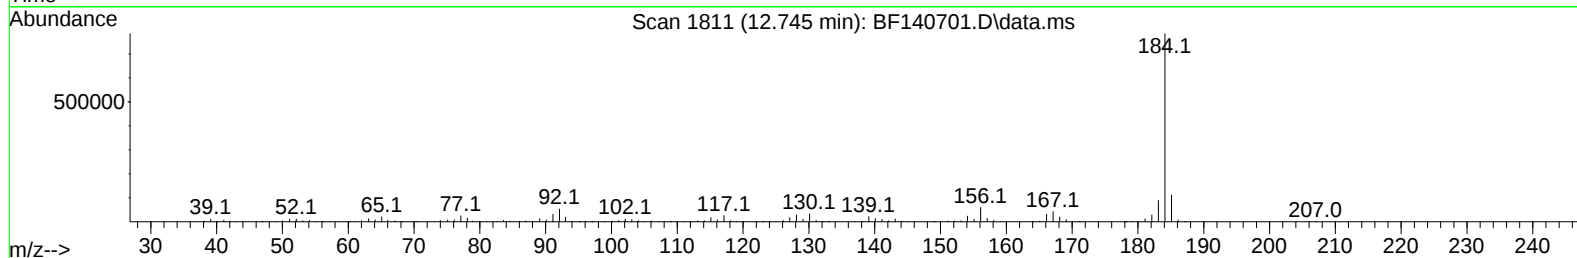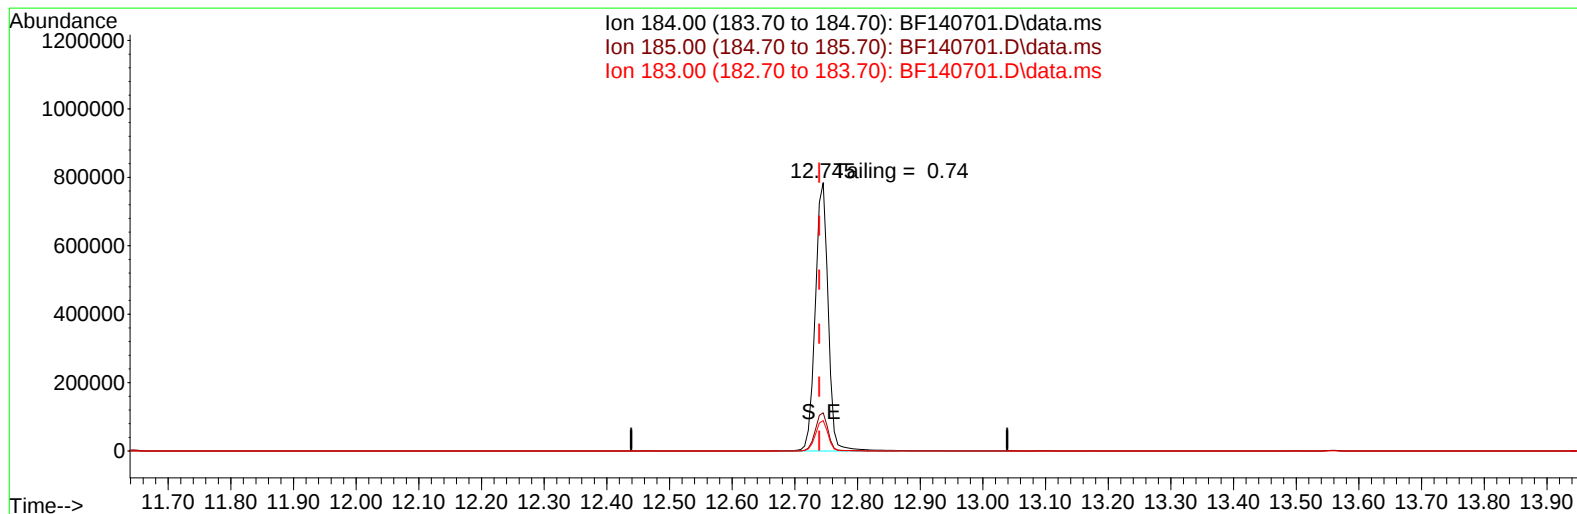

TIC: BF140701.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 19954.27 ng

response 1120287

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.27
183.00	11.00	11.36
0.00	0.00	0.00