
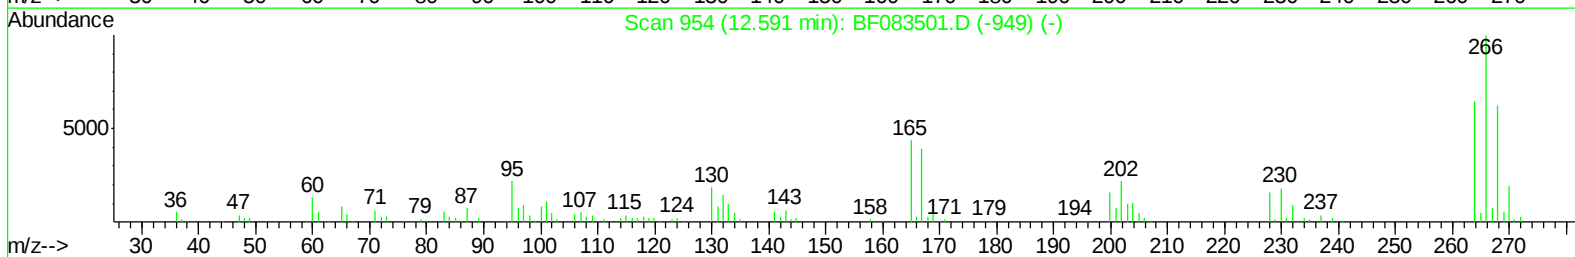
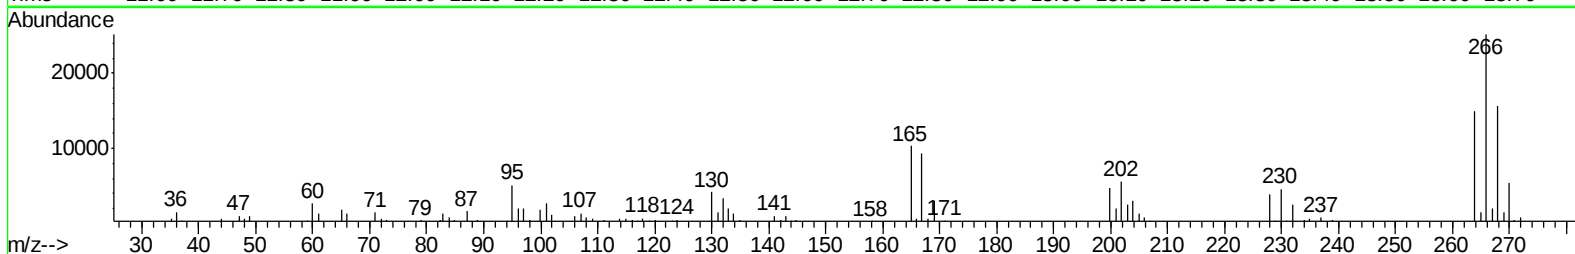


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120415\
Data File : BF083506.D
Acq On : 5 Dec 2015 3:24
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 07:29:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

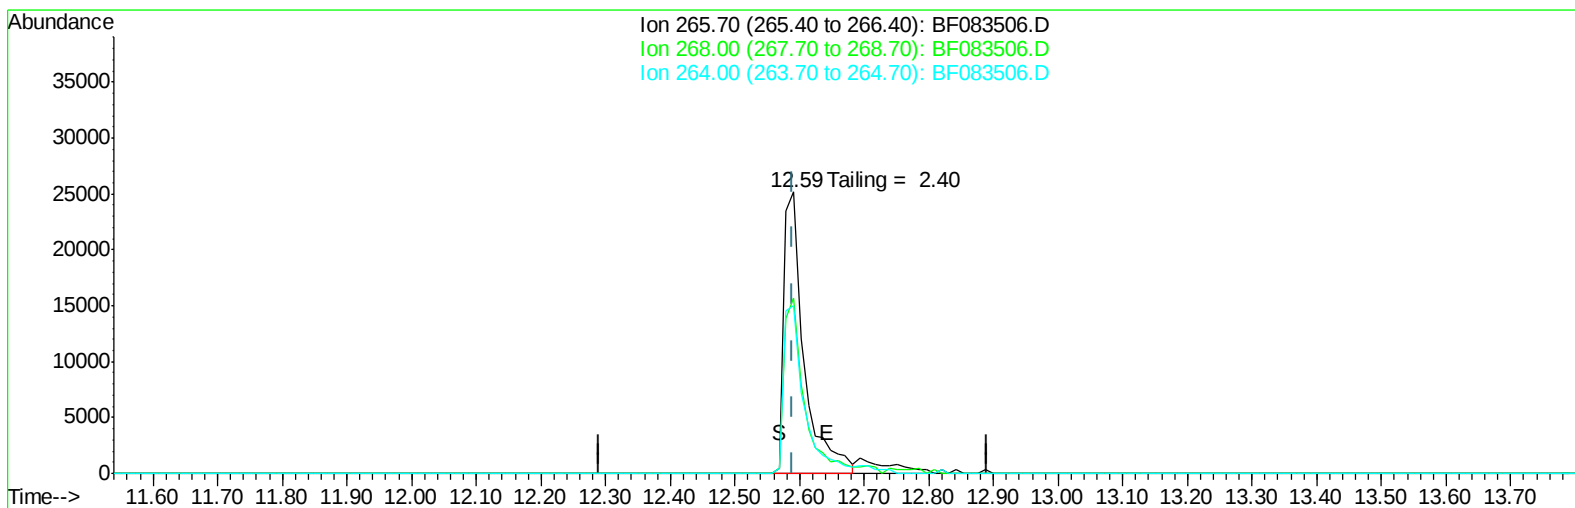

TIC: BF083506.D

(69) Pentachlorophenol (C)




12.591min (+0.001) 0.00ng

response 59576

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	62.24
264.00	64.30	59.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120415\
 Data File : BF083506.D
 Acq On : 5 Dec 2015 3:24
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 07:29:04 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 05 04:12:46 2015
 Response via : Initial Calibration

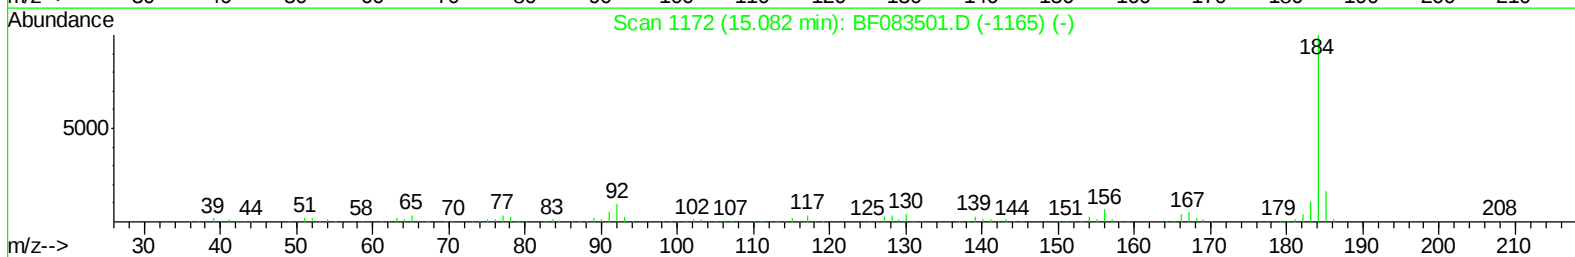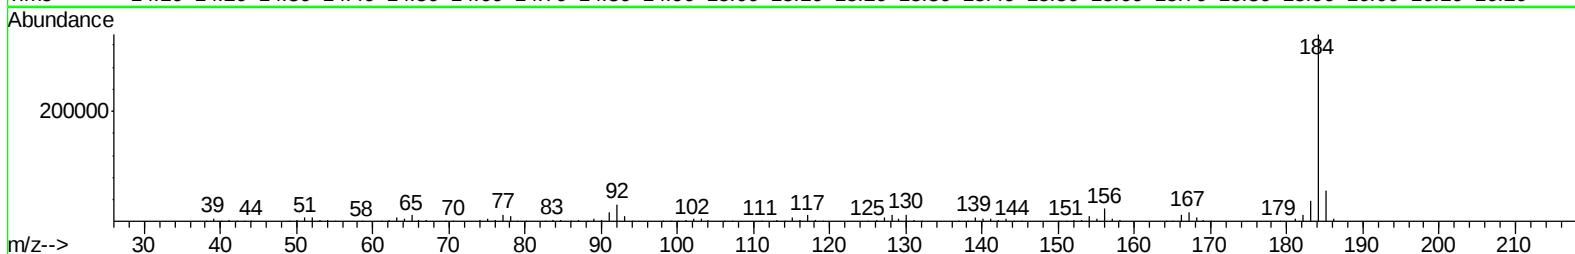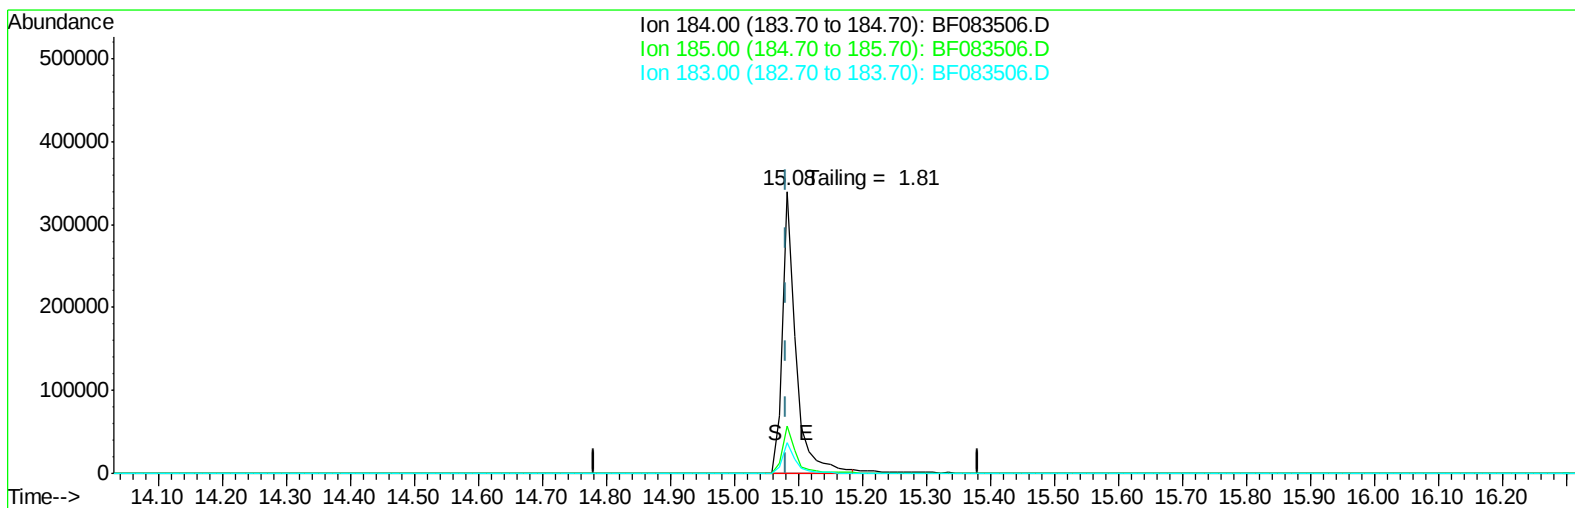

TIC: BF083506.D

(76) Benzidine

15.082min (+0.000) 0.00ng

response 502482

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.72
183.00	11.20	11.14
0.00	0.00	0.00