

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120415\
 Data File : BF083511.D
 Acq On : 5 Dec 2015 13:28
 Operator : UM/IZ
 Sample : G4595-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20151124MGP224BRV139

Quant Time: Dec 07 01:17:02 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 05 04:12:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.77	152	146144	20.00	ng	0.00
21) Naphthalene-d8	7.66	136	575275	20.00	ng	-0.01
38) Acenaphthene-d10	10.45	164	285615	20.00	ng	-0.01
63) Phenanthrene-d10	12.85	188	529687	20.00	ng	0.00
75) Chrysene-d12	17.05	240	420346	20.00	ng	0.00
86) Perylene-d12	18.67	264	339777	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.03	112	548867	56.98	ng	0.00
7) Phenol-d6	5.32	99	443341	33.40	ng	0.00
23) Nitrobenzene-d5	6.59	82	1135087	92.23	ng	-0.01
41) 2,4,6-Tribromophenol	11.74	330	348438	132.25	ng	-0.01
44) 2-Fluorobiphenyl	9.41	172	1785768	84.80	ng	-0.01
78) Terphenyl-d14	15.49	244	1782658	94.37	ng	0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120415\
Data File : BF083511.D
Acq On : 5 Dec 2015 13:28
Operator : UM/IZ
Sample : G4595-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20151124MGP224BRV139

Quant Time: Dec 07 01:17:02 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

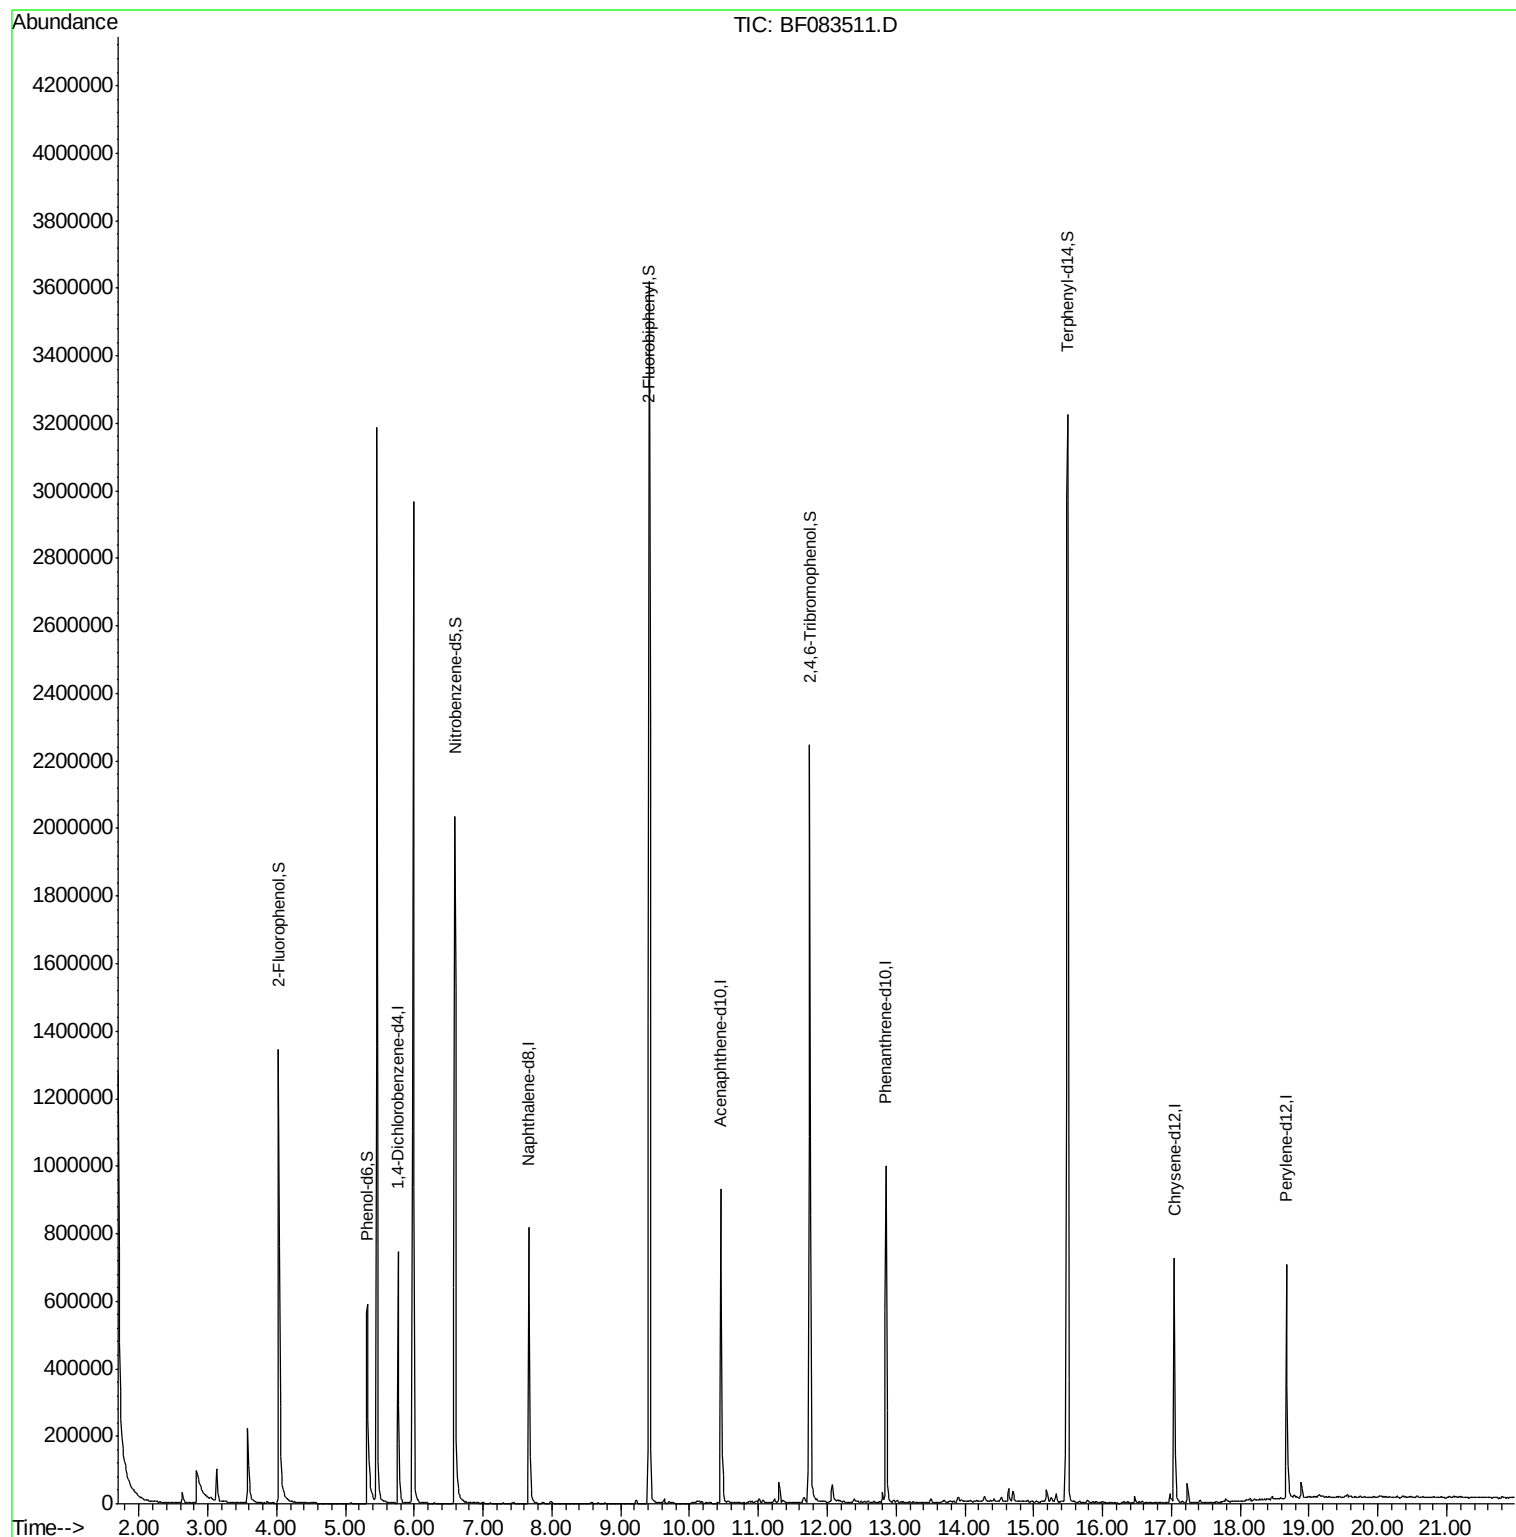

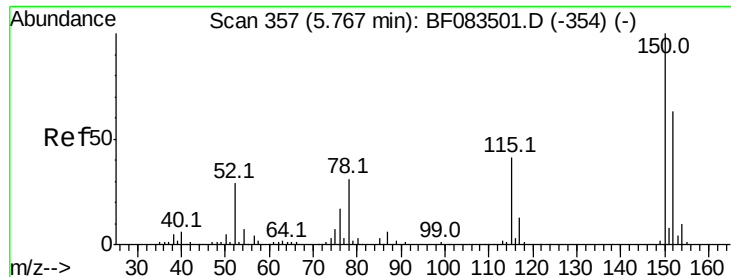


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.77 min Scan# 357
Delta R.T. 0.00 min
Lab File: BF083511.D
Acq: 5 Dec 2015 13:28

Instrument :
BNA_F
ClientSampleId :
20151124MGP224BRV139

Tot Ion:152 Resp: 146144
Ion Ratio Lower Upper
152 100
150 156.9 126.5 189.7
115 63.6 52.3 78.5

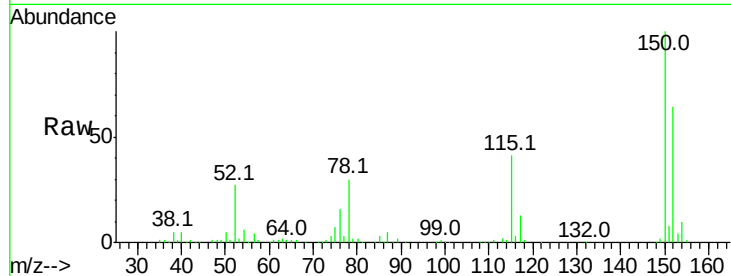


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

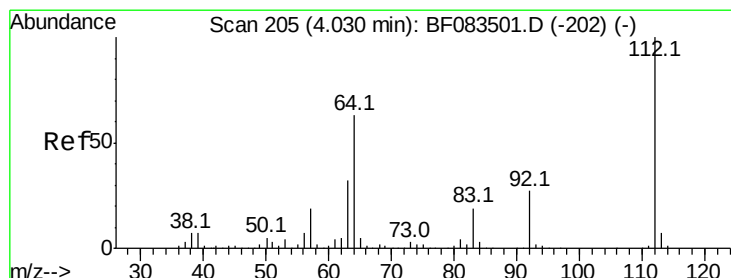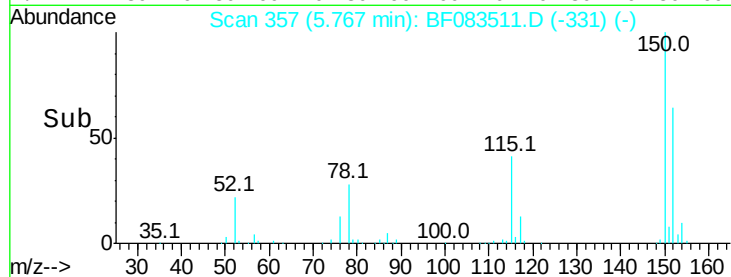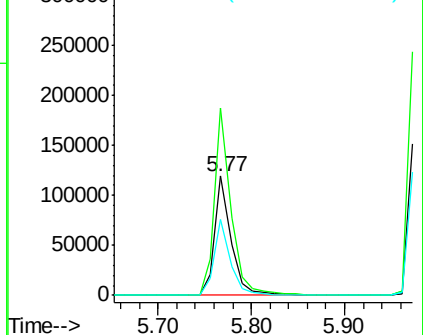



#5


2-Fluorophenol
Concen: 56.98 ng
RT: 4.03 min Scan# 205
Delta R.T. 0.00 min
Lab File: BF083511.D
Acq: 5 Dec 2015 13:28

Tgt Ion:112 Resp: 548867
Ion Ratio Lower Upper
112 100
64 69.6 50.5 75.7
63 35.2 25.8 38.6

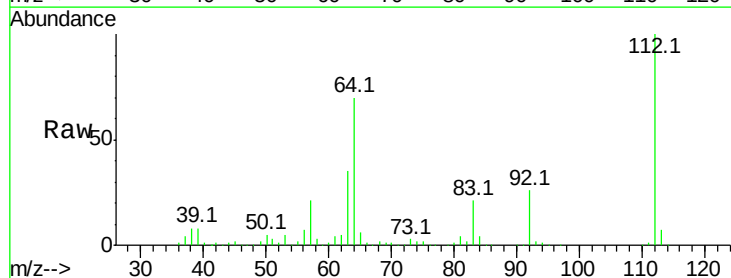

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

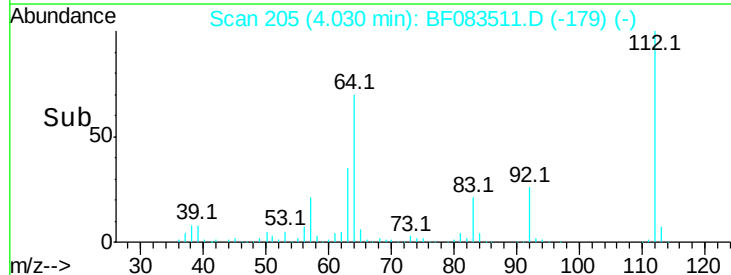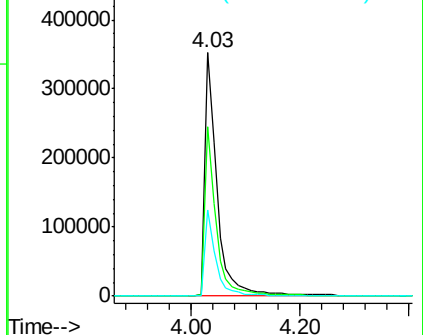

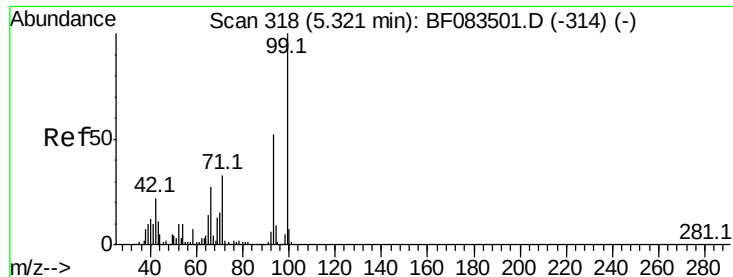

#7

Phenol-d6

Concen: 33.40 ng

RT: 5.32 min Scan# 318

Delta R.T. 0.00 min

Lab File: BF083511.D

Acq: 5 Dec 2015 13:28

Instrument :

BNA_F

ClientSampleId :

20151124MGP224BRV139





Tot Ion: 99 Resp: 443341

Ion Ratio Lower Upper

99 100

42 18.0 17.3 25.9

71 31.3 26.6 40.0

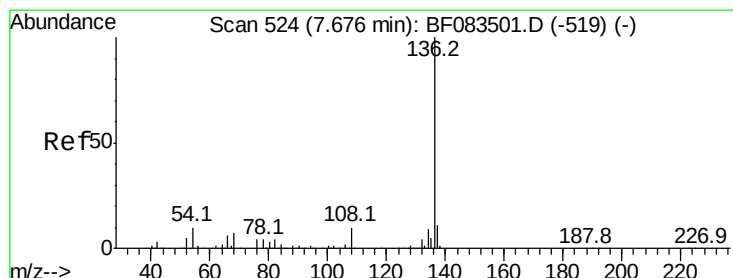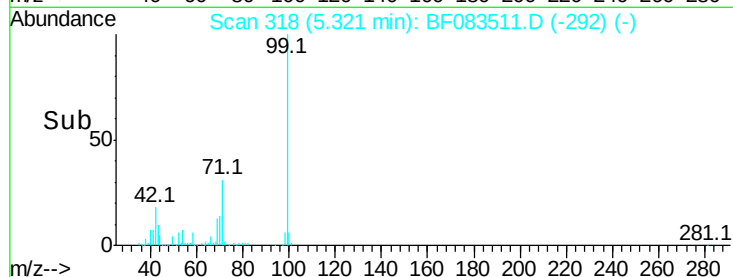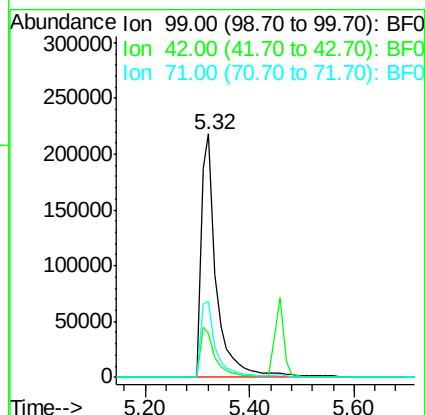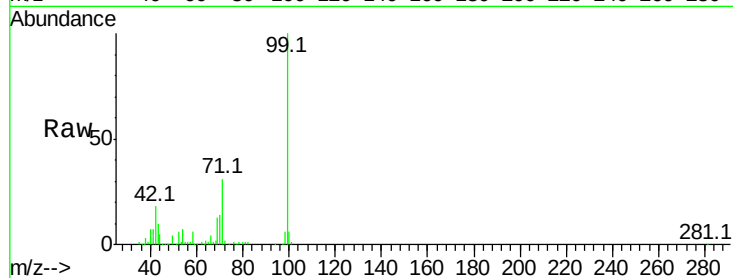

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.66 min Scan# 523

Delta R.T. -0.01 min

Lab File: BF083511.D

Acq: 5 Dec 2015 13:28

Tgt Ion: 136 Resp: 575275




Ion Ratio Lower Upper


136 100

137 10.9 8.7 13.1

54 11.5 7.8 11.6

68 8.0 5.7 8.5

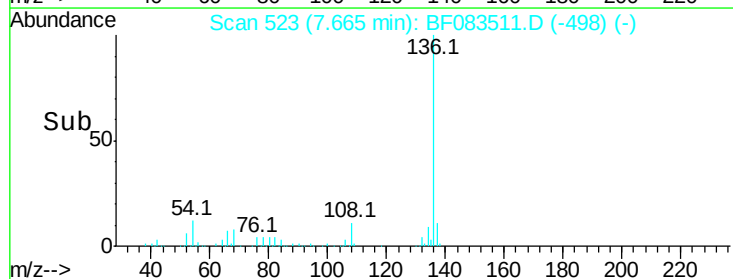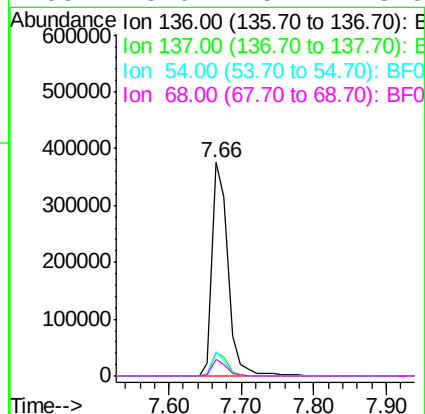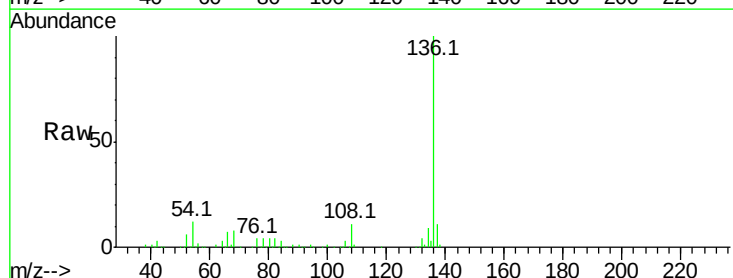




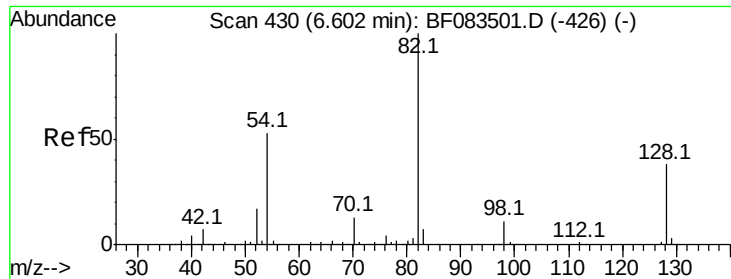


#23
 Nitrobenzene-d5
 Concen: 92.23 ng
 RT: 6.59 min Scan# 429
 Delta R.T. -0.01 min
 Lab File: BF083511.D
 Acq: 5 Dec 2015 13:28

Instrument :
 BNA_F
 ClientSampleId :
 20151124MGP224BRV139

Tot Ion: 82 Resp: 1135087




Ion	Ratio	Lower	Upper
82	100		
128	36.8	30.7	46.1
54	55.2	42.5	63.7

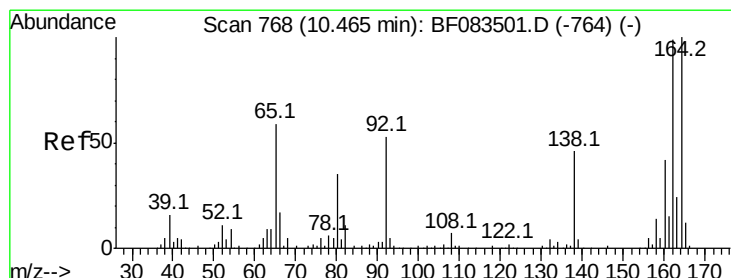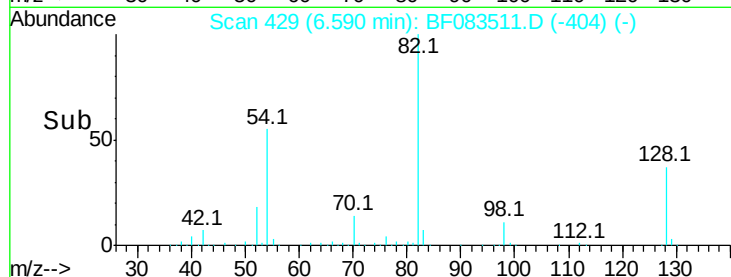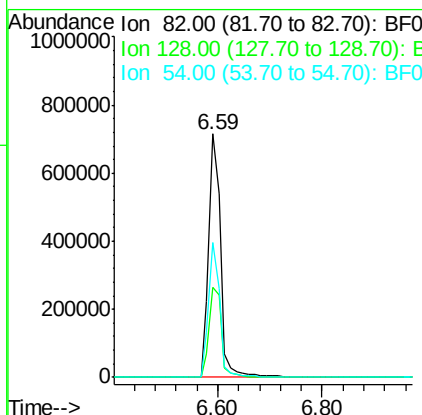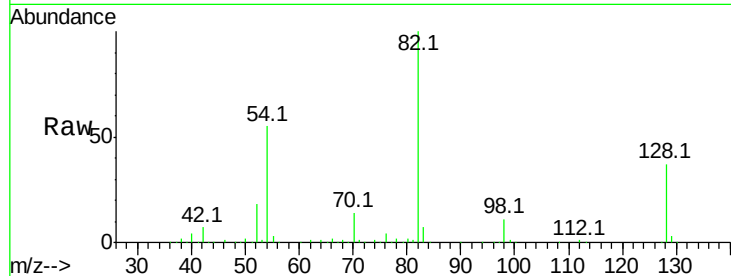


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.45 min Scan# 767
 Delta R.T. -0.01 min
 Lab File: BF083511.D
 Acq: 5 Dec 2015 13:28

Tgt Ion: 164 Resp: 285615

Ion	Ratio	Lower	Upper
164	100		
162	99.3	78.8	118.2
160	43.0	33.4	50.2

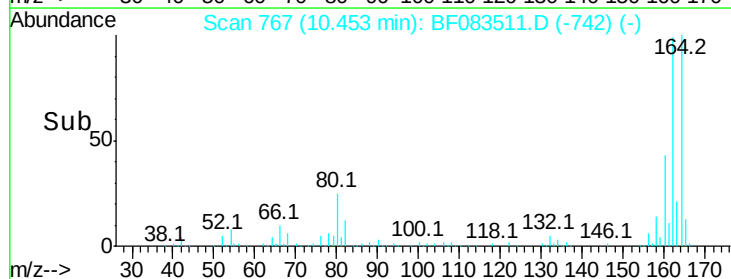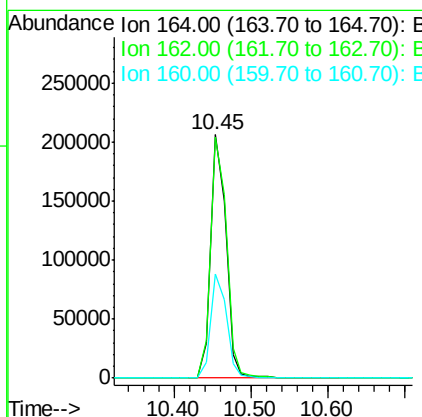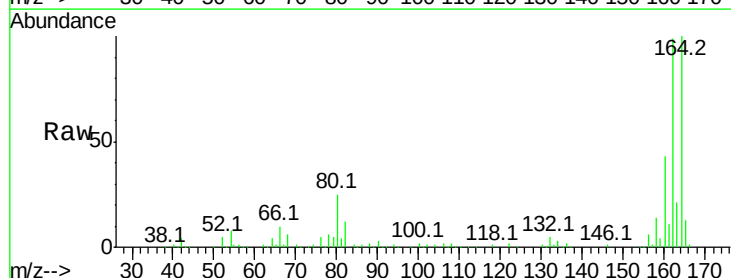


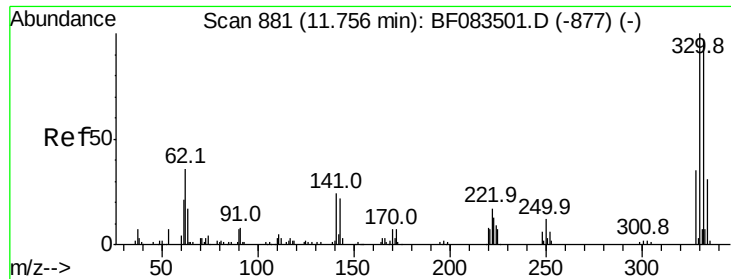




#41
 2,4,6-Tribromophenol
 Concen: 132.25 ng
 RT: 11.74 min Scan# 880
 Delta R.T. -0.01 min
 Lab File: BF083511.D
 Acq: 5 Dec 2015 13:28

Instrument :
 BNA_F
 ClientSampleId :
 20151124MGP224BRV139

Tot Ion:330 Resp: 348438
 Ion Ratio Lower Upper
 330 100
 332 98.4 0.0 0.0#
 141 37.9 0.0 0.0#

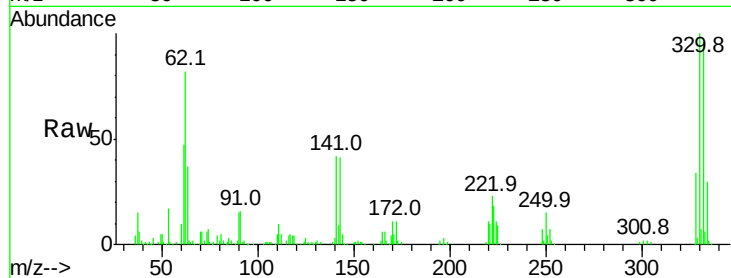


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

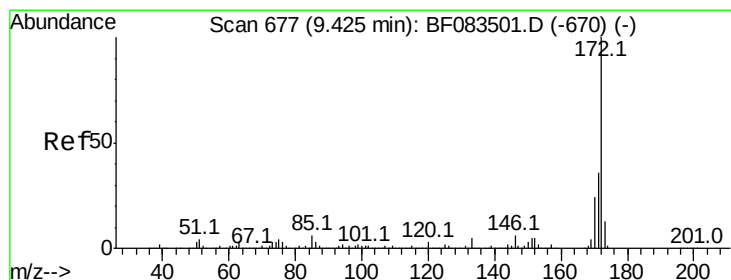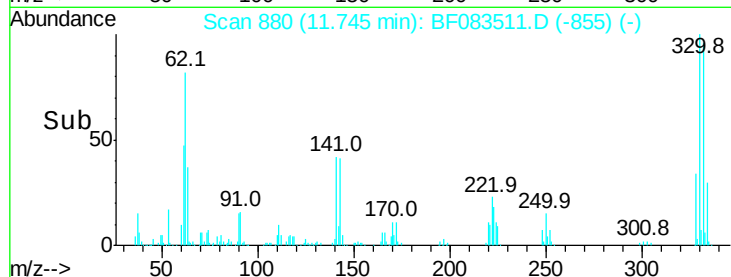
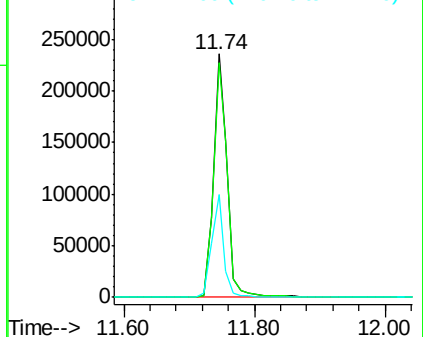



#44
 2-Fluorobiphenyl
 Concen: 84.80 ng
 RT: 9.41 min Scan# 676
 Delta R.T. -0.01 min
 Lab File: BF083511.D
 Acq: 5 Dec 2015 13:28

Tgt Ion:172 Resp: 1785768
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.6 42.8
 170 24.9 19.4 29.0

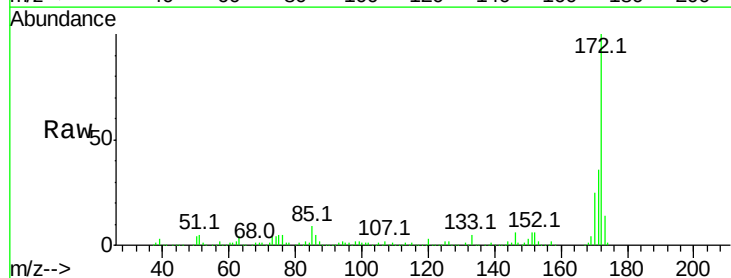

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

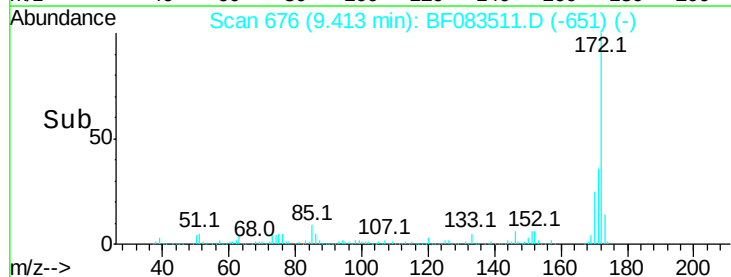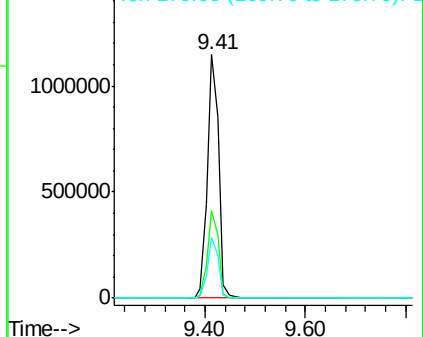


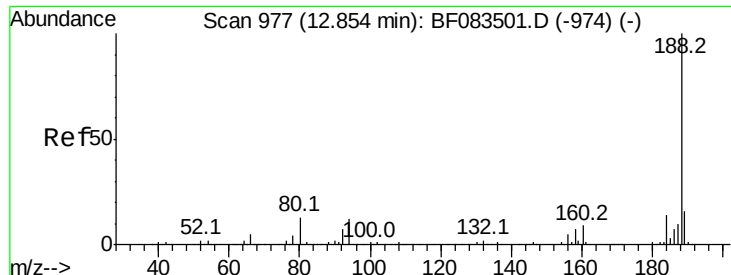




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.85 min Scan# 977
Delta R.T. 0.00 min
Lab File: BF083511.D
Acq: 5 Dec 2015 13:28

Instrument :
BNA_F
ClientSampleId :
20151124MGP224BRV139

Tot Ion:188 Resp: 529687
Ion Ratio Lower Upper
188 100
94 9.6 9.4 14.2
80 11.2 10.6 16.0

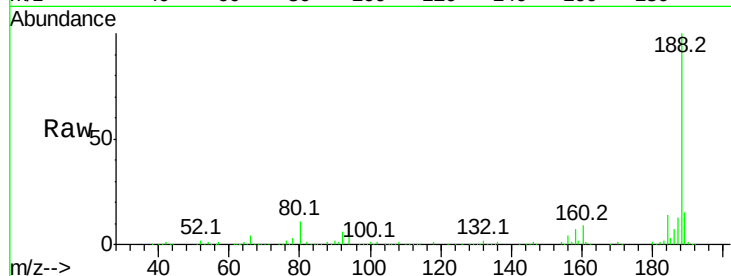


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

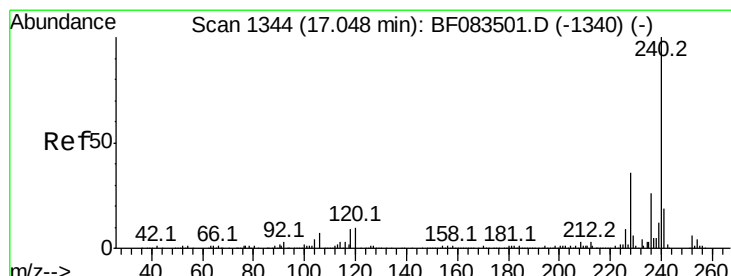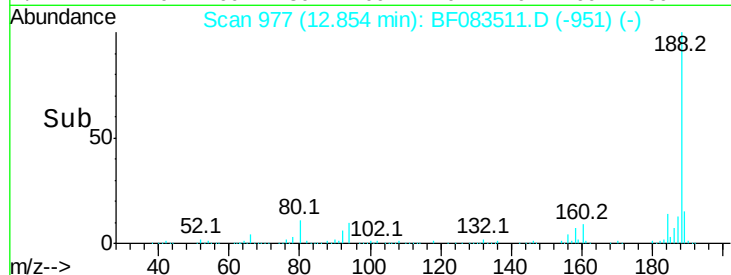
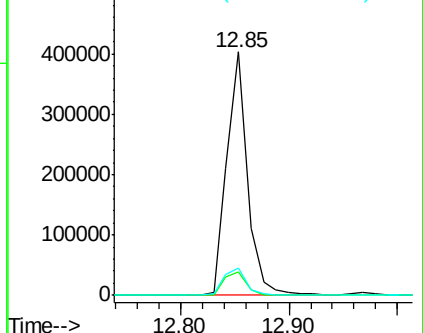



#75
Chrysene-d12
Concen: 20.00 ng
RT: 17.05 min Scan# 1344
Delta R.T. 0.00 min
Lab File: BF083511.D
Acq: 5 Dec 2015 13:28

Tgt Ion:240 Resp: 420346
Ion Ratio Lower Upper
240 100
120 9.3 8.1 12.1
236 25.6 20.8 31.2

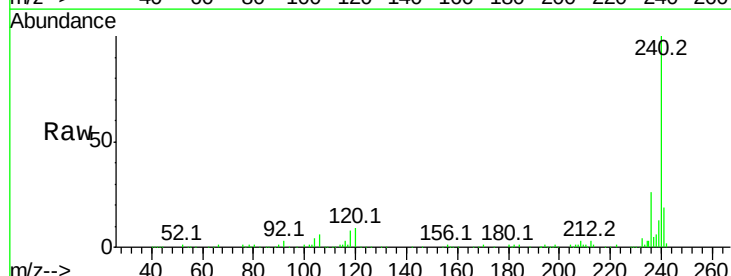

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

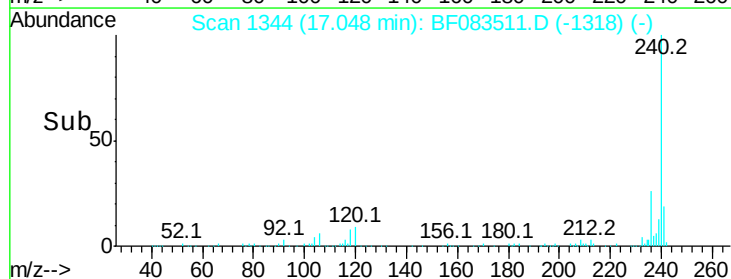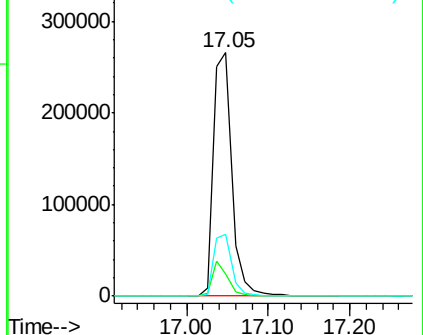

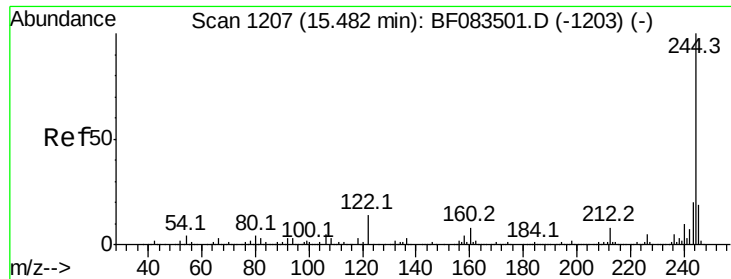

#78

Terphenyl-d14

Concen: 94.37 ng

RT: 15.49 min Scan# 1208

Delta R.T. 0.01 min

Lab File: BF083511.D

Acq: 5 Dec 2015 13:28

Instrument :

BNA_F

ClientSampleId :

20151124MGP224BRV139


Tot Ion:244 Resp: 1782658

Ion Ratio Lower Upper




244 100

212 7.3 6.1 9.1

122 10.9 11.0 16.6#

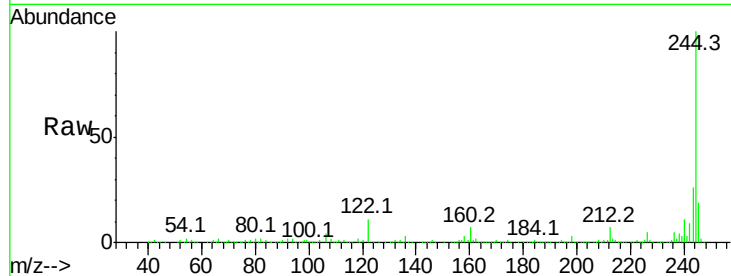

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

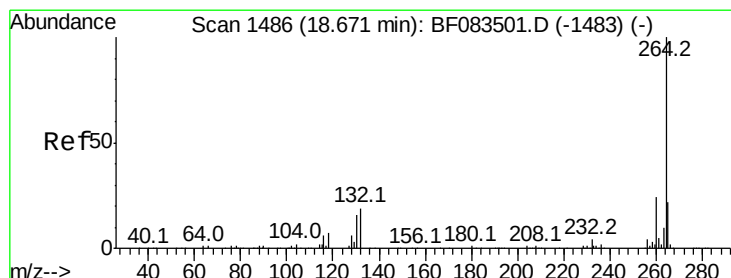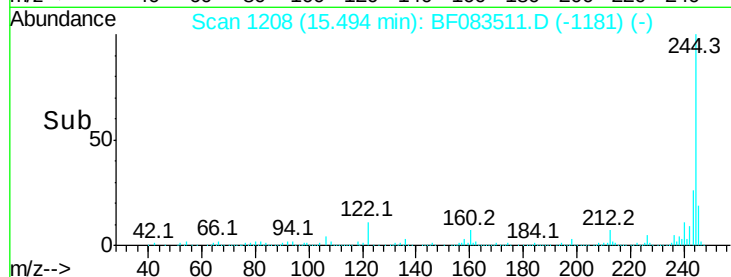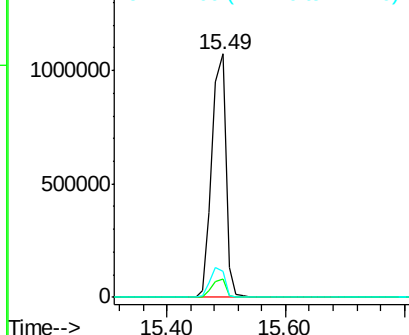

#86

Perylene-d12

Concen: 20.00 ng

RT: 18.67 min Scan# 1486

Delta R.T. 0.00 min

Lab File: BF083511.D

Acq: 5 Dec 2015 13:28


Tgt Ion:264 Resp: 339777

Ion Ratio Lower Upper

264 100

260 22.5 19.4 29.0

265 21.2 17.8 26.6

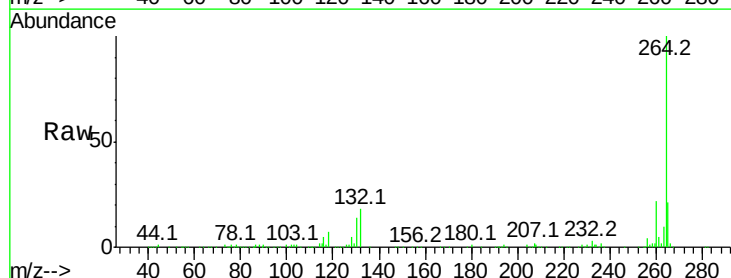

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

