


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120415\
 Data File : BF083497.D
 Acq On : 4 Dec 2015 22:54
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 05 04:12:46 2015

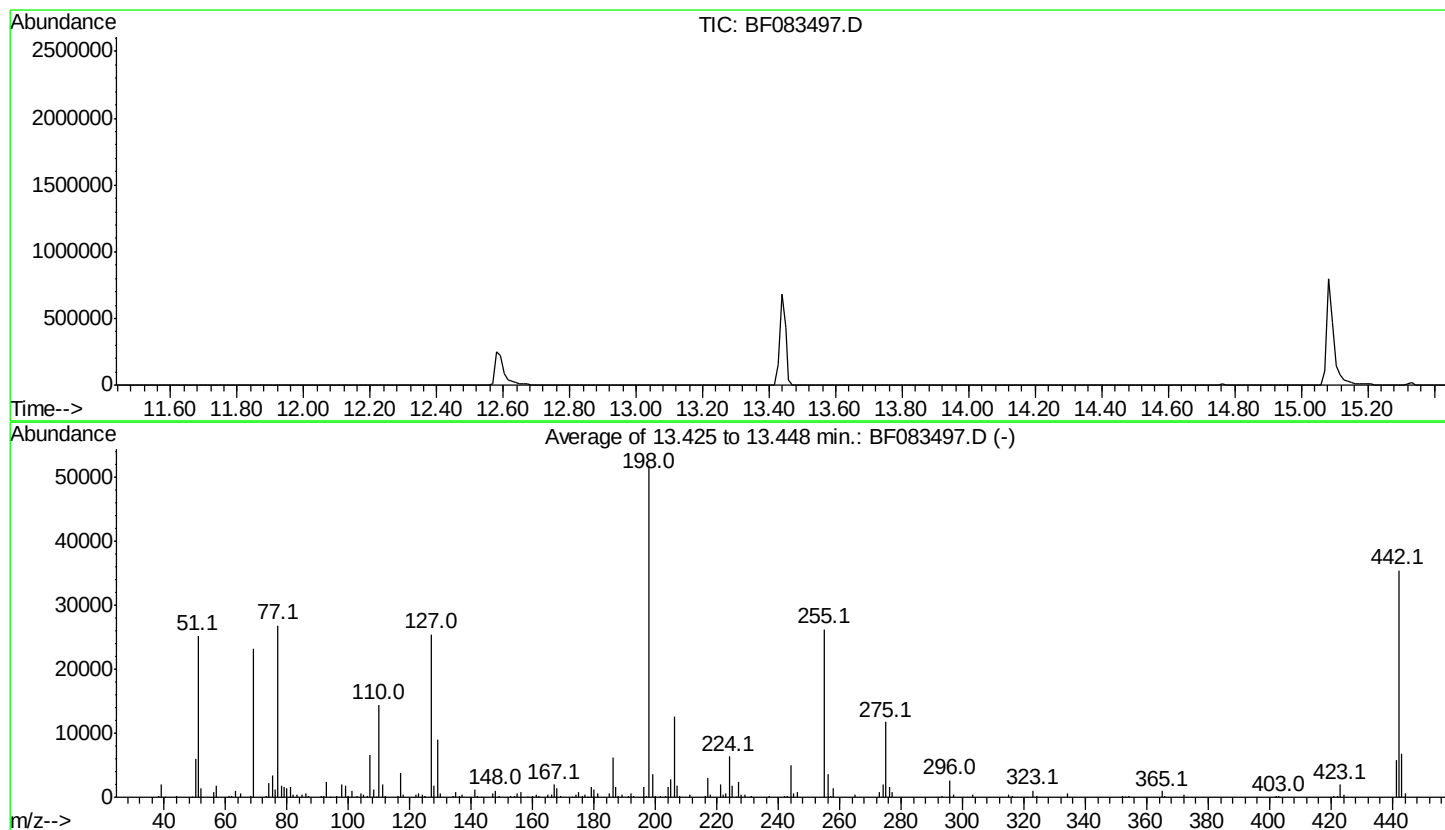

AutoFind: Scans 1027, 1028, 1029; Background Corrected with Scan 1023

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	25310	PASS
68	69	0.00	2	0.9	209	PASS
69	198	0.00	100	44.9	23272	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	25468	PASS
197	198	0.00	2	0.3	174	PASS
198	198	100	100	100.0	51882	PASS
199	198	5	9	6.8	3551	PASS
275	198	10	60	22.7	11762	PASS
365	198	1	100	1.9	989	PASS
441	442	0.01	24	16.6	5897	PASS
442	198	50	100	68.4	35463	PASS
443	442	15	24	19.2	6800	PASS