


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120415\
 Data File : BF083506.D
 Acq On : 5 Dec 2015 3:24
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 05 04:12:46 2015

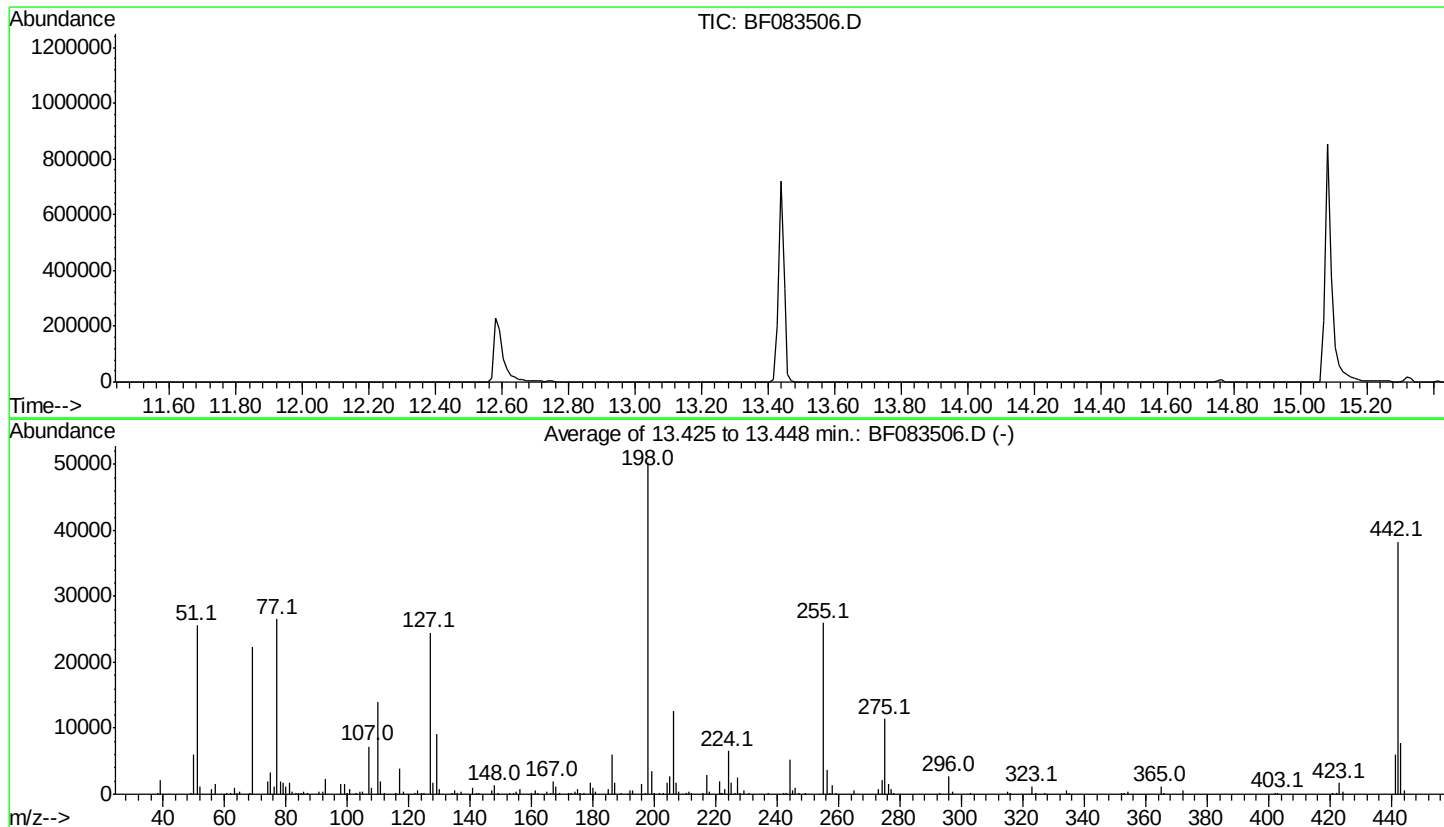

AutoFind: Scans 1027, 1028, 1029; Background Corrected with Scan 1023

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	25554	PASS
68	69	0.00	2	0.9	207	PASS
69	198	0.00	100	44.4	22306	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	24548	PASS
197	198	0.00	2	0.4	177	PASS
198	198	100	100	100.0	50261	PASS
199	198	5	9	7.1	3589	PASS
275	198	10	60	22.6	11364	PASS
365	198	1	100	2.3	1149	PASS
441	442	0.01	24	15.6	5985	PASS
442	198	50	100	76.1	38245	PASS
443	442	15	24	20.1	7681	PASS