


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120415\
 Data File : BF083513.D
 Acq On : 5 Dec 2015 14:27
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 05 04:12:46 2015

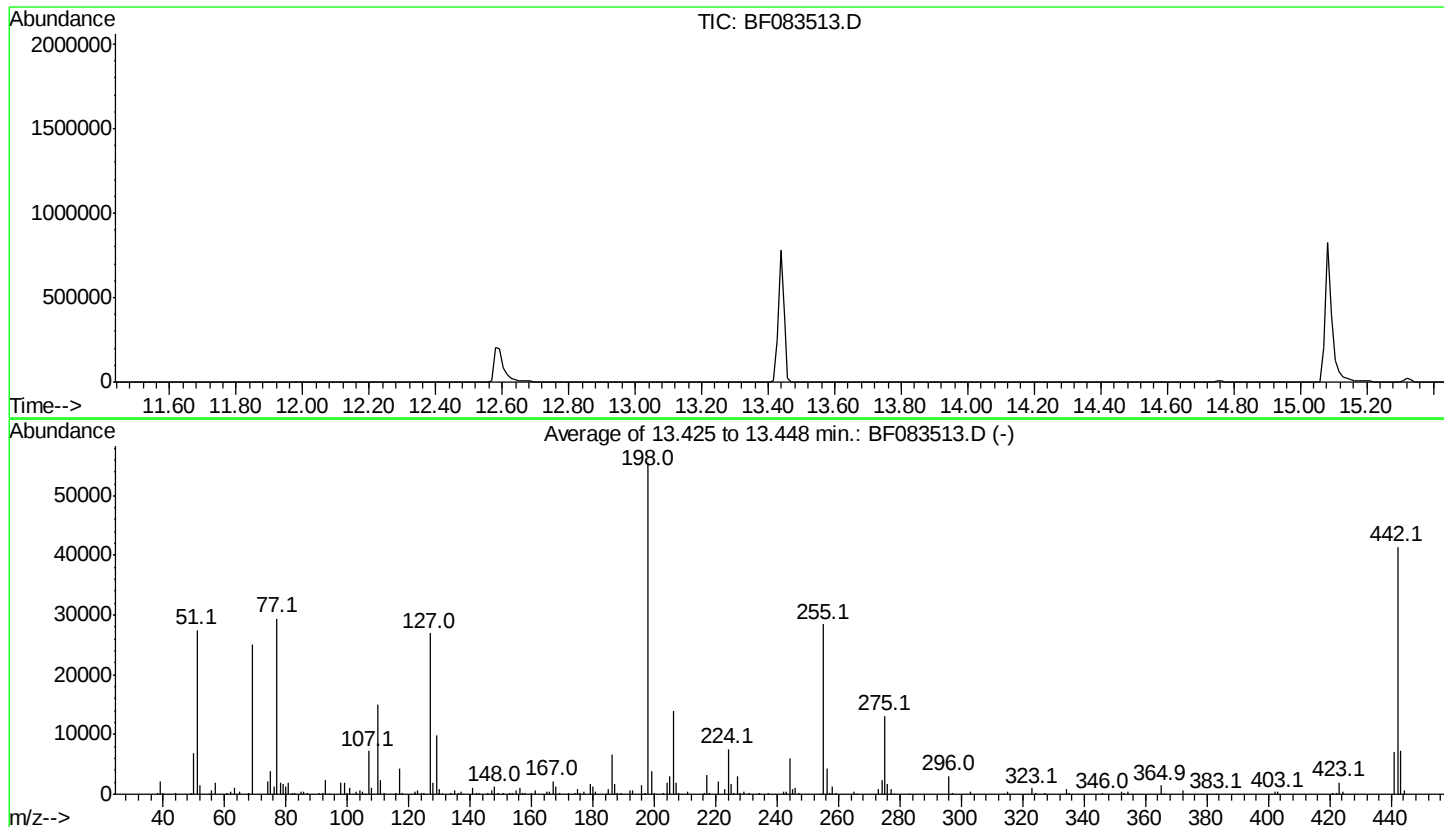

AutoFind: Scans 1027, 1028, 1029; Background Corrected with Scan 1023

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	27476	PASS
68	69	0.00	2	1.2	307	PASS
69	198	0.00	100	45.1	25049	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	27007	PASS
197	198	0.00	2	0.3	176	PASS
198	198	100	100	100.0	55544	PASS
199	198	5	9	6.8	3803	PASS
275	198	10	60	23.7	13137	PASS
365	198	1	100	2.5	1402	PASS
441	442	0.01	24	17.2	7124	PASS
442	198	50	100	74.6	41445	PASS
443	442	15	24	17.7	7347	PASS