


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120417\
 Data File : BF101085.D
 Acq On : 4 Dec 2017 9:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 04 13:07:49 2017

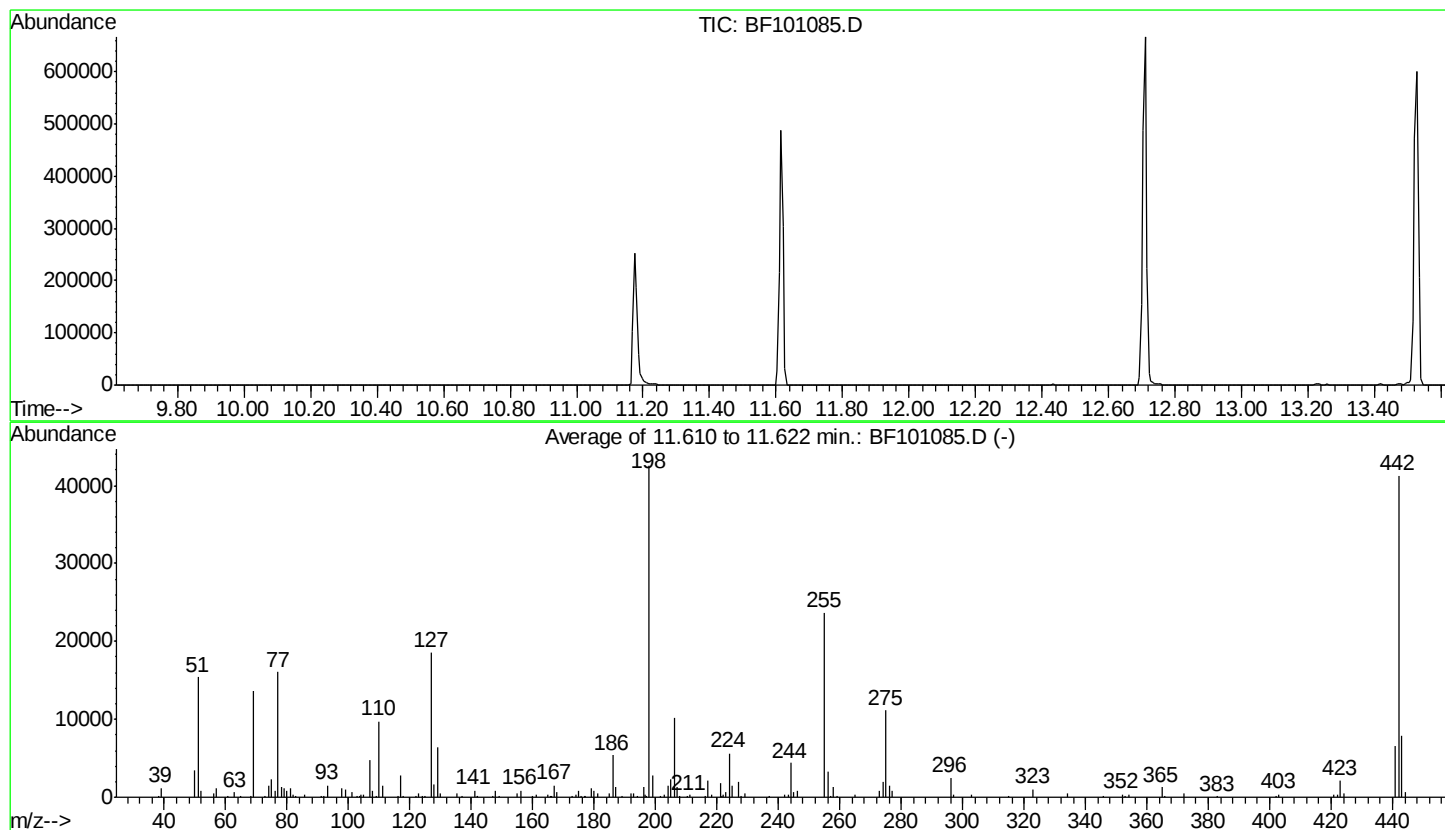

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	15388	PASS
68	69	0.00	2	1.2	170	PASS
69	198	0.00	100	32.2	13712	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	18563	PASS
197	198	0.00	2	0.8	330	PASS
198	198	100	100	100.0	42554	PASS
199	198	5	9	6.5	2776	PASS
275	198	10	60	26.1	11104	PASS
365	198	1	100	3.0	1256	PASS
441	443	0.01	100	84.1	6636	PASS
442	198	50	100	96.9	41247	PASS
443	442	15	24	19.1	7888	PASS