
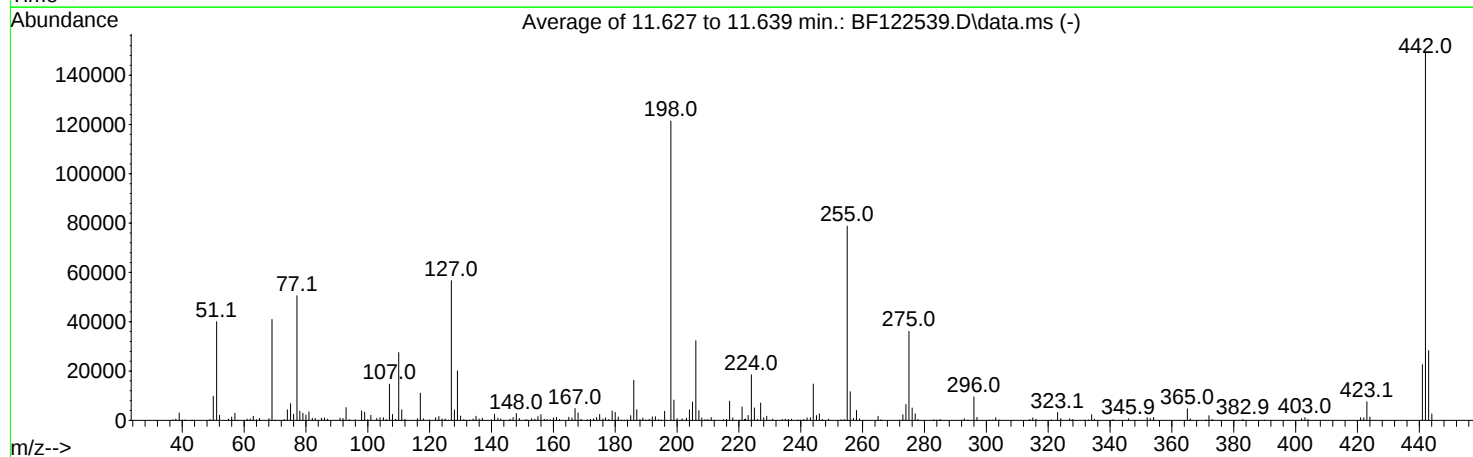


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120420\
 Data File : BF122539.D
 Acq On : 4 Dec 2020 10:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 04 12:52:10 2020

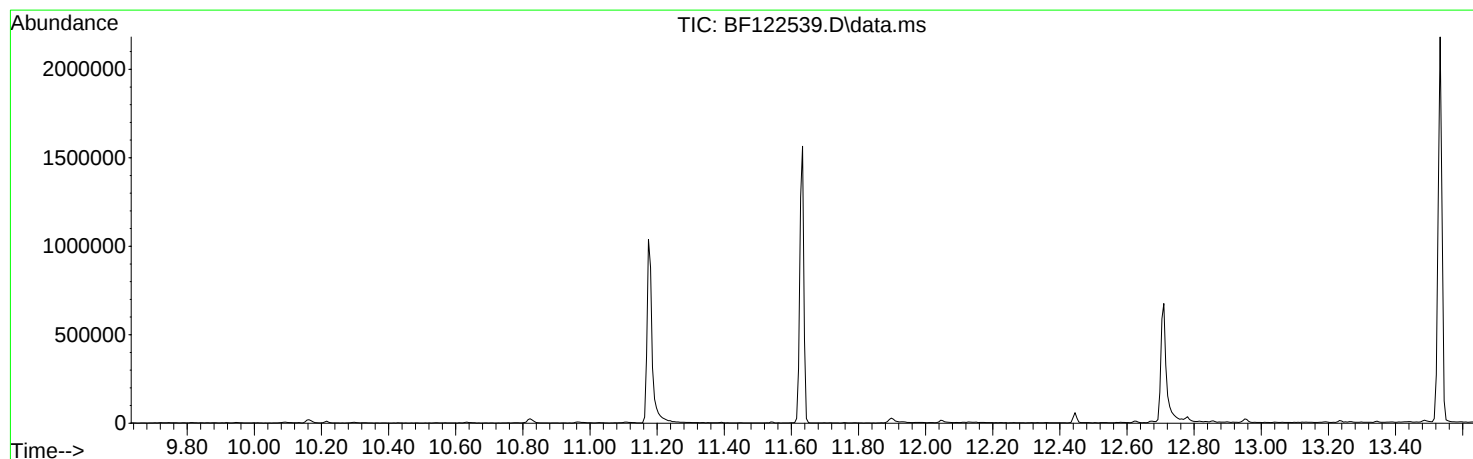

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	40044	PASS
68	69	0.00	2	1.7	699	PASS
69	198	0.00	100	33.7	40948	PASS
70	69	0.00	2	0.3	115	PASS
127	198	10	80	46.7	56656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121419	PASS
199	198	5	9	6.8	8258	PASS
275	198	10	60	29.7	36104	PASS
365	198	1	100	3.8	4674	PASS
441	198	0.01	100	18.6	22570	PASS
442	442	100	100	100.0	149195	PASS
443	442	15	24	19.0	28283	PASS