

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
 Data File : BF140726.D
 Acq On : 04 Dec 2024 14:01
 Operator : RC/JU
 Sample : PB165356BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165356BL

Quant Time: Dec 04 14:20:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 15:23:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	89820	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	363420	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	219573	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	452822	20.000	ng	0.00
76) Chrysene-d12	14.057	240	326311	20.000	ng	0.00
86) Perylene-d12	15.562	264	268136	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	763792	145.089	ng	0.02
7) Phenol-d6	6.516	99	1006734	144.656	ng	0.00
23) Nitrobenzene-d5	7.439	82	664117	93.472	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	377124	160.591	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1374719	93.283	ng	0.00
79) Terphenyl-d14	12.992	244	1808338	86.292	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.439	70	91651	22.283	ng	# 75
25) Isophorone	7.439	82	653512	55.146	ng	# 66
51) 2,6-Dinitrotoluene	9.910	165	27372	8.346	ng	# 20
57) 2,4-Dinitrotoluene	9.910	165	27372	6.280	ng	# 18
67) 4-Bromophenyl-phenylether	10.710	248	23777	5.099	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140726.D
Acq On : 04 Dec 2024 14:01
Operator : RC/JU
Sample : PB165356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165356BL

Quant Time: Dec 04 14:20:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration




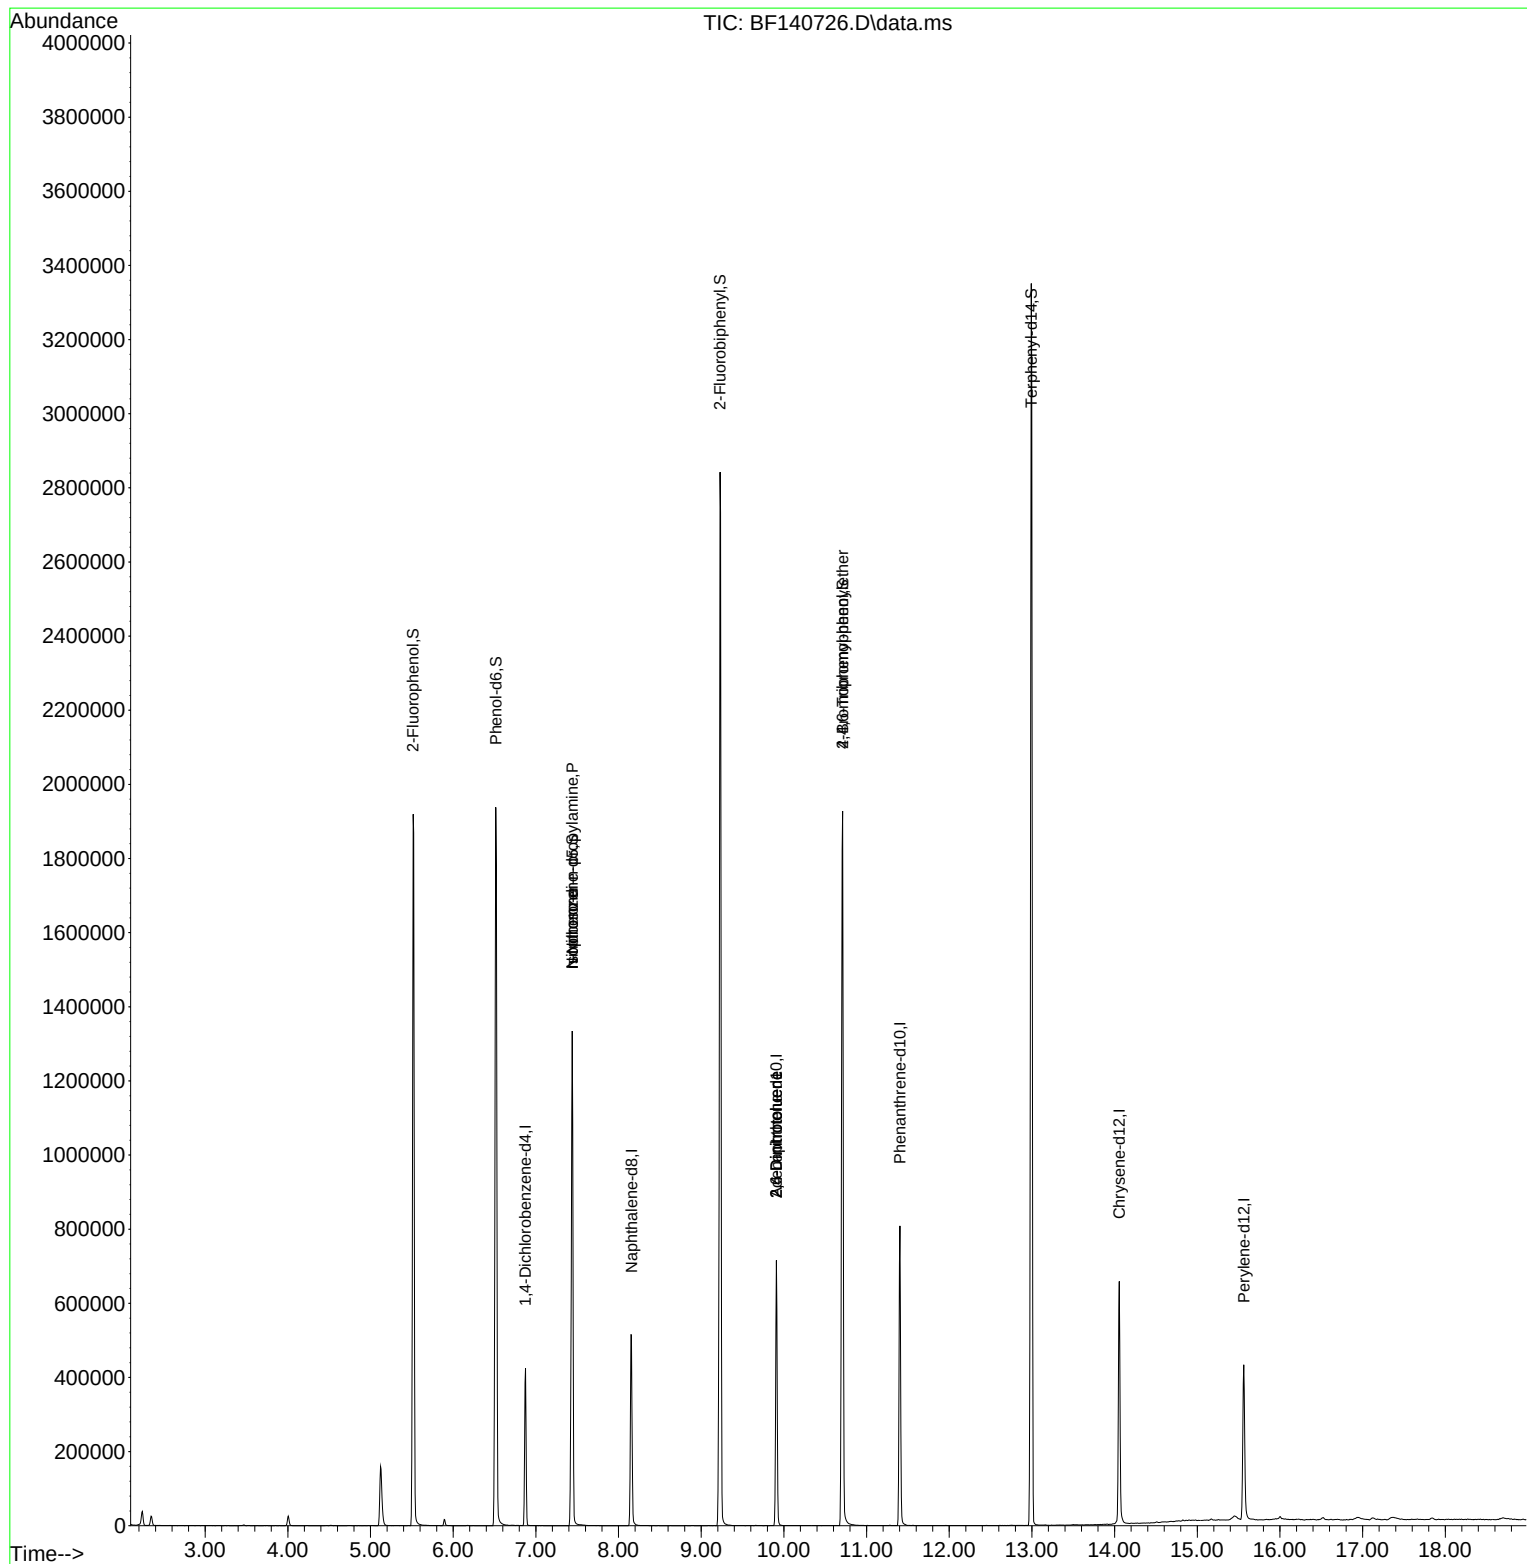




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 813
Delta R.T. -0.000 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion:152 Resp: 89820
Ion Ratio Lower Upper
152 100
150 156.7 128.5 192.7
115 60.5 50.2 75.4

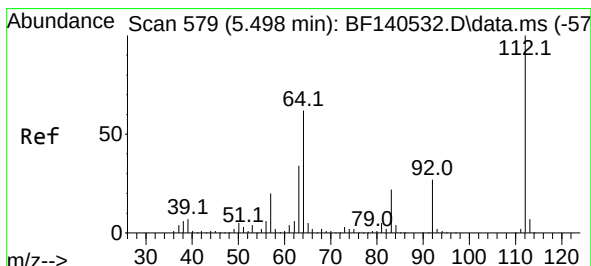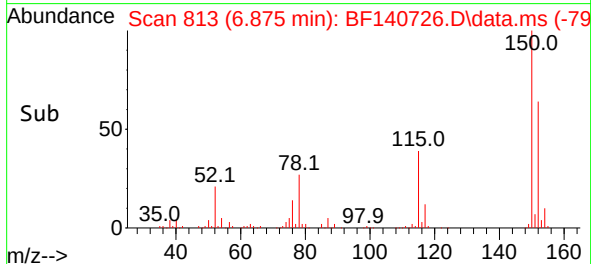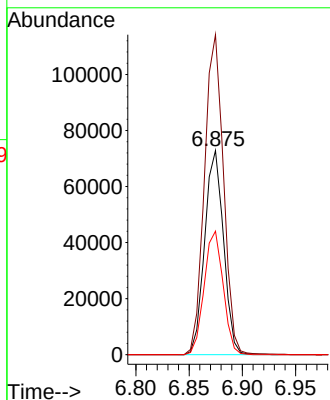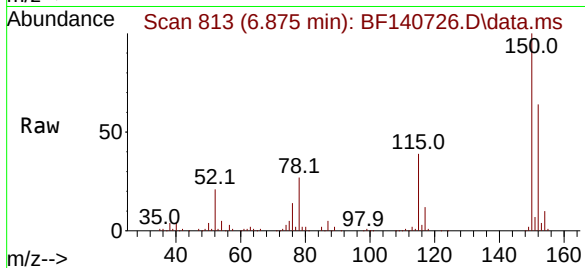

#5
2-Fluorophenol
Concen: 145.089 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.018 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion:112 Resp: 763792
Ion Ratio Lower Upper
112 100
64 59.9 49.2 73.8
63 32.4 27.0 40.4


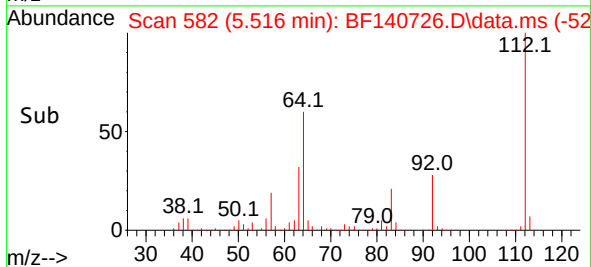
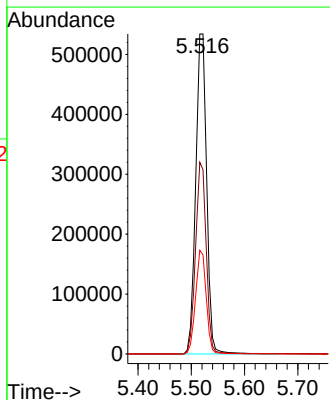
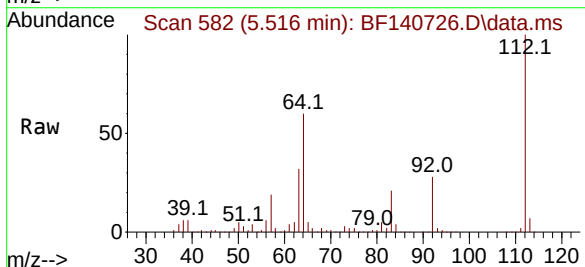


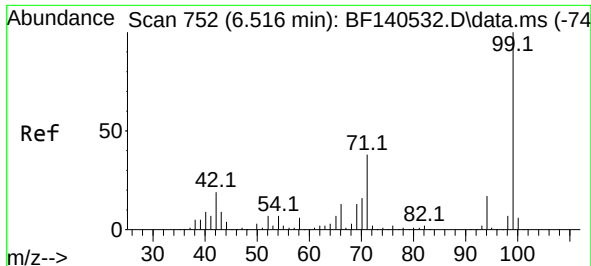

#7
Phenol-d6
Concen: 144.656 ng
RT: 6.516 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion: 99 Resp: 1006734
Ion Ratio Lower Upper
99 100
42 18.1 15.4 23.0
71 36.9 30.6 46.0

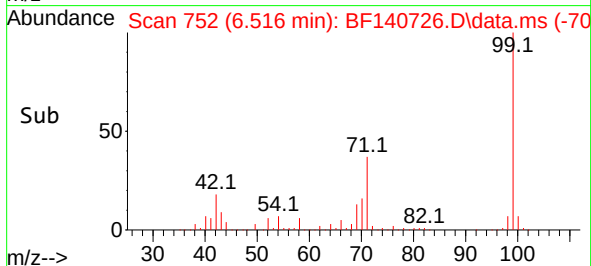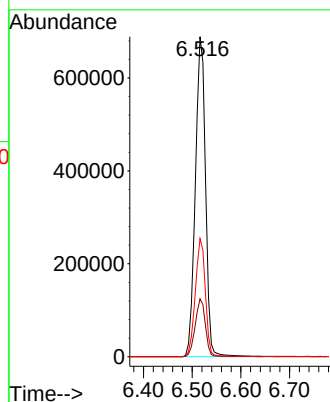

#19
n-Nitroso-di-n-propylamine
Concen: 22.283 ng
RT: 7.439 min Scan# 909
Delta R.T. 0.153 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion: 70 Resp: 91651
Ion Ratio Lower Upper
70 100
42 44.3 47.6 71.4#
101 0.0 7.6 11.4#
130 1.8 16.2 24.4#


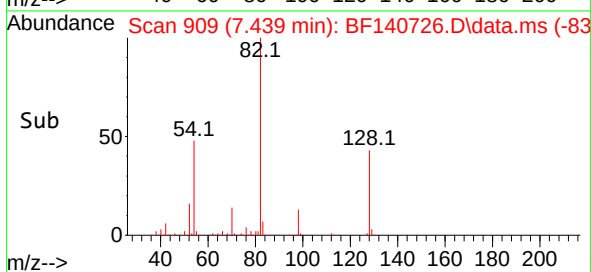
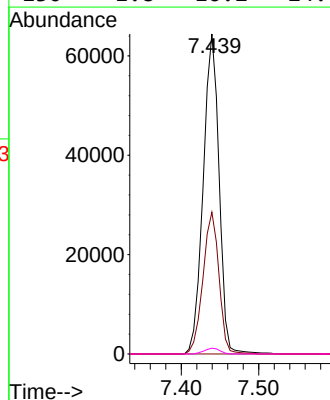
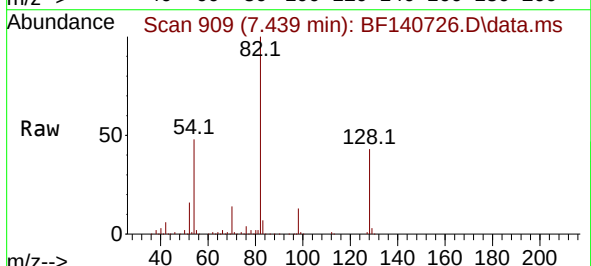


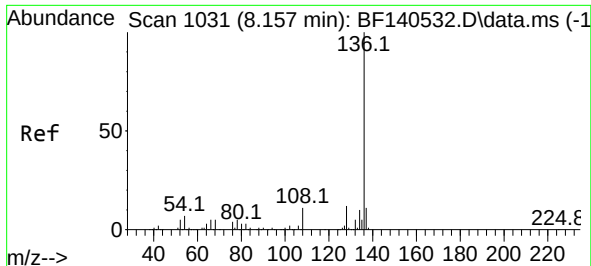

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1031
Delta R.T. -0.000 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion:136 Resp: 363420
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 6.7 5.8 8.8
68 4.9 4.1 6.1

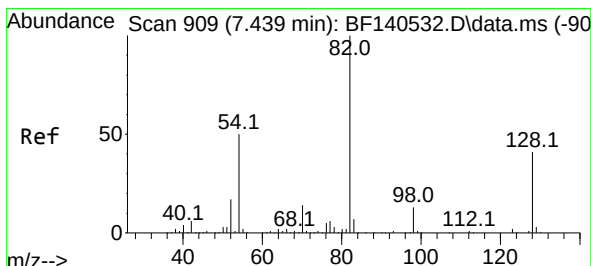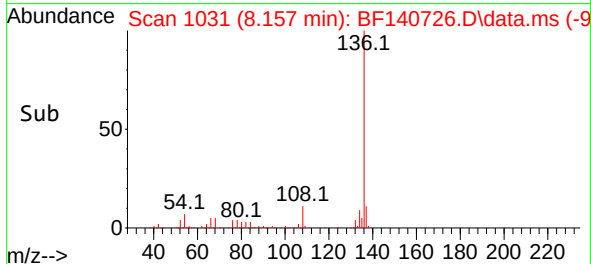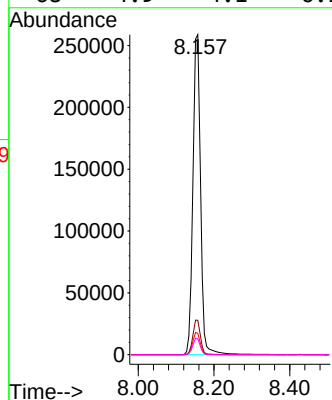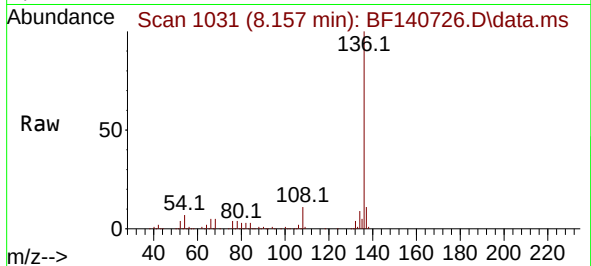

#23
Nitrobenzene-d5
Concen: 93.472 ng
RT: 7.439 min Scan# 909
Delta R.T. -0.000 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion: 82 Resp: 664117
Ion Ratio Lower Upper
82 100
128 43.3 33.0 49.4
54 48.4 39.5 59.3


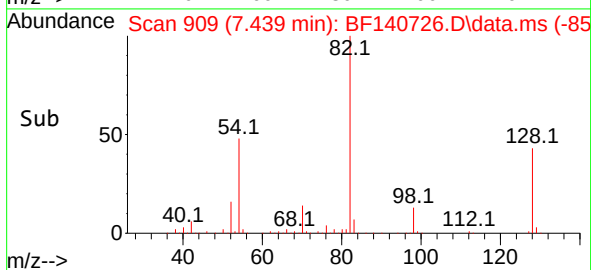
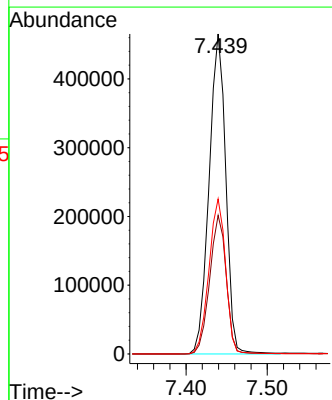
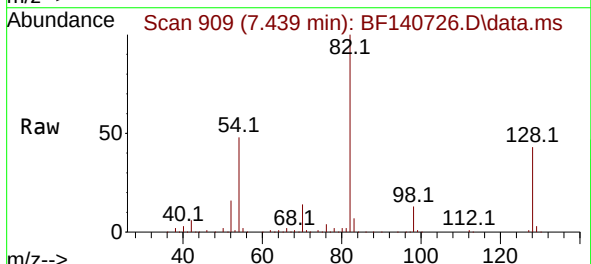


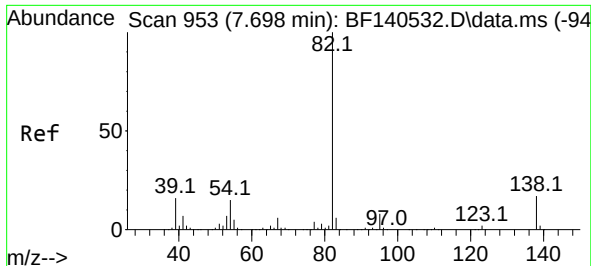

#25
Isophorone
Concen: 55.146 ng
RT: 7.439 min Scan# 90
Delta R.T. -0.259 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion: 82 Resp: 653512
Ion Ratio Lower Upper
82 100
95 0.0 6.4 9.6#
138 0.0 13.8 20.6#

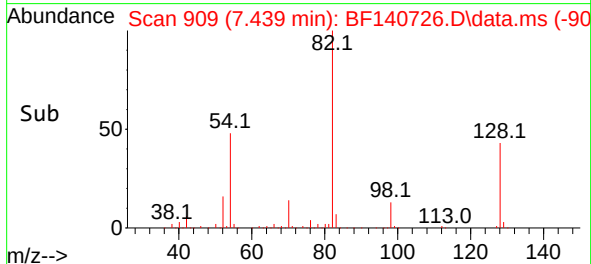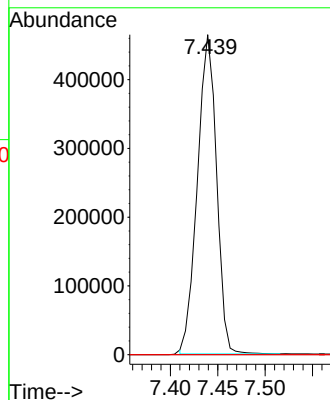

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01


Tgt Ion:164 Resp: 219573
Ion Ratio Lower Upper
164 100
162 101.4 80.6 120.8
160 44.5 36.2 54.4

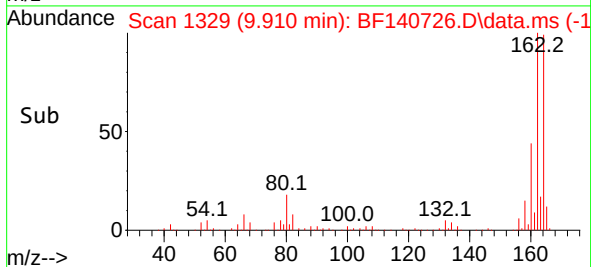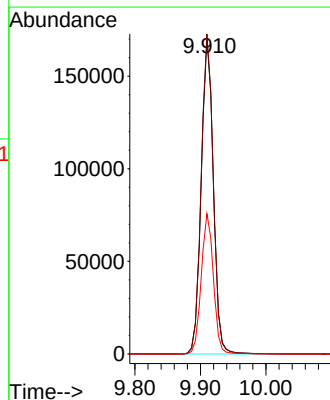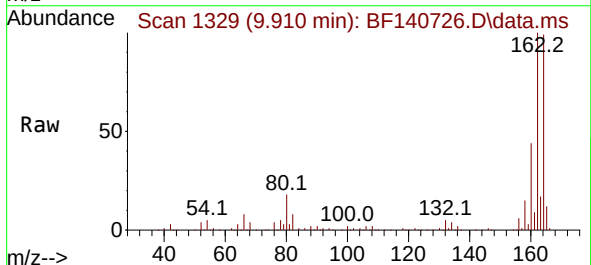






#42
2,4,6-Tribromophenol
Concen: 160.591 ng
RT: 10.710 min Scan# 1465
Delta R.T. 0.006 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Instrument :
BNA_F
ClientSampleId :
PB165356BL



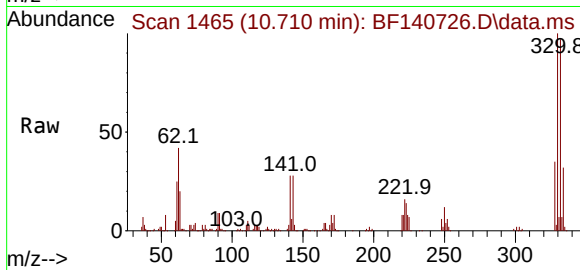



Tgt Ion:330 Resp: 377124
Ion Ratio Lower Upper
330 100
332 96.8 76.9 115.3
141 30.2 26.7 40.1

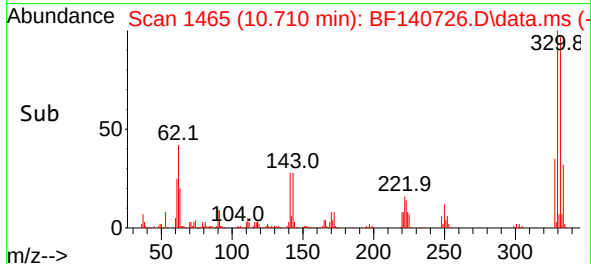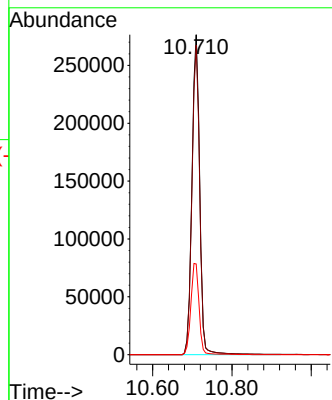

#45
2-Fluorobiphenyl
Concen: 93.283 ng
RT: 9.228 min Scan# 1213
Delta R.T. -0.006 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion:172 Resp: 1374719
Ion Ratio Lower Upper
172 100
171 35.5 28.4 42.6
170 23.7 19.0 28.6


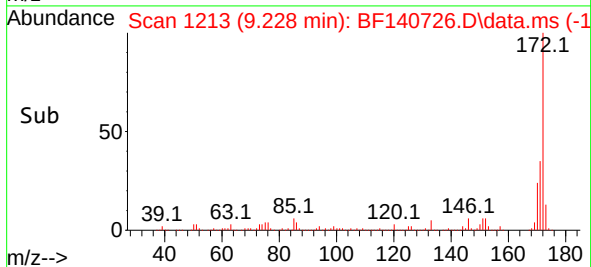
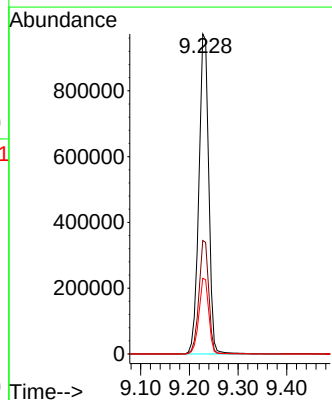
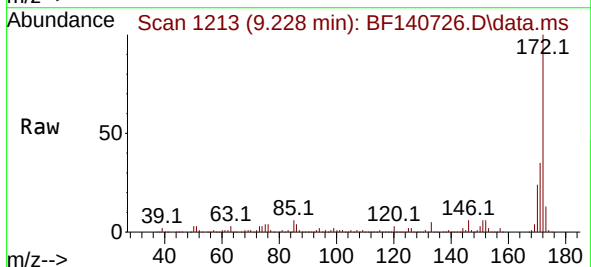


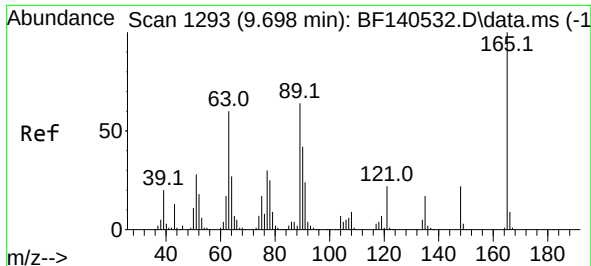

#51
2,6-Dinitrotoluene
Concen: 8.346 ng
RT: 9.910 min Scan# 11
Delta R.T. 0.212 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion:165 Resp: 27372
Ion Ratio Lower Upper
165 100
63 1.1 49.9 74.9#
89 1.4 50.9 76.3#

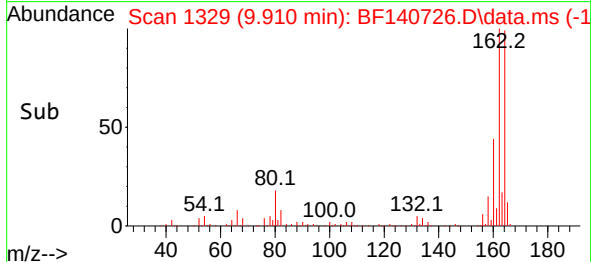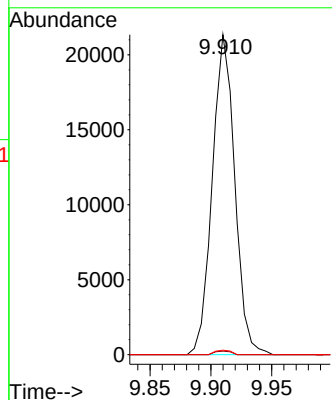

#57
2,4-Dinitrotoluene
Concen: 6.280 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.194 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion:165 Resp: 27372
Ion Ratio Lower Upper
165 100
63 1.1 41.7 62.5#
89 1.4 65.8 98.8#
182 0.0 2.1 3.1#


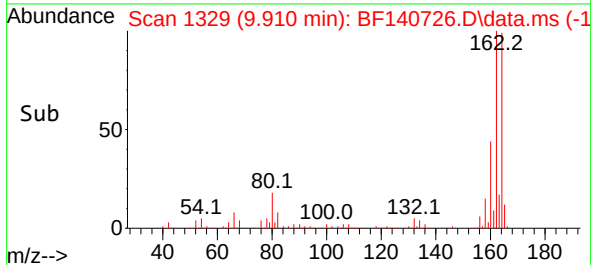
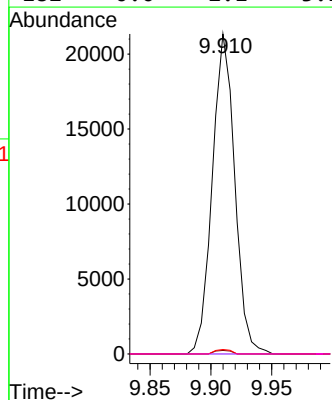
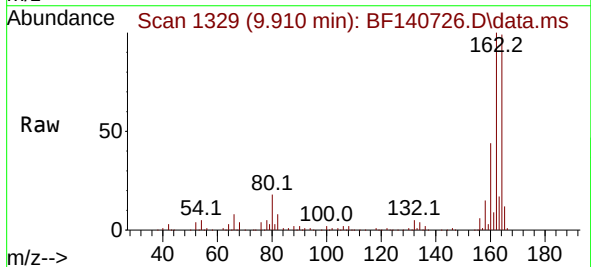


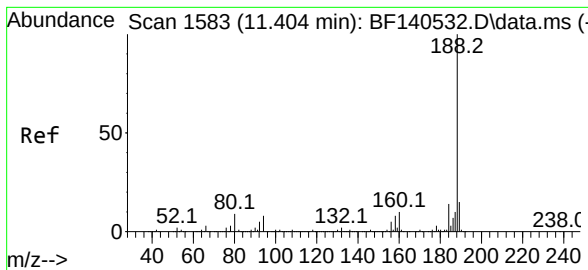

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion:188 Resp: 452822
Ion Ratio Lower Upper
188 100
94 8.2 6.4 9.6
80 8.8 6.9 10.3

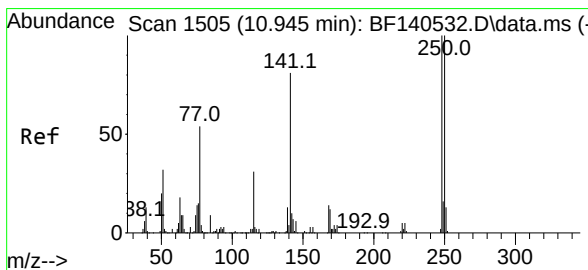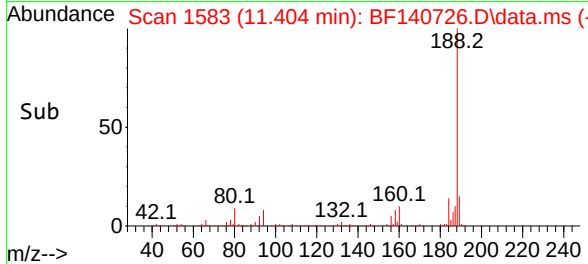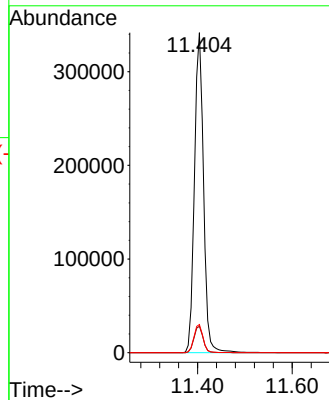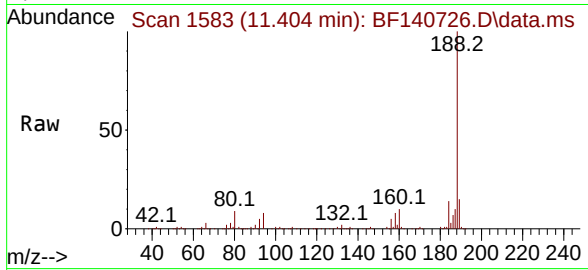

#67
4-Bromophenyl-phenylether
Concen: 5.099 ng
RT: 10.710 min Scan# 1465
Delta R.T. -0.235 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion:248 Resp: 23777
Ion Ratio Lower Upper
248 100
250 198.6 79.8 119.8#
141 459.1 64.7 97.1#


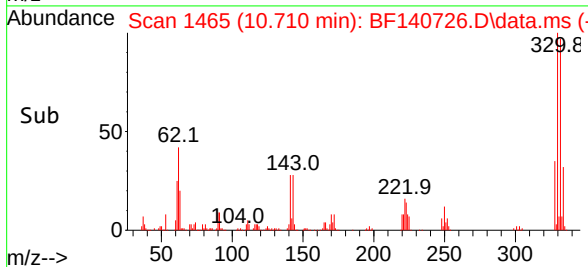
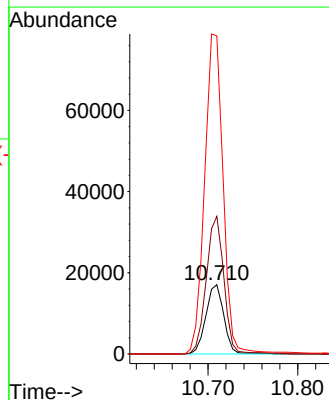
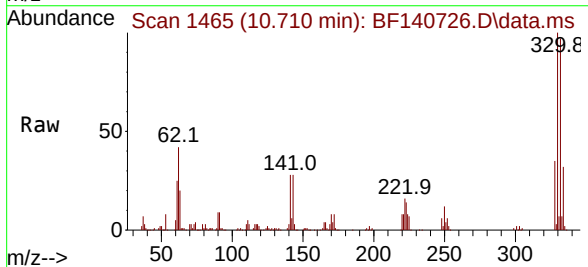




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.057 min Scan# 2033
Delta R.T. 0.006 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01




Instrument :
BNA_F
ClientSampleId :
PB165356BL


Tgt Ion:240 Resp: 326311
Ion Ratio Lower Upper
240 100
120 8.9 7.3 10.9
236 25.9 20.6 31.0

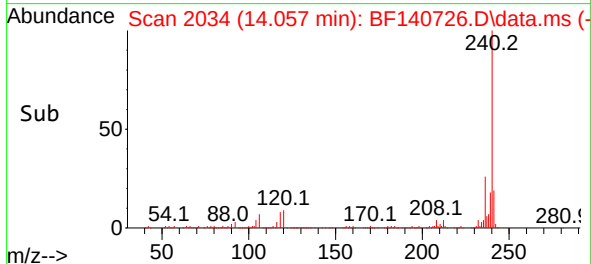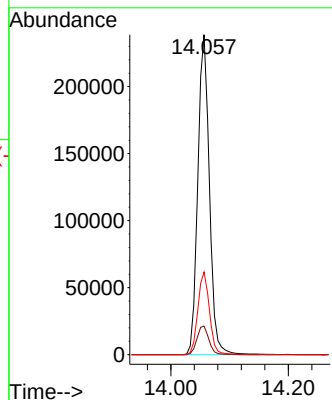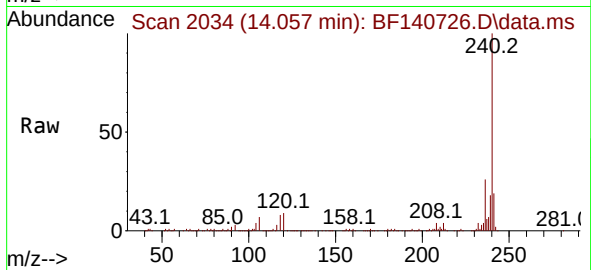

#79
Terphenyl-d14
Concen: 86.292 ng
RT: 12.992 min Scan# 1853
Delta R.T. -0.000 min
Lab File: BF140726.D
Acq: 04 Dec 2024 14:01

Tgt Ion:244 Resp: 1808338
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.8
122 10.8 8.0 12.0

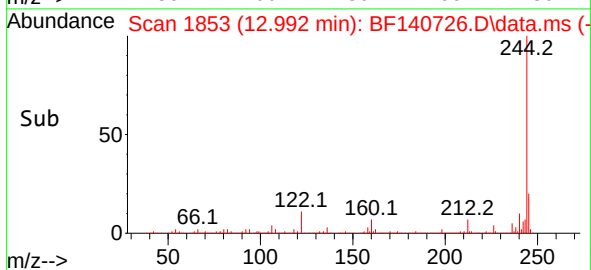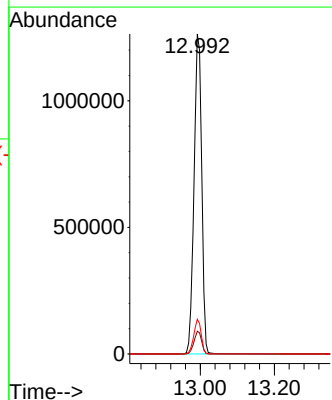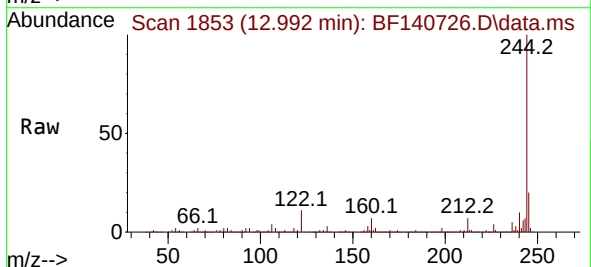



#86

Perylene-d12

Concen: 20.000 ng

RT: 15.562 min Scan# 21

Delta R.T. 0.023 min

Lab File: BF140726.D


Acq: 04 Dec 2024 14:01

Instrument :

BNA_F

ClientSampleId :

PB165356BL

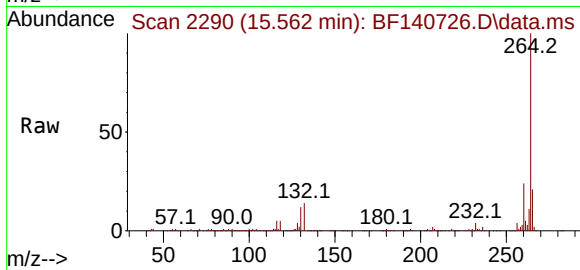

Tgt Ion:264 Resp: 268136

Ion Ratio Lower Upper

264 100

260 23.8 19.0 28.6

265 21.2 16.6 25.0

