
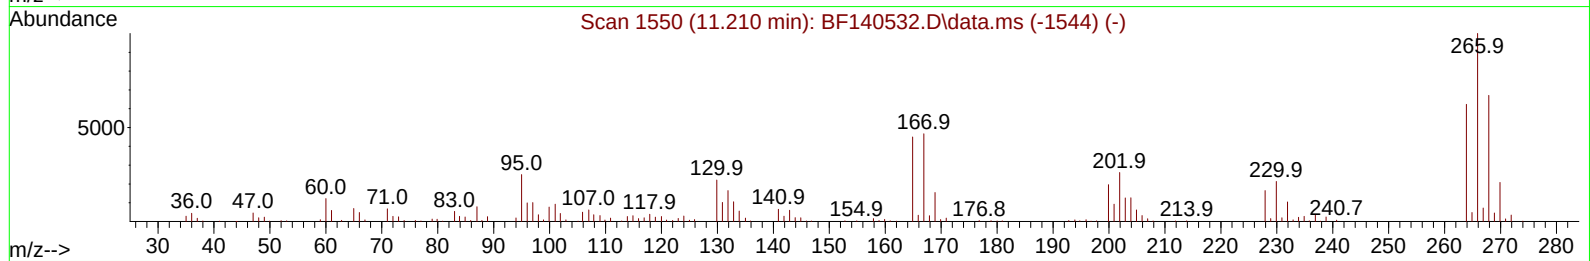
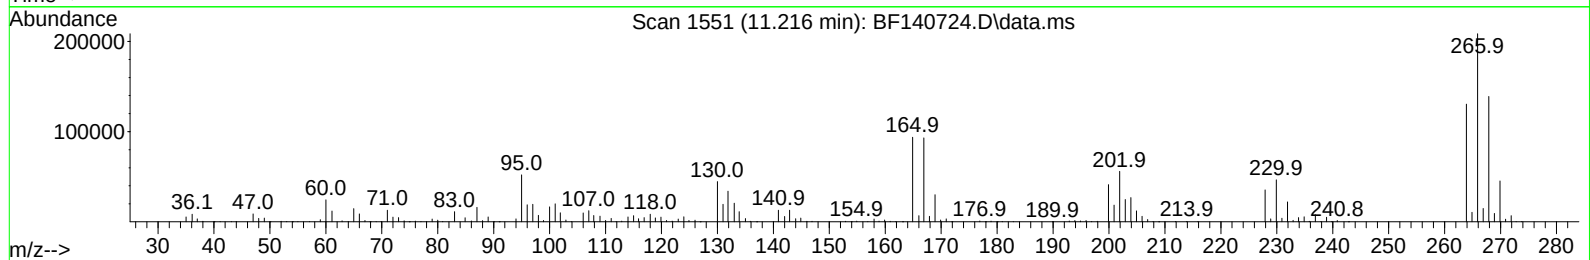


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140724.D
Acq On : 04 Dec 2024 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 13:27:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

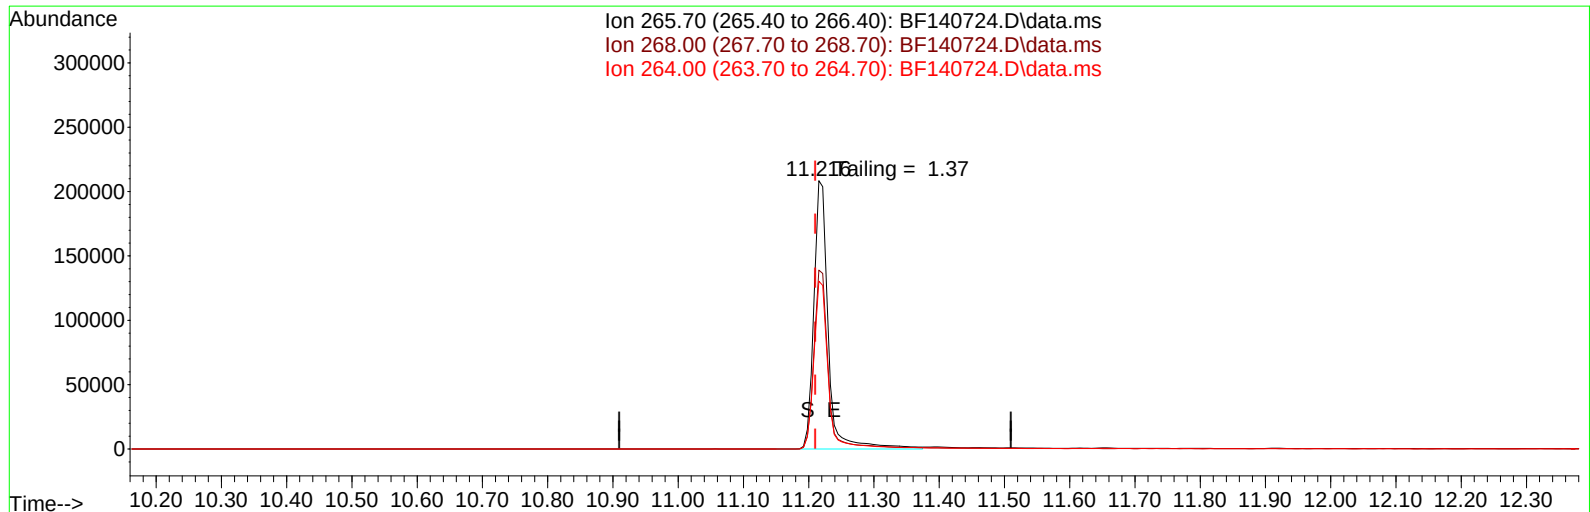

TIC: BF140724.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 20244.19 ng

response 321187

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.67
264.00	62.30	62.55
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\  
Data File : BF140724.D  
Acq On    : 04 Dec 2024 12:41  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 04 13:27:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

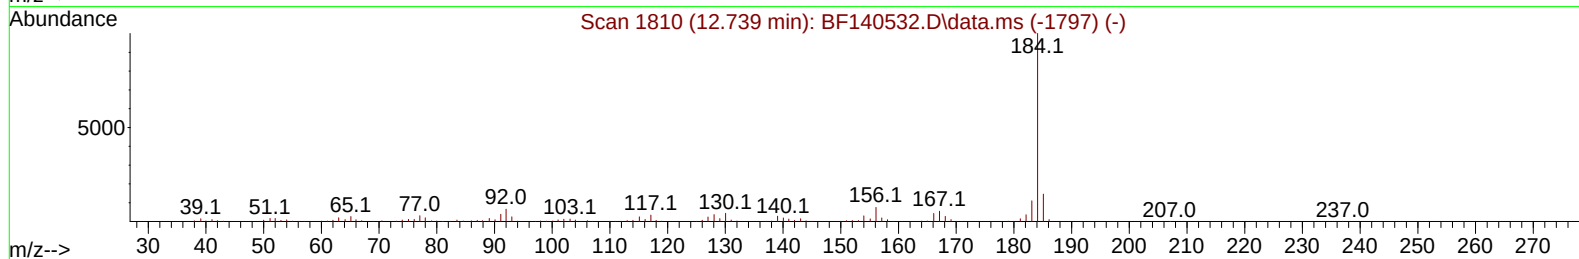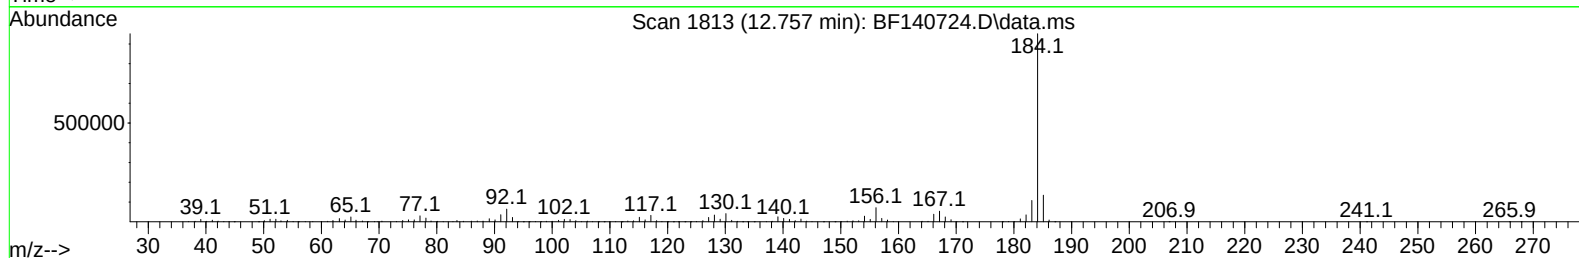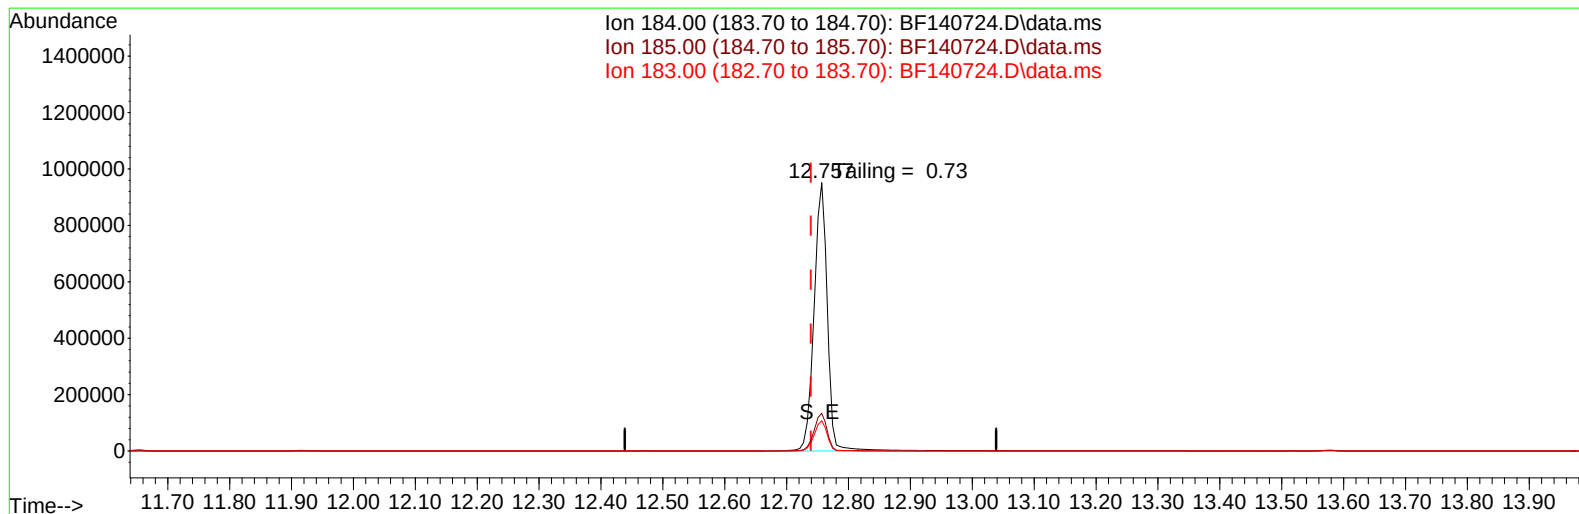

TIC: BF140724.D\data.ms

(77) Benzidine

12.757min (+ 0.018) 13484.71 ng

response **1431804**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.10
183.00	11.00	11.30
0.00	0.00	0.00