

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
 Data File : BF140726.D
 Acq On : 04 Dec 2024 14:01
 Operator : RC/JU
 Sample : PB165356BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165356BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	12	25	33	rVB	37466	66230	1.41%	0.276%
2	5.122	509	515	536	rBV	159715	300515	6.38%	1.252%
3	5.516	576	582	605	rBV	1919316	2699499	57.29%	11.245%
4	6.516	746	752	779	rBV	1937826	2831024	60.08%	11.793%
5	6.875	808	813	823	rBV	423818	526220	11.17%	2.192%
6	7.439	902	909	914	rBV	1334587	1884410	39.99%	7.850%
7	8.151	1025	1030	1047	rBV	514838	717392	15.22%	2.988%
8	9.228	1206	1213	1239	rBV	2842309	3955267	83.94%	16.476%
9	9.910	1323	1329	1348	rVB	715230	915694	19.43%	3.814%
10	10.710	1458	1465	1494	rBV	1927979	2707438	57.46%	11.278%
11	11.404	1577	1583	1602	rBV	808537	1062630	22.55%	4.426%
12	12.992	1847	1853	1859	rBV	3349973	4712266	100.00%	19.629%
13	14.057	2023	2034	2049	rBV	653902	931014	19.76%	3.878%
14	15.562	2283	2290	2303	rBV	417486	696956	14.79%	2.903%




Sum of corrected areas: 24006555

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140726.D
Acq On : 04 Dec 2024 14:01
Operator : RC/JU
Sample : PB165356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165356BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

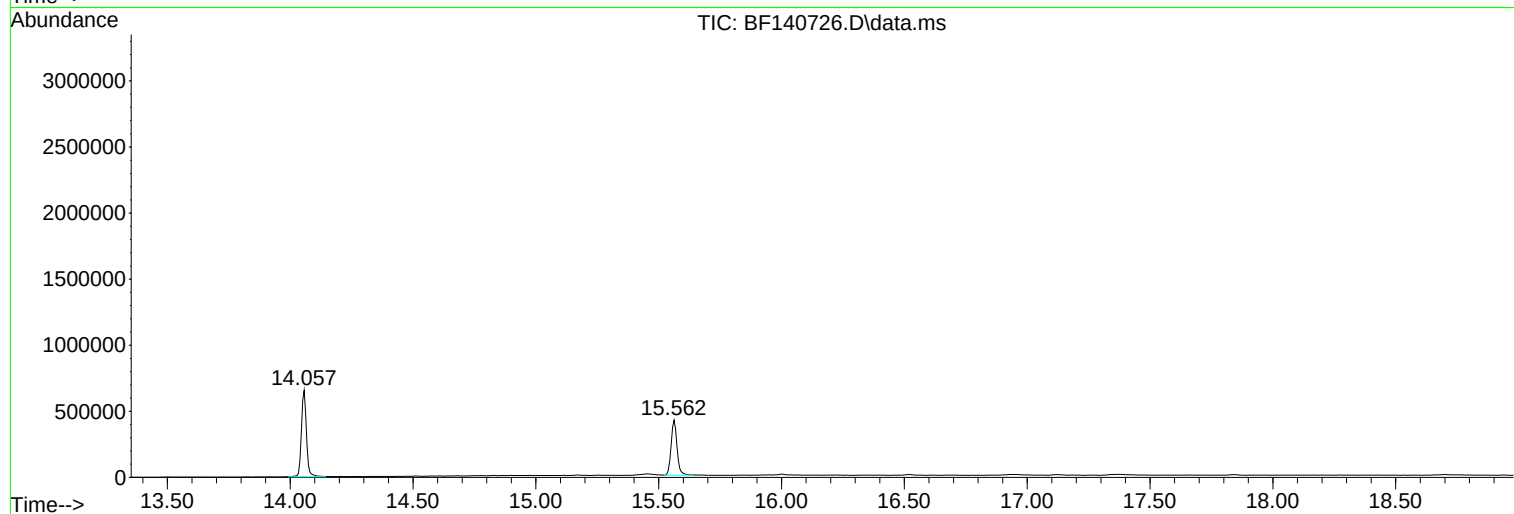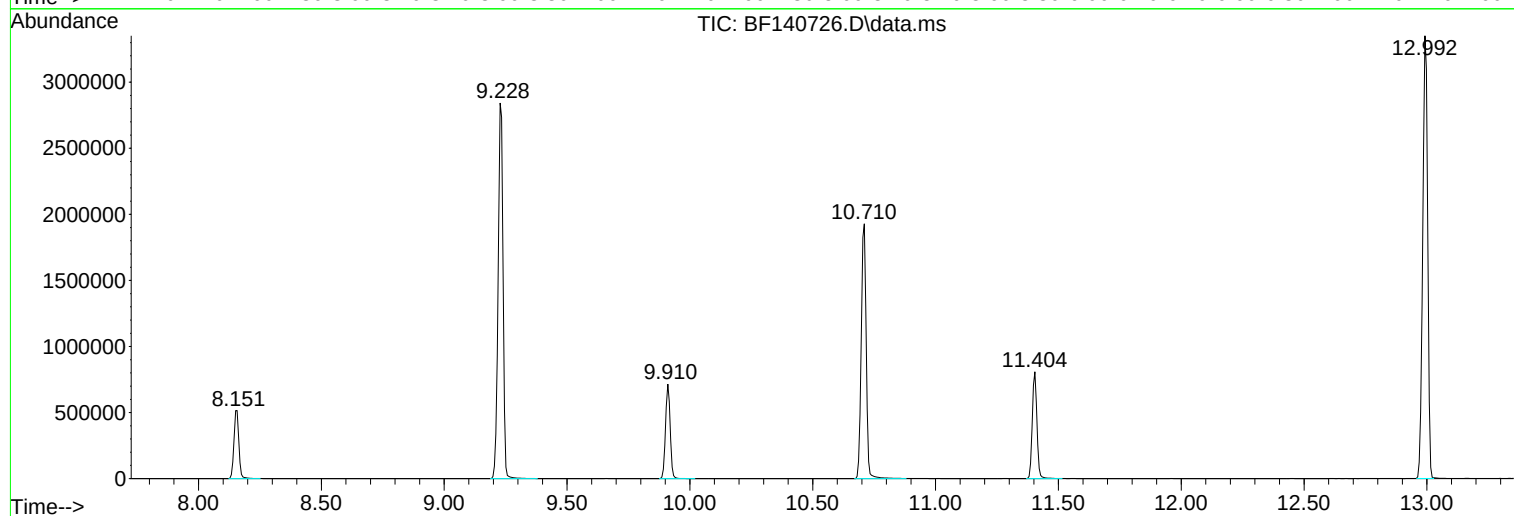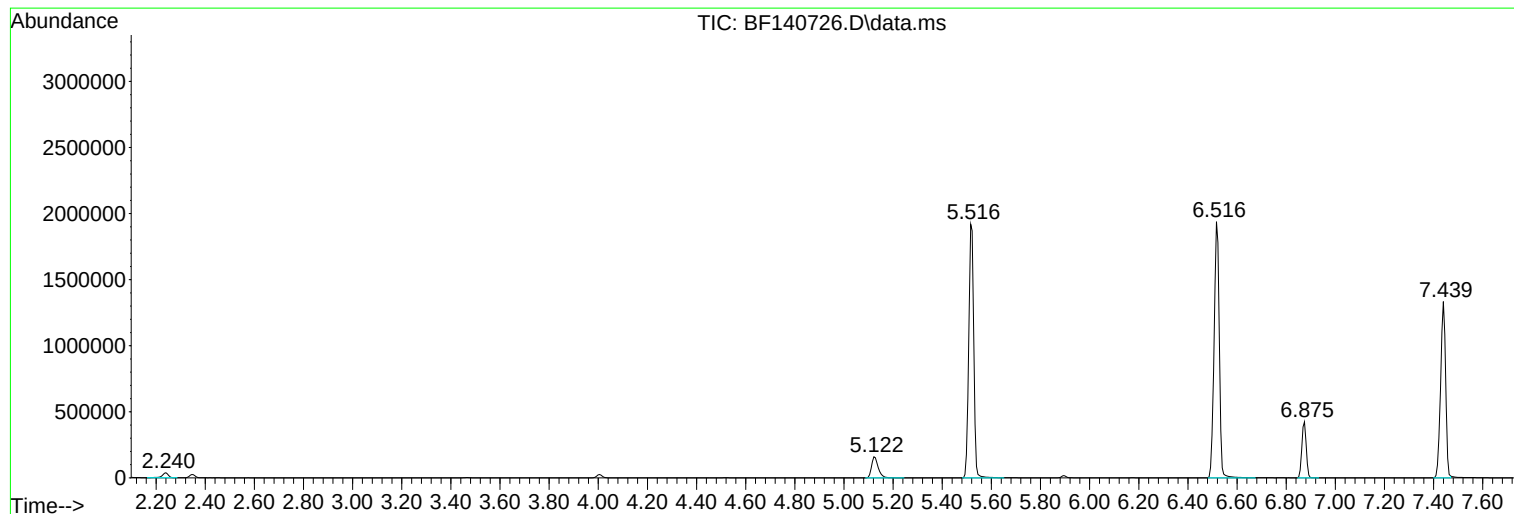

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140726.D
Acq On : 04 Dec 2024 14:01
Operator : RC/JU
Sample : PB165356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165356BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140726.D
Acq On : 04 Dec 2024 14:01
Operator : RC/JU
Sample : PB165356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165356BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------