
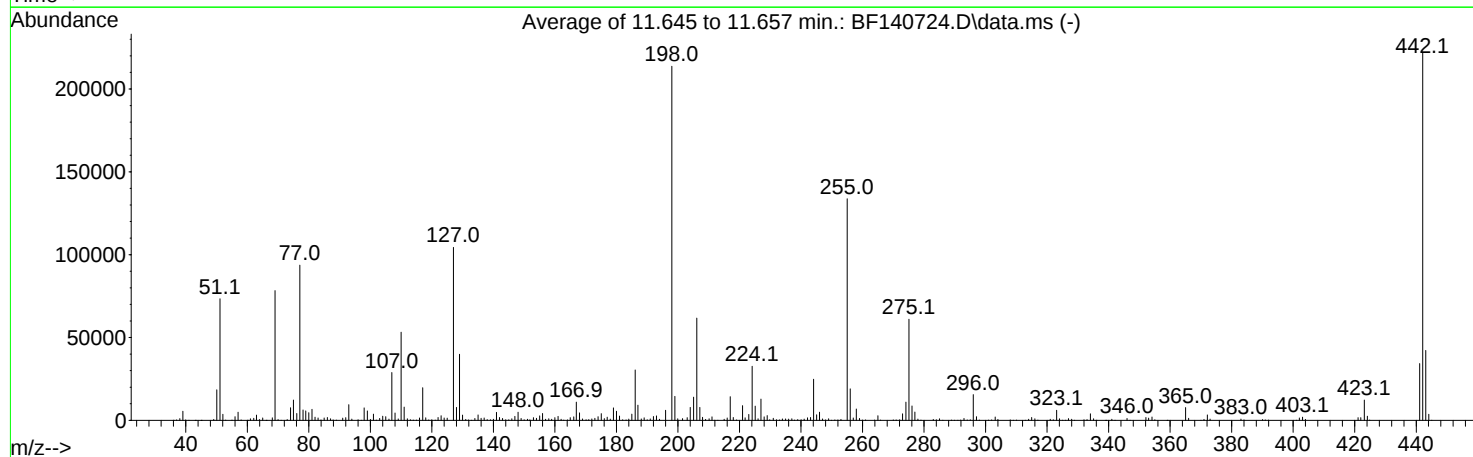


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140724.D
Acq On : 04 Dec 2024 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

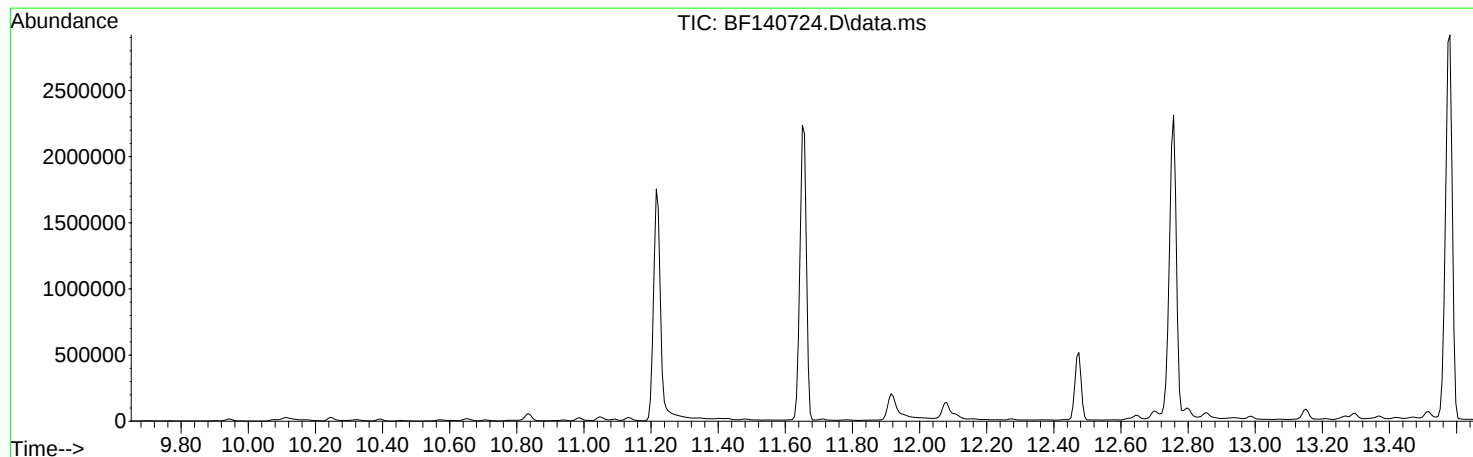

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	73368	PASS
68	69	0.00	2	1.9	1508	PASS
69	198	0.00	100	36.6	78314	PASS
70	69	0.00	2	0.7	514	PASS
127	198	10	80	48.9	104408	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	213696	PASS
199	198	5	9	6.8	14509	PASS
275	198	10	60	28.6	61037	PASS
365	198	1	100	3.6	7751	PASS
441	198	0.01	100	16.0	34283	PASS
442	442	50	100	100.0	222019	PASS
443	442	15	24	19.0	42173	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/4/2024	BNA_F	<u>BF140724.D</u>
Compound Name	Response	Retention Time
DDT	810257	13.58
DDD	19304	13.298
DDE	7866	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27170	837427	3.24

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140724.D
Acq On : 04 Dec 2024 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 04 13:27:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

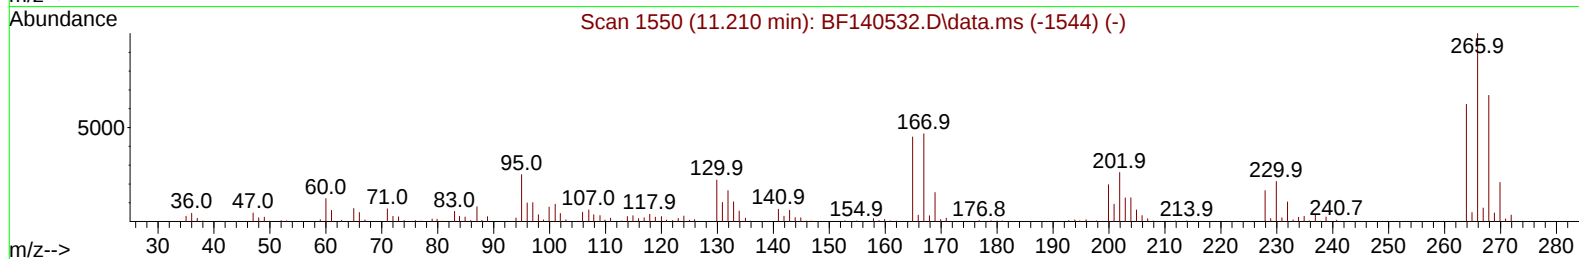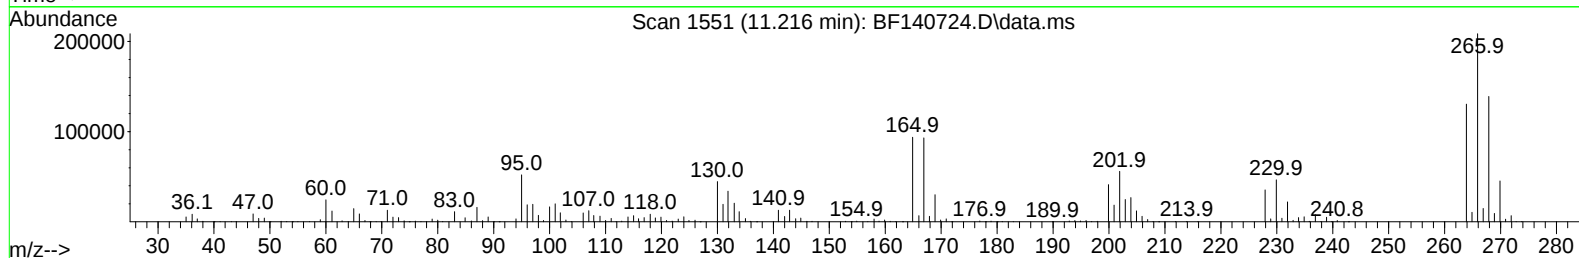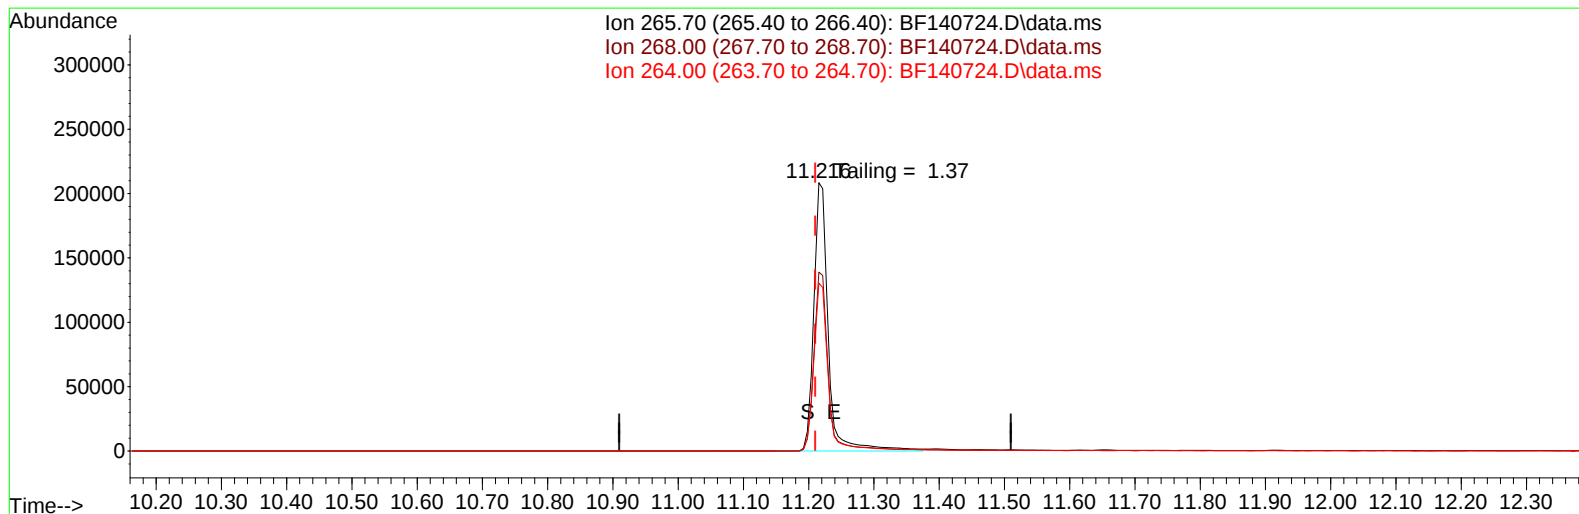

TIC: BF140724.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 20244.19 ng




response 321187

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.67
264.00	62.30	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120424\
Data File : BF140724.D
Acq On : 04 Dec 2024 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 04 13:27:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

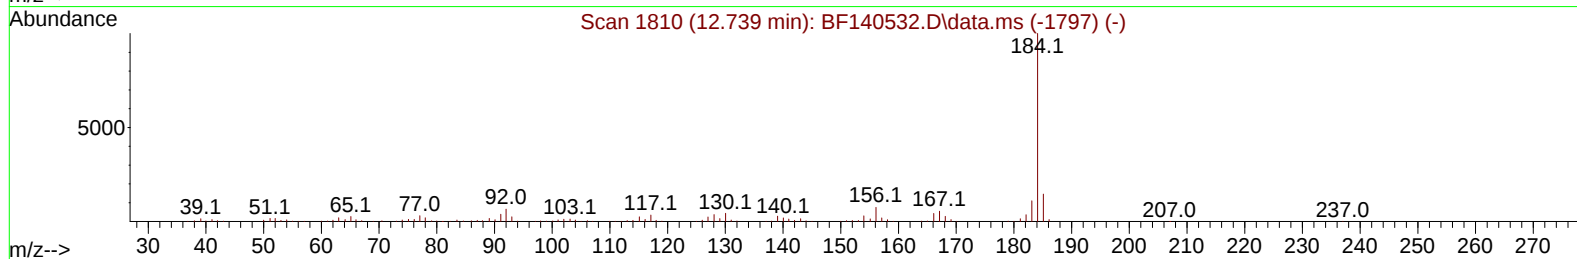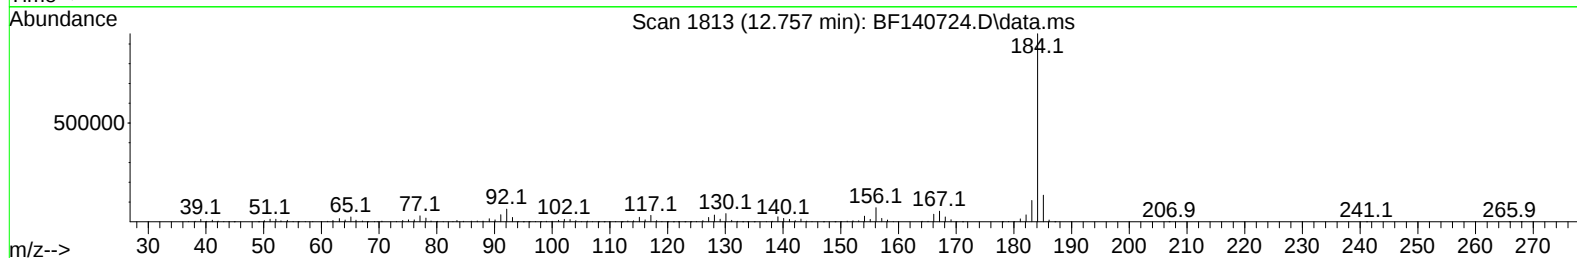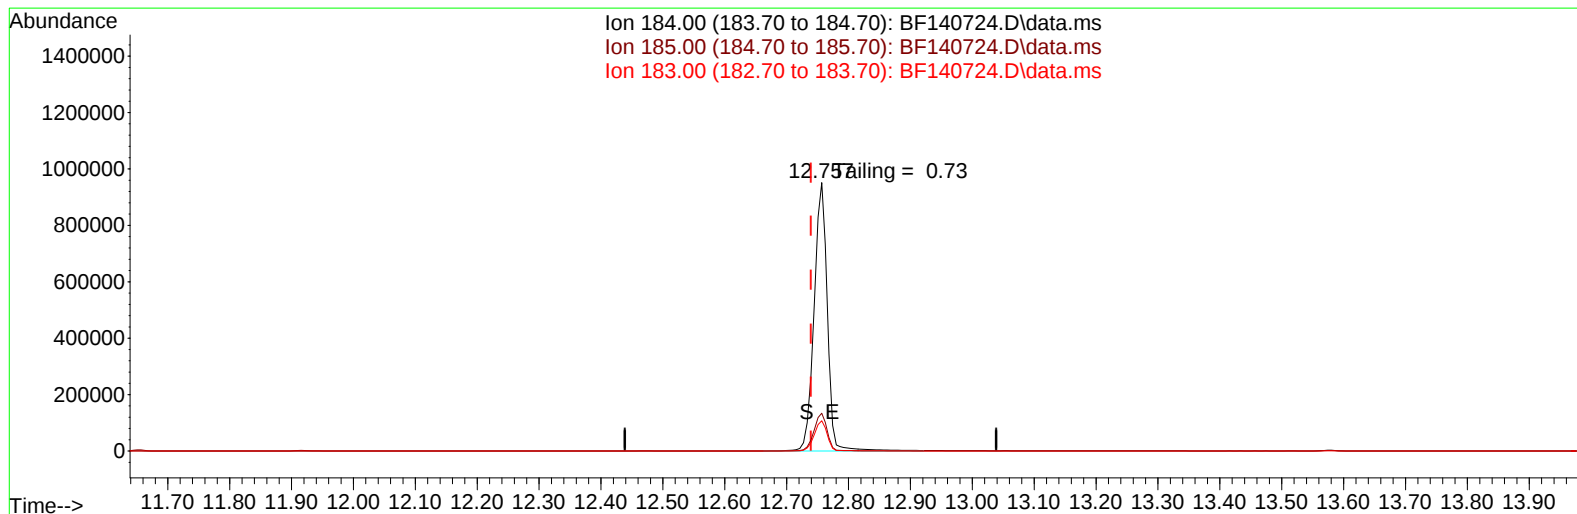

TIC: BF140724.D\data.ms

(77) Benzidine

12.757min (+ 0.018) 13484.71 ng

response 1431804

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.10
183.00	11.00	11.30
0.00	0.00	0.00