

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120516\
 Data File : BF091423.D
 Acq On : 5 Dec 2016 17:42
 Operator : UM/SJ
 Sample : H5838-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-6

Quant Time: Dec 06 00:06:27 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 13:33:46 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	125031	20.00	ng	-0.03
21) Naphthalene-d8	8.13	136	466650	20.00	ng	-0.04
38) Acenaphthene-d10	9.89	164	312488	20.00	ng	-0.03
63) Phenanthrene-d10	11.36	188	539486	20.00	ng	-0.04
75) Chrysene-d12	14.00	240	497345	20.00	ng	-0.04
86) Perylene-d12	15.42	264	331164	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	496764	64.91	ng	-0.03
7) Phenol-d6	6.47	99	375305	39.84	ng	-0.03
23) Nitrobenzene-d5	7.41	82	888863	106.74	ng	-0.04
41) 2,4,6-Tribromophenol	10.68	330	427018	144.34	ng	-0.03
44) 2-Fluorobiphenyl	9.21	172	1621629	93.96	ng	-0.03
78) Terphenyl-d14	12.96	244	2154398	94.15	ng	-0.03
Target Compounds						
9) Benzaldehyde	6.62	77	25257	4.17	ng	Qvalue 89
15) Benzyl Alcohol	7.01	79	16092	2.13	ng	# 40
19) n-Nitroso-di-n-propylamine	7.41	70	118223	19.92	ng	# 74
25) Isophorone	7.41	82	786065	53.28	ng	# 67
50) 2,6-Dinitrotoluene	9.89	165	41229	9.75	ng	# 17
56) 2,4-Dinitrotoluene	9.89	165	41230	7.52	ng	# 34
66) 4-Bromophenyl-phenylether	10.68	248	28909	4.99	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120516\
Data File : BF091423.D
Acq On : 5 Dec 2016 17:42
Operator : UM/SJ
Sample : H5838-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6

Quant Time: Dec 06 00:06:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

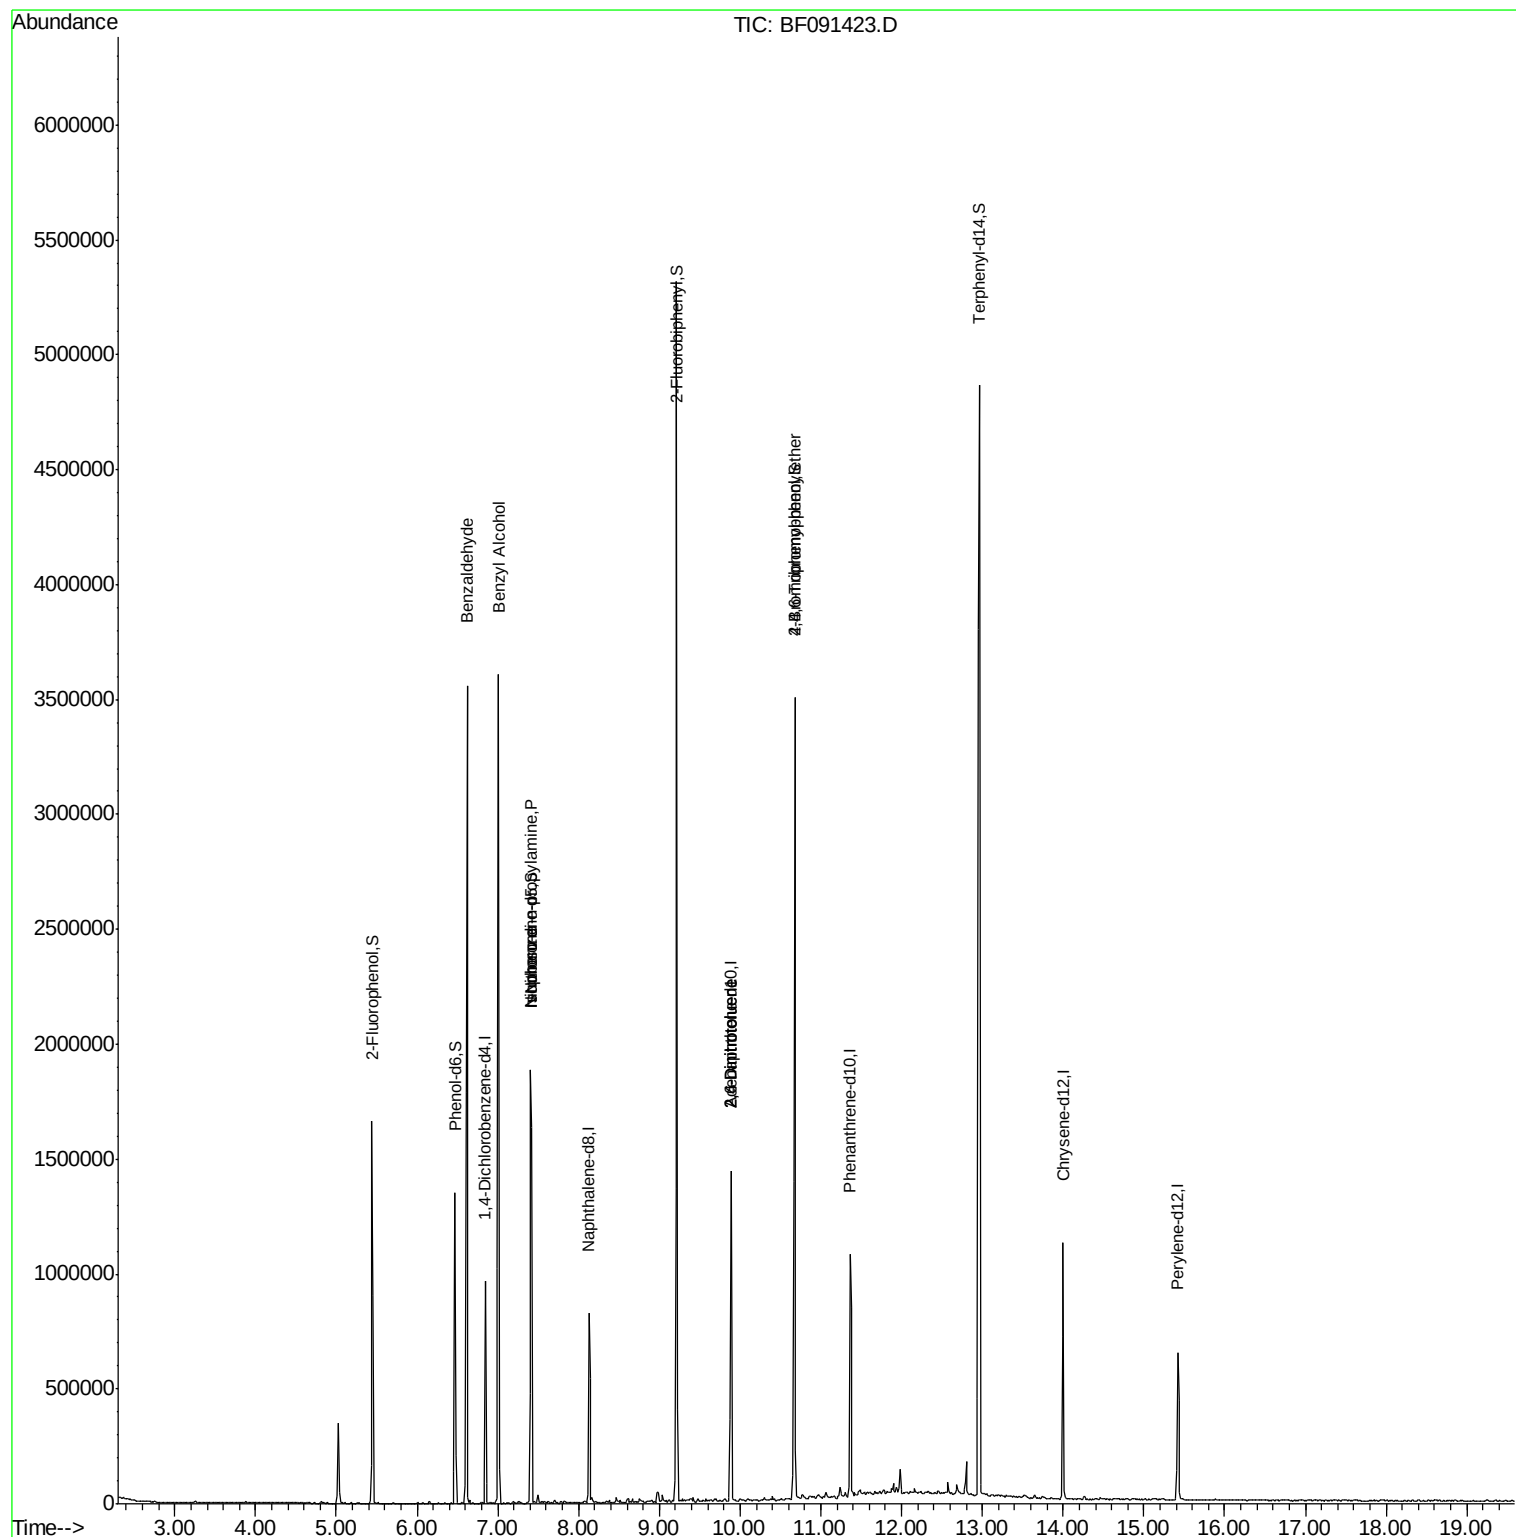

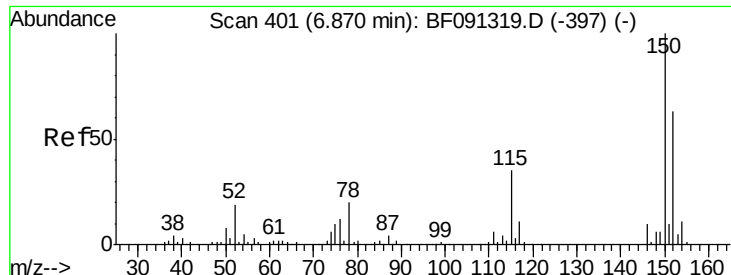

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 399

Delta R.T. -0.03 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42

Instrument :

BNA_F

ClientSampleId :

MW-6


Tgt Ion:152 Resp: 125031

Ion Ratio Lower Upper

152 100

150 158.5 122.5 183.7




115 64.4 51.8 77.8

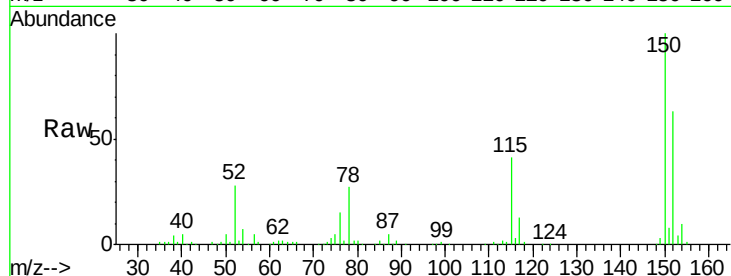

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

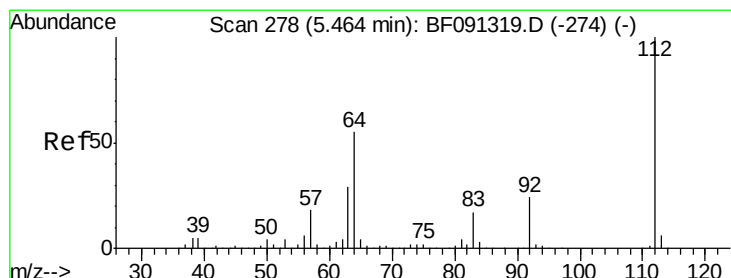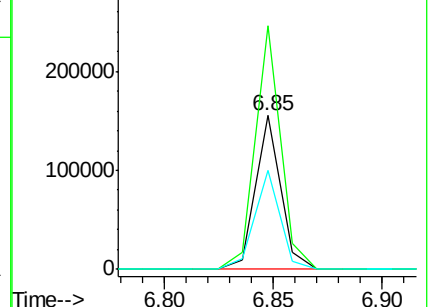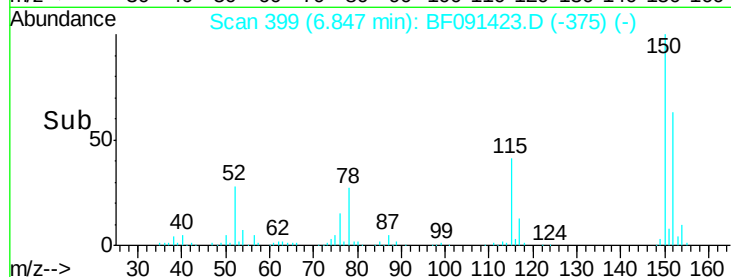

#5

2-Fluorophenol

Concen: 64.91 ng

RT: 5.44 min Scan# 276

Delta R.T. -0.03 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42


Tgt Ion:112 Resp: 496764

Ion Ratio Lower Upper

112 100

64 78.0 61.5 92.3



63 42.3 33.3 49.9

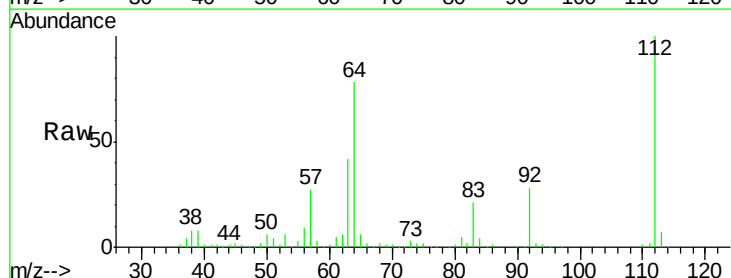


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

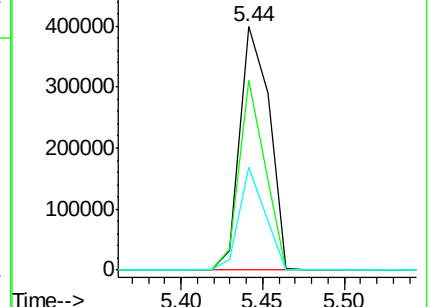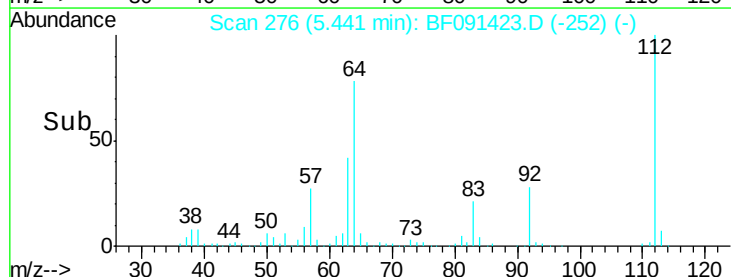

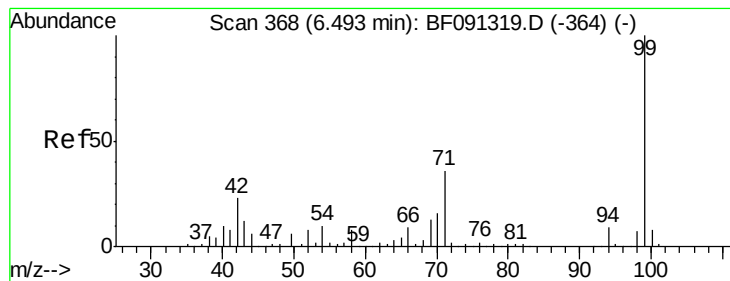

#7

Phenol-d6

Concen: 39.84 ng

RT: 6.47 min Scan# 366

Delta R.T. -0.03 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42

Instrument :

BNA_F

ClientSampled :

MW-6


Tgt Ion: 99 Resp: 375305

Ion Ratio Lower Upper




99 100

42 25.4 20.6 31.0

71 37.9 29.9 44.9



Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

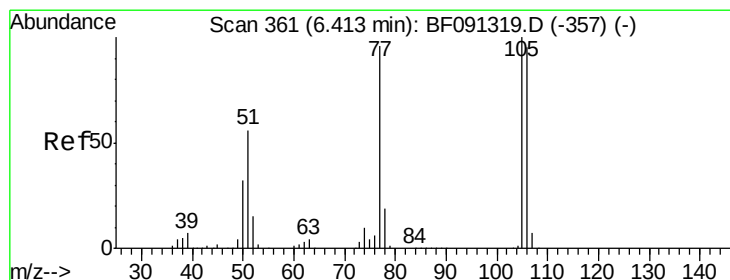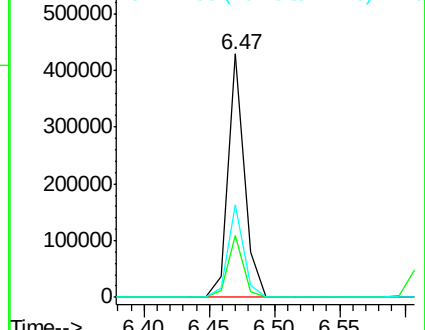

#9

Benzaldehyde

Concen: 4.17 ng

RT: 6.62 min Scan# 379

Delta R.T. 0.20 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42


Tgt Ion: 77 Resp: 25257

Ion Ratio Lower Upper



77 100


105 78.5 66.4 106.4

106 68.4 60.9 100.9

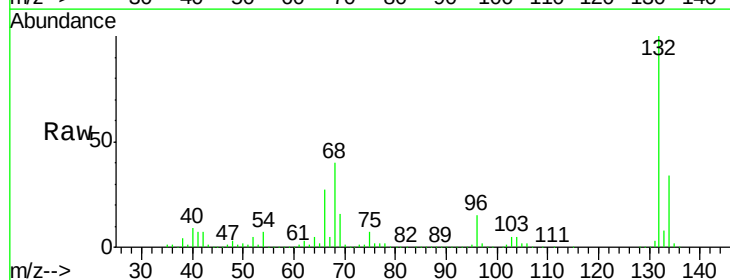

Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E

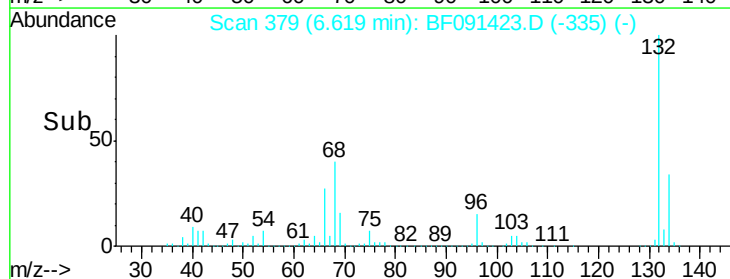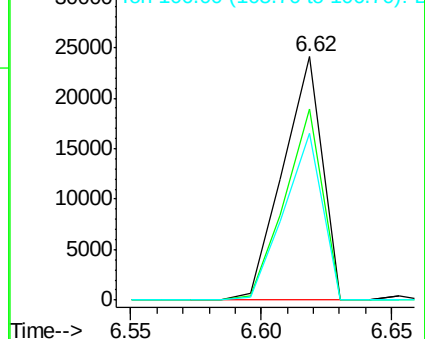

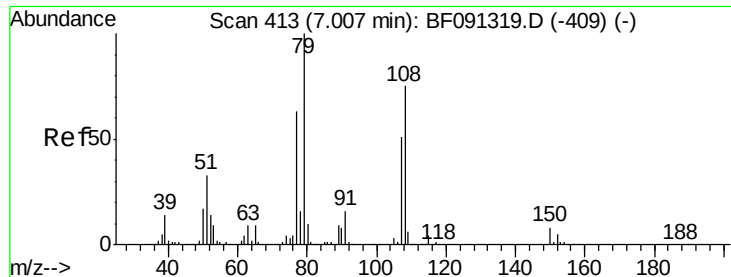

#15

Benzyl Alcohol

Concen: 2.13 ng

RT: 7.01 min Scan# 413

Delta R.T. -0.02 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42

Instrument :

BNA_F

ClientSampled :

MW-6





Tgt Ion: 79 Resp: 16092

Ion Ratio Lower Upper

79 100

108 26.8 62.7 94.1#

77 113.0 51.7 77.5#

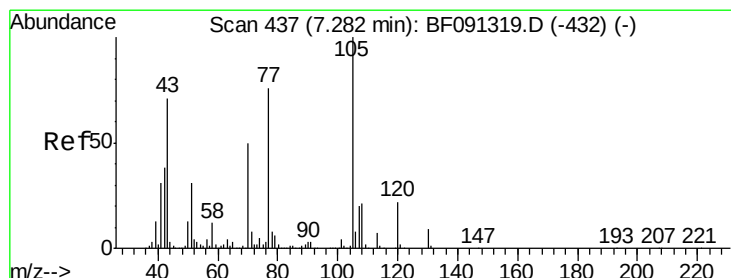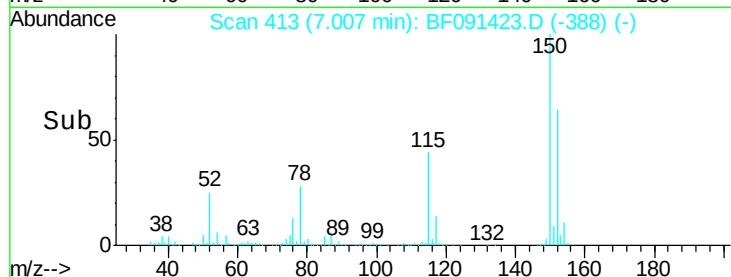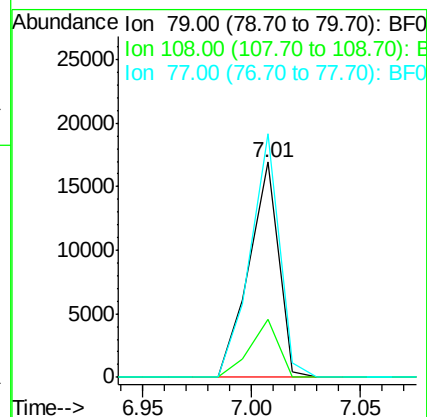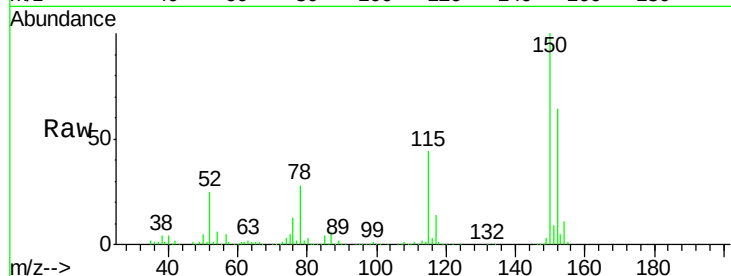

#19

n-Nitroso-di-n-propylamine

Concen: 19.92 ng

RT: 7.41 min Scan# 448

Delta R.T. 0.11 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42

Tgt Ion: 70 Resp: 118223




Ion Ratio Lower Upper


70 100

42 58.3 64.8 97.2#

101 0.0 6.2 9.4#

130 2.4 11.7 17.5#


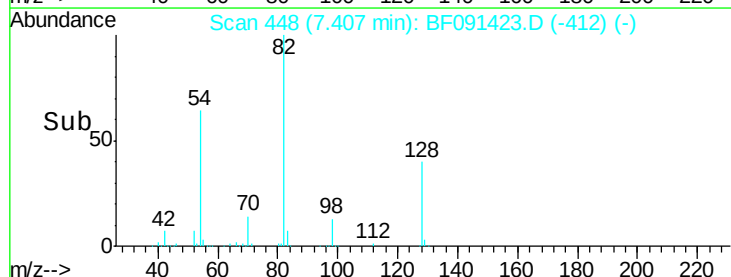
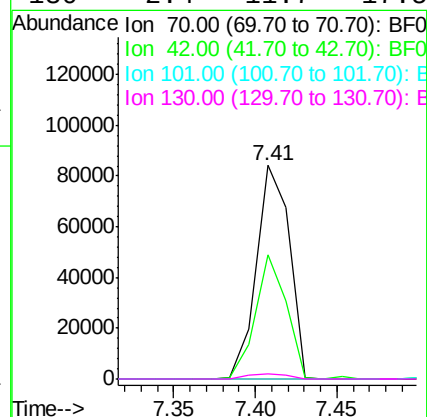
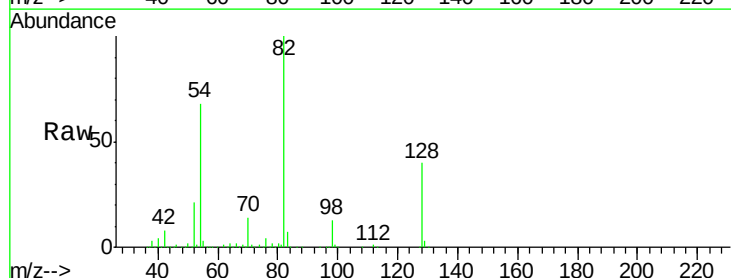




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.13 min Scan# 511
Delta R.T. -0.04 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42




Instrument :
BNA_F
ClientSampled :
MW-6


Tgt Ion:	136	Resp:	466650
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.1	13.7
54	14.1	9.1	13.7#
68	6.1	5.9	8.9

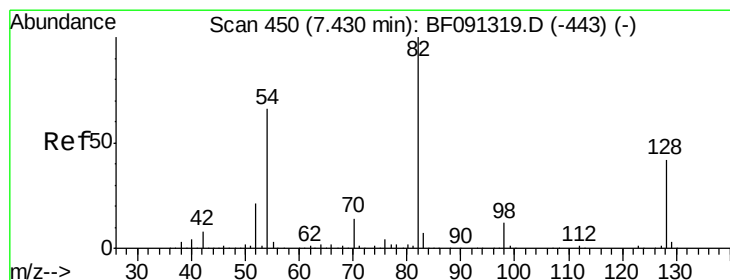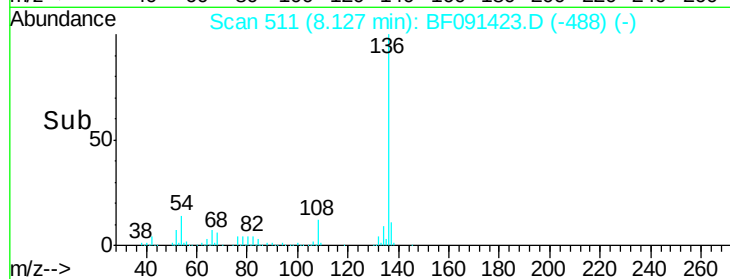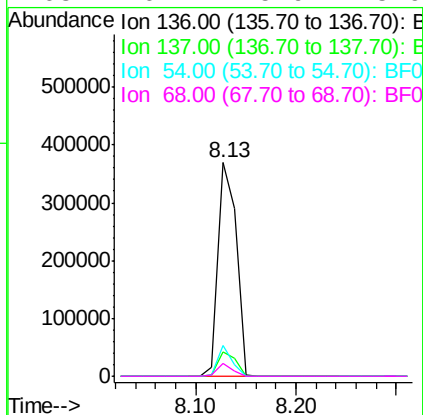

#23
Nitrobenzene-d5
Concen: 106.74 ng
RT: 7.41 min Scan# 448
Delta R.T. -0.04 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42

Tgt Ion:	82	Resp:	888863
Ion	Ratio	Lower	Upper
82	100		
128	39.8	31.8	47.6
54	67.6	49.1	73.7

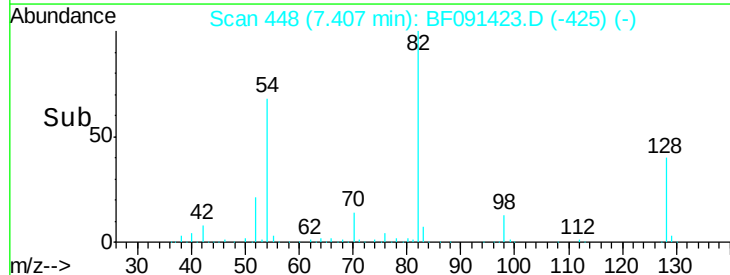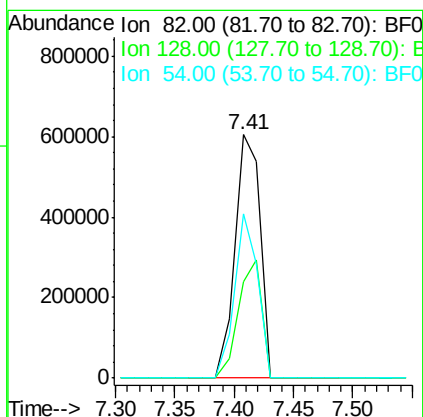

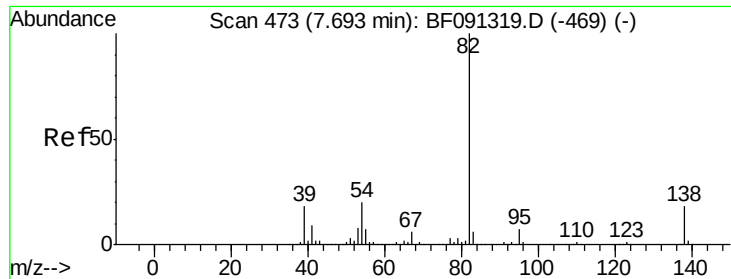

#25

Isophorone

Concen: 53.28 ng

RT: 7.41 min Scan# 448

Delta R.T. -0.30 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42

Instrument :

BNA_F

ClientSampleId :

MW-6


Tgt Ion: 82 Resp: 786065

Ion Ratio Lower Upper




82 100

95 0.0 5.7 8.5#

138 0.0 13.4 20.0#

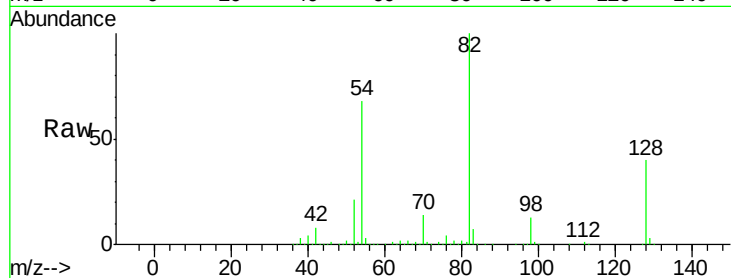

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

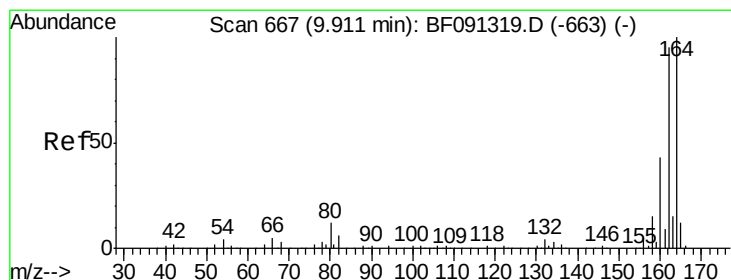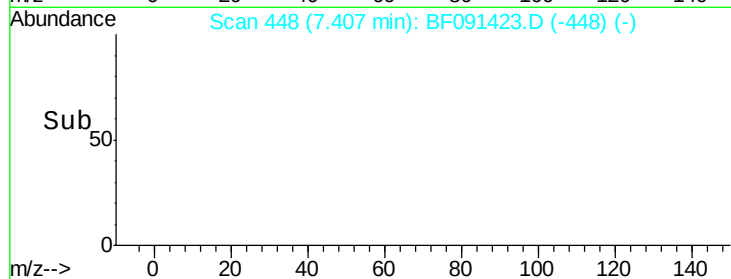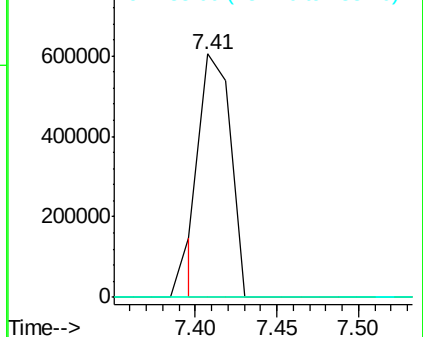

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.89 min Scan# 665

Delta R.T. -0.03 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42


Tgt Ion: 164 Resp: 312488

Ion Ratio Lower Upper



164 100


162 95.5 82.6 124.0

160 43.4 36.7 55.1

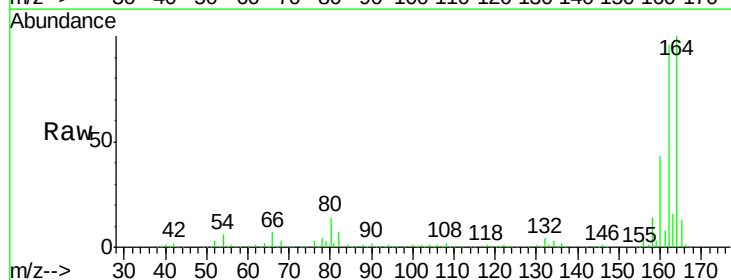

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

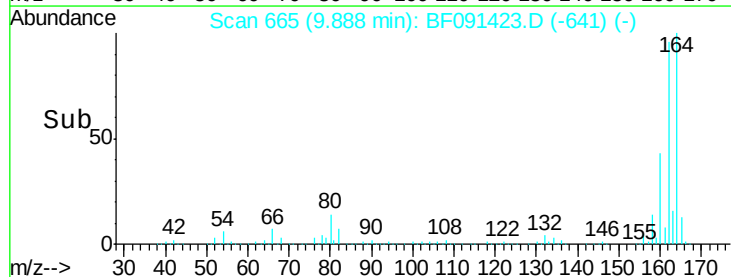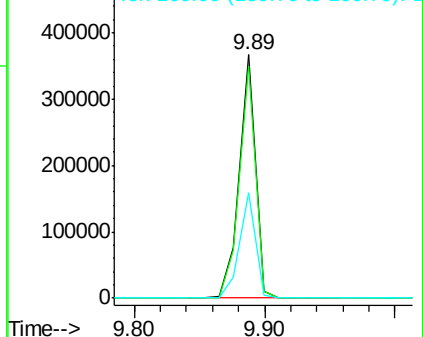







#41
 2,4,6-Tribromophenol
 Concen: 144.34 ng
 RT: 10.68 min Scan# 734
 Delta R.T. -0.03 min
 Lab File: BF091423.D
 Acq: 5 Dec 2016 17:42

Instrument :
 BNA_F
 ClientSampleId :
 MW-6

Tgt Ion:330 Resp: 427018
 Ion Ratio Lower Upper
 330 100
 332 96.6 76.2 114.4
 141 35.7 33.6 50.4

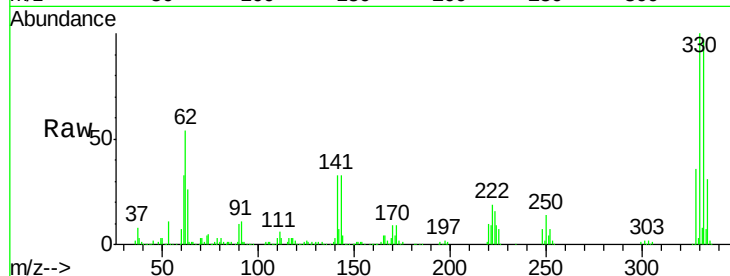


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


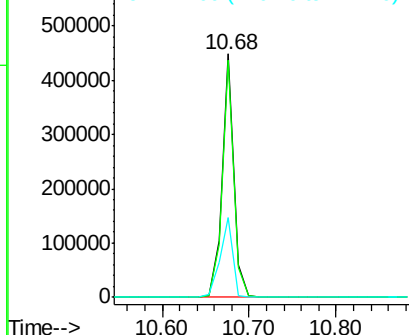



#44
 2-Fluorobiphenyl
 Concen: 93.96 ng
 RT: 9.21 min Scan# 606
 Delta R.T. -0.03 min
 Lab File: BF091423.D
 Acq: 5 Dec 2016 17:42

Tgt Ion:172 Resp: 1621629
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.4 44.0
 170 24.1 19.7 29.5



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

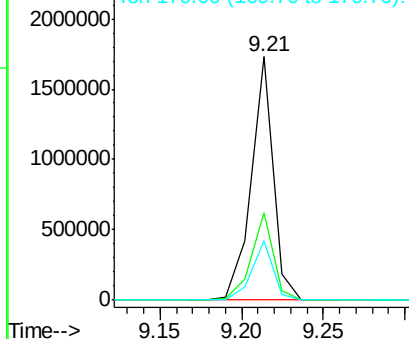


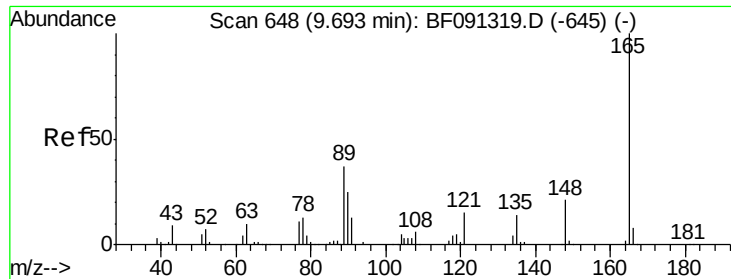

#50
2,6-Dinitrotoluene
Concen: 9.75 ng
RT: 9.89 min Scan# 665
Delta R.T. 0.19 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42

Instrument :
BNA_F
ClientSampleId :
MW-6




Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.0	59.4	89.0#
89	1.3	50.8	76.2#

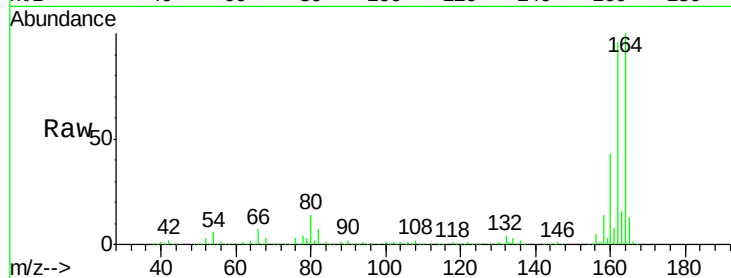

Abundance Ion 165.00 (164.70 to 165.70): E


Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

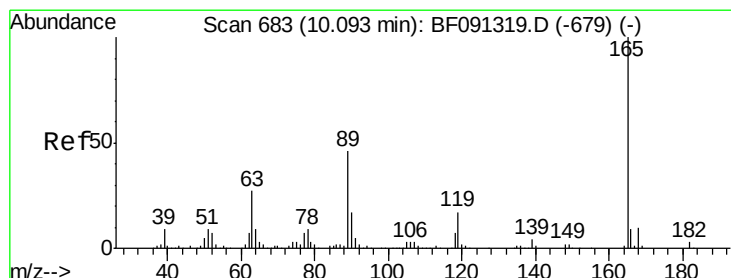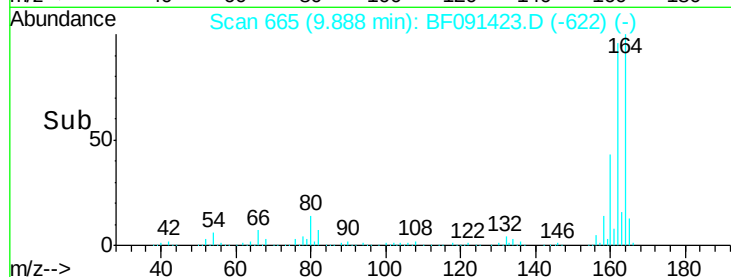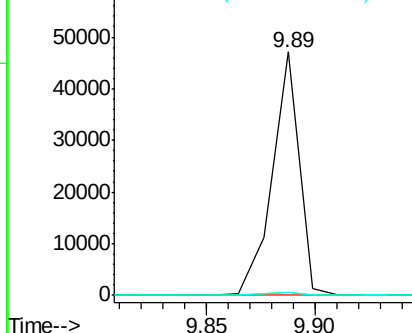

#56
2,4-Dinitrotoluene
Concen: 7.52 ng
RT: 9.89 min Scan# 665
Delta R.T. -0.21 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.0	29.0	43.4#
89	1.3	43.1	64.7#
182	0.0	1.9	2.9#


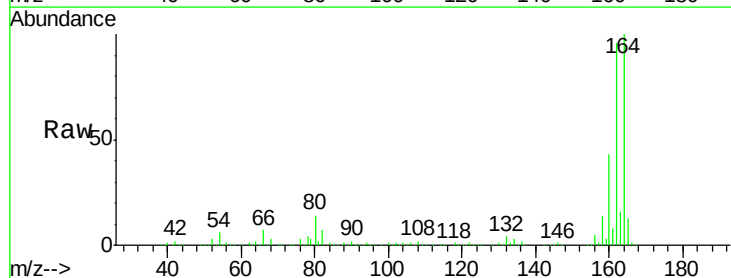



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

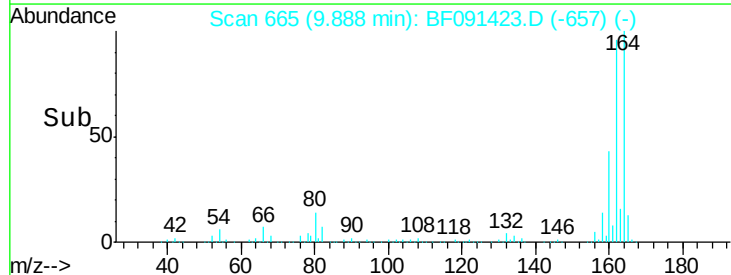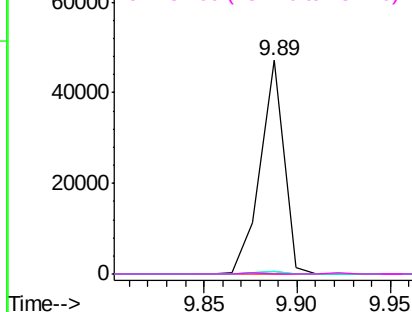







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 794
Delta R.T. -0.04 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42

Instrument :
BNA_F
ClientSampled :
MW-6

Tgt Ion:188 Resp: 539486
Ion Ratio Lower Upper
188 100
94 10.7 9.2 13.8
80 11.8 10.5 15.7

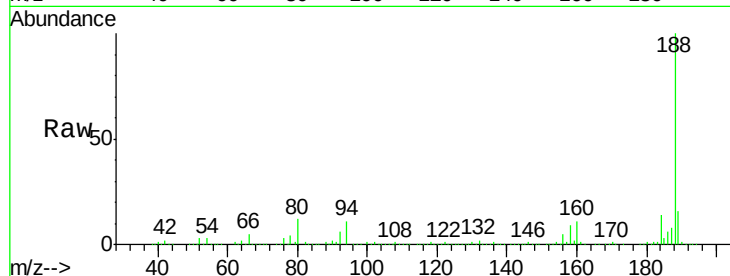


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


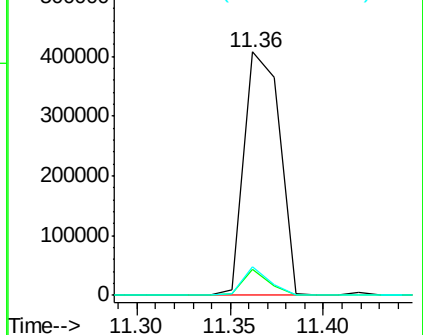



#66
4-Bromophenyl-phenylether
Concen: 4.99 ng
RT: 10.68 min Scan# 734
Delta R.T. -0.28 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42

Tgt Ion:248 Resp: 28909
Ion Ratio Lower Upper
248 100
250 197.0 78.2 117.4#
141 472.8 71.9 107.9#



Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

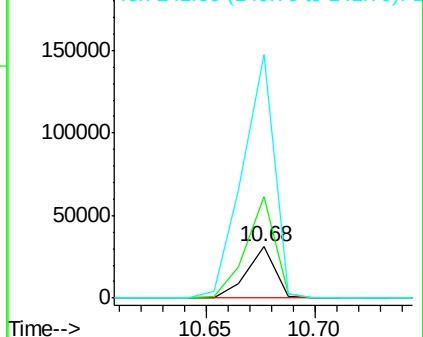



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.00 min Scan# 1025

Delta R.T. -0.04 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42

Instrument :

BNA_F

ClientSampleId :

MW-6


Tgt Ion:240 Resp: 497345

Ion Ratio Lower Upper

240 100

120 6.2 12.1 18.1#




236 25.5 21.0 31.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

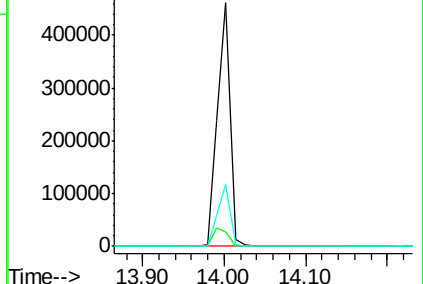

#78

Terphenyl-d14

Concen: 94.15 ng

RT: 12.96 min Scan# 934

Delta R.T. -0.03 min

Lab File: BF091423.D

Acq: 5 Dec 2016 17:42


Tgt Ion:244 Resp: 2154398

Ion Ratio Lower Upper

244 100

212 7.0 6.5 9.7



122 6.6 9.5 14.3#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

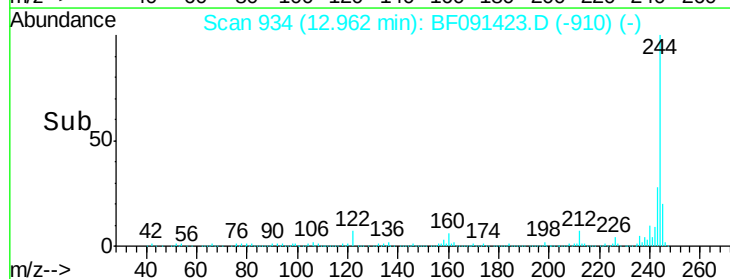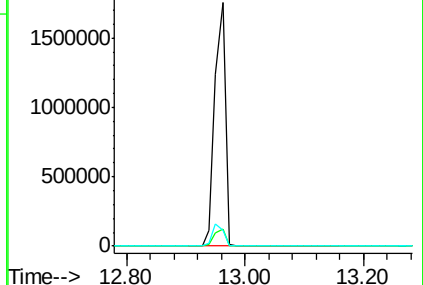


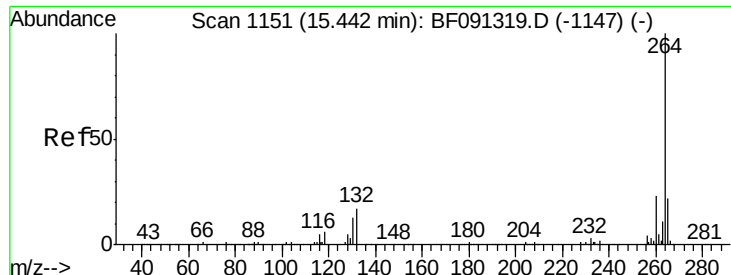

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.42 min Scan# 1149
Delta R.T. -0.05 min
Lab File: BF091423.D
Acq: 5 Dec 2016 17:42

Instrument :
BNA_F
ClientSampleId :
MW-6

Tgt Ion: 264 Resp: 331164
Ion Ratio Lower Upper
264 100
260 23.9 18.8 28.2
265 22.6 17.0 25.6

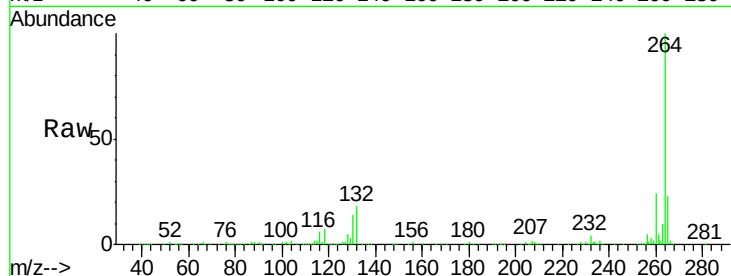

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

