
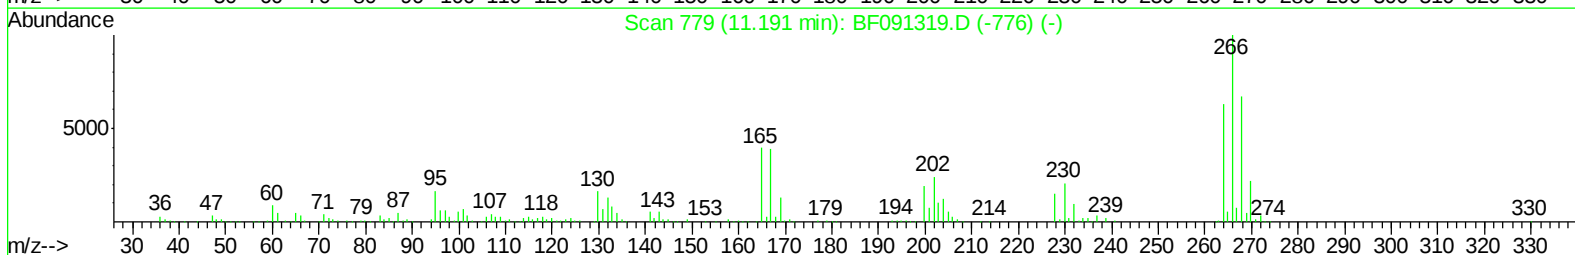
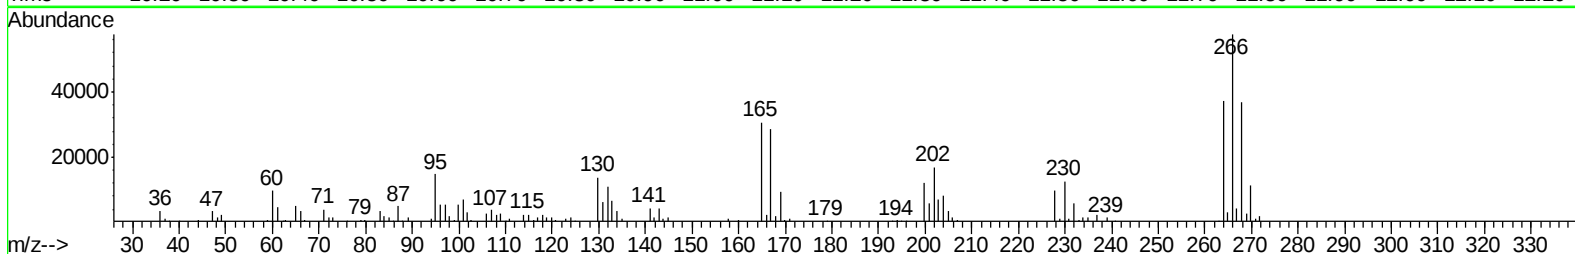


Data Path : Z:\HPCHEM1\BNA F\Data\BF120516\
Data File : BF091417.D
Acq On : 5 Dec 2016 13:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 14:22:17 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

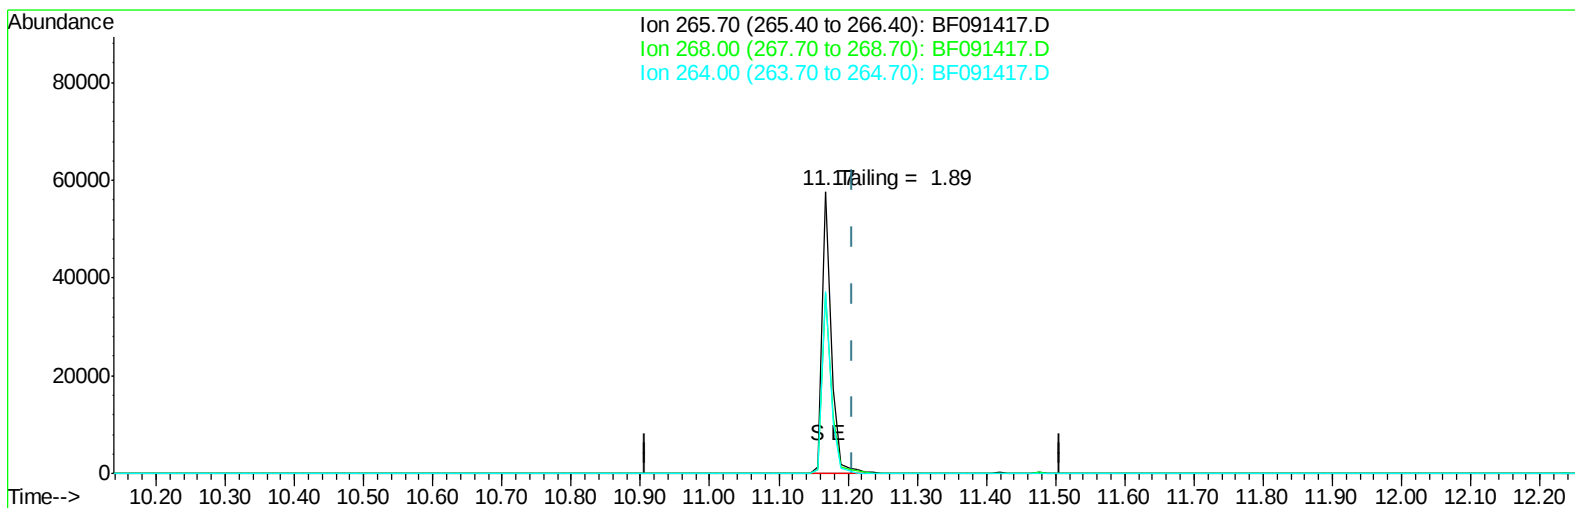

TIC: BF091417.D

(69) Pentachlorophenol (C)




11.168min (-0.040) 0.00ng

response 55268

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	63.65
264.00	60.20	64.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF120516\
Data File : BF091417.D
Acq On : 5 Dec 2016 13:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 14:22:17 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

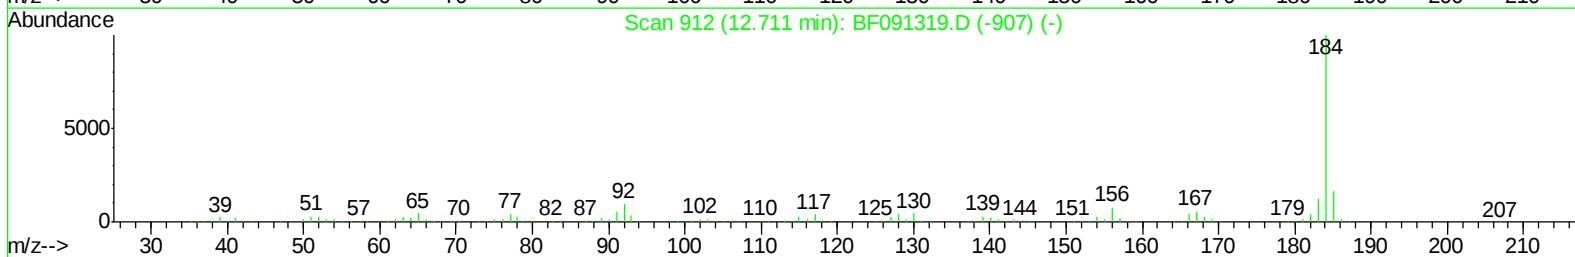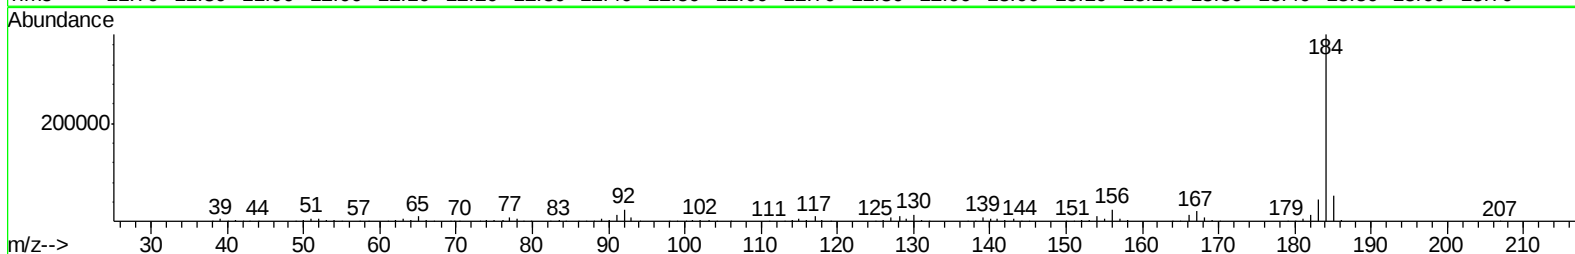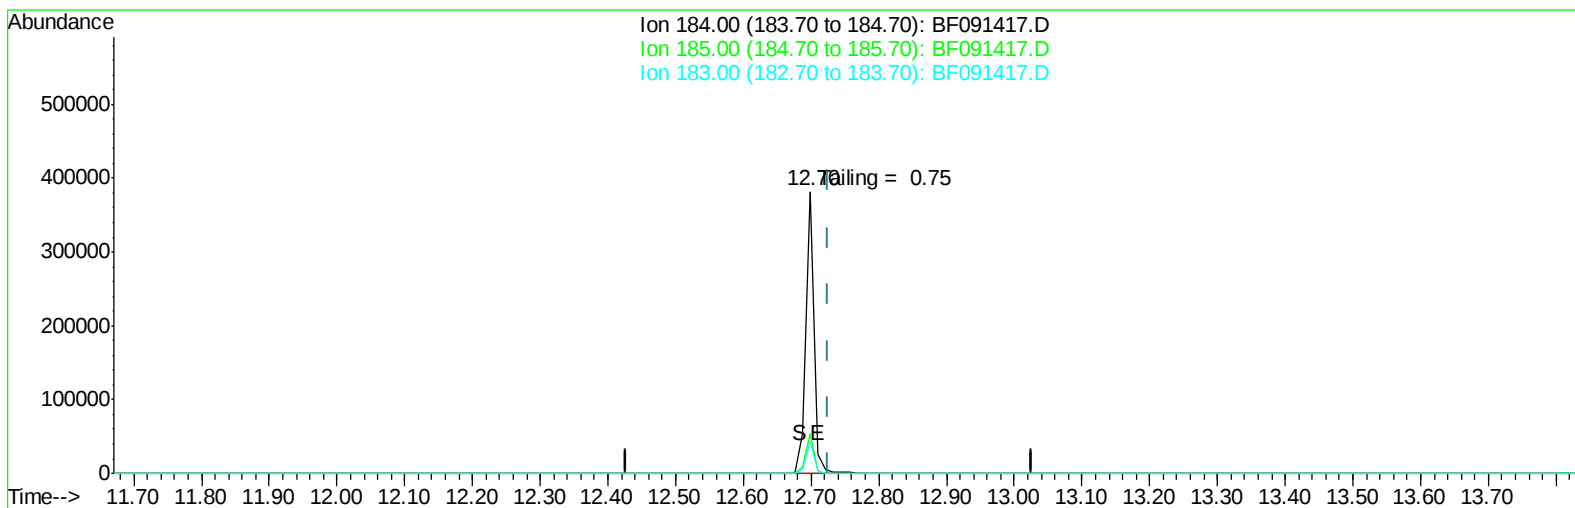

TIC: BF091417.D

(76) Benzidine

12.699min (-0.028) 0.00ng

response 326101

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.11
183.00	11.10	11.48
0.00	0.00	0.00