
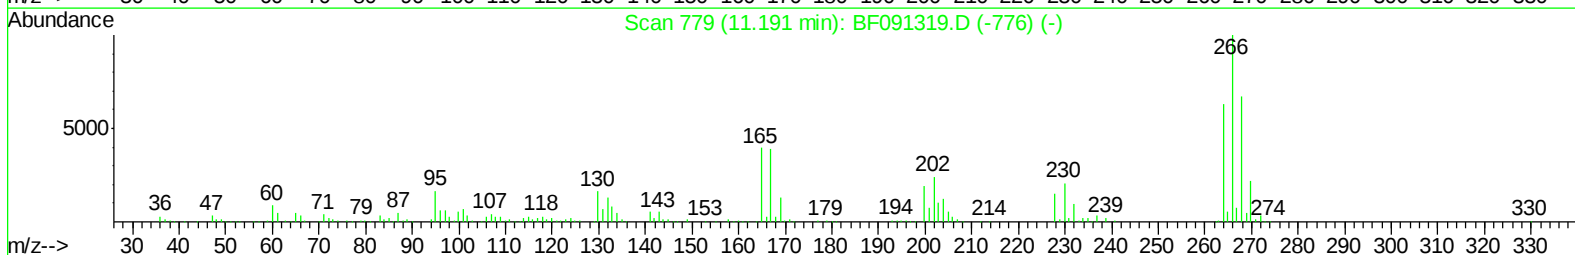
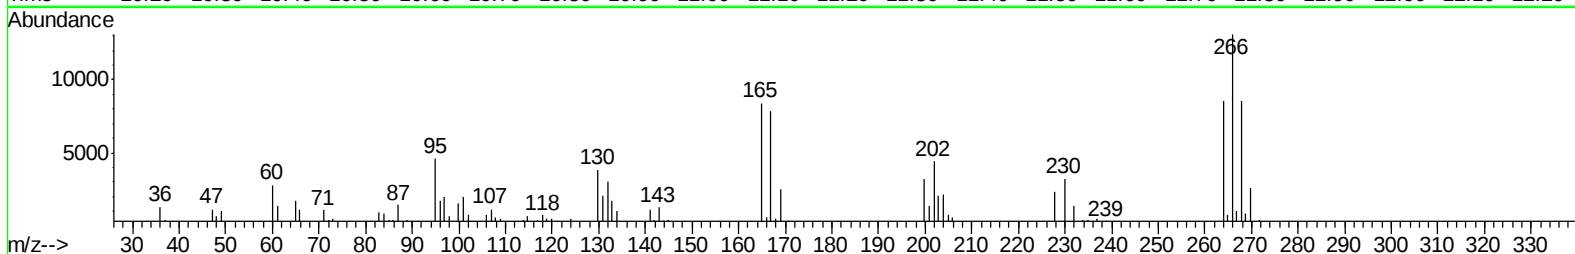


Data Path : Z:\HPCHEM1\BNA F\Data\BF120516\
Data File : BF091443.D
Acq On : 6 Dec 2016 4:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 14:23:35 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

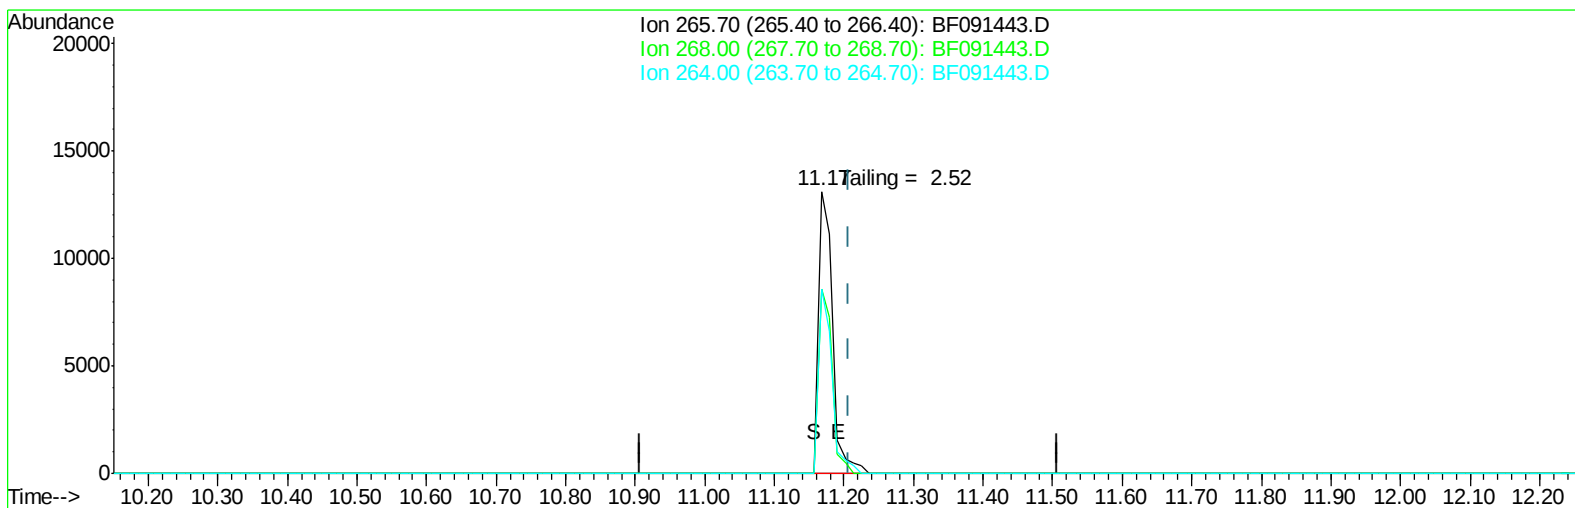

TIC: BF091443.D

(69) Pentachlorophenol (C)




11.168min (-0.040) 0.00ng

response 18690

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	65.36
264.00	60.20	65.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF120516\
 Data File : BF091443.D
 Acq On : 6 Dec 2016 4:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 14:23:35 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 13:33:46 2016
 Response via : Initial Calibration

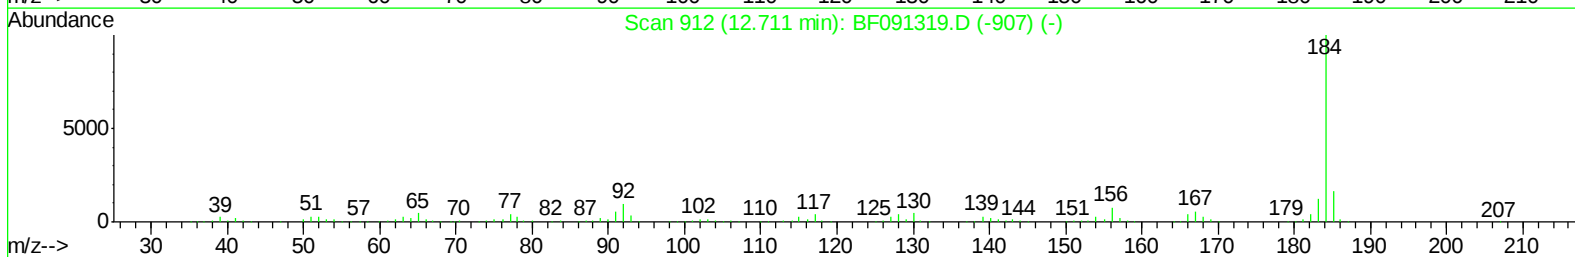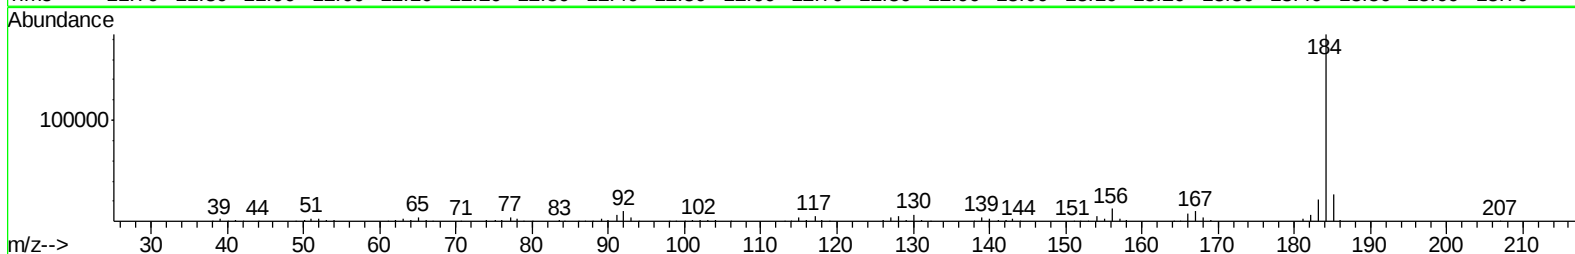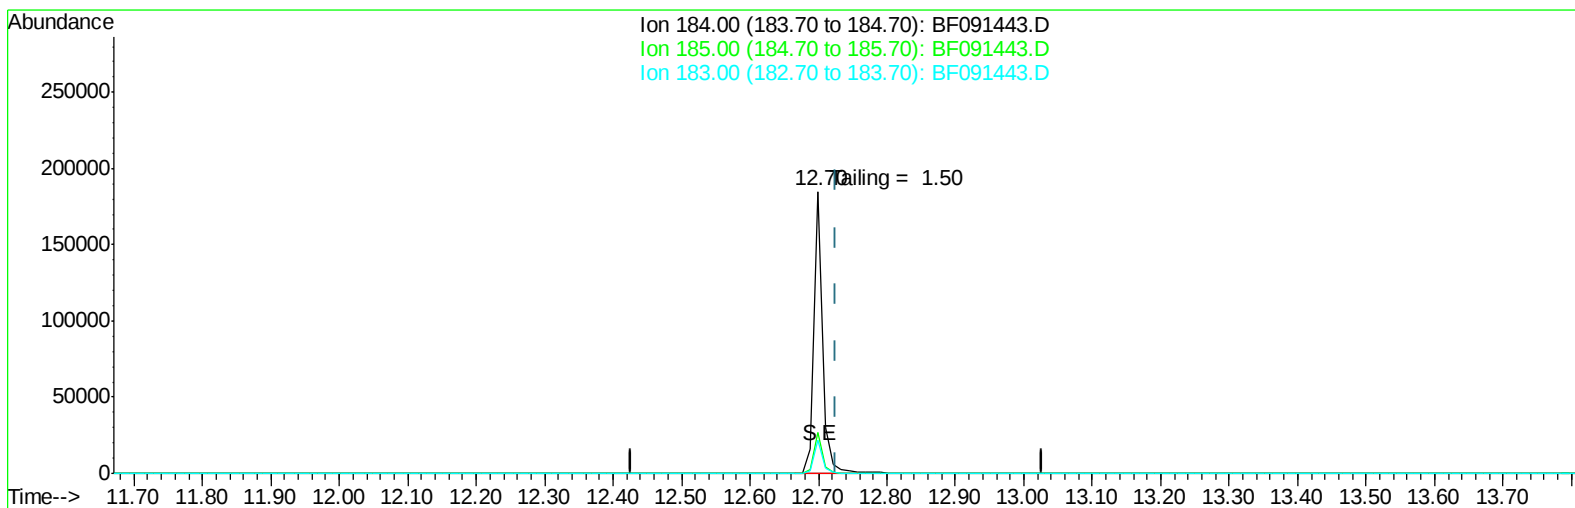

TIC: BF091443.D

(76) Benzidine

12.699min (-0.028) 0.00ng

response 167060

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.59
183.00	11.10	11.63
0.00	0.00	0.00