

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120516\
 Data File : BF091432.D
 Acq On : 5 Dec 2016 21:50
 Operator : UM/SJ
 Sample : H5838-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-17

Quant Time: Dec 06 00:46:27 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 00:16:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	148387	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	568689	20.00	ng	-0.01
38) Acenaphthene-d10	9.89	164	374463	20.00	ng	0.00
63) Phenanthrene-d10	11.36	188	588184	20.00	ng	-0.01
75) Chrysene-d12	14.00	240	507226	20.00	ng	0.00
86) Perylene-d12	15.42	264	375287	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	510151	56.16	ng	0.00
7) Phenol-d6	6.47	99	395156	35.34	ng	-0.01
23) Nitrobenzene-d5	7.41	82	1033800	101.87	ng	-0.01
41) 2,4,6-Tribromophenol	10.68	330	488493	137.79	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	1854970	89.69	ng	0.00
78) Terphenyl-d14	12.96	244	2031948	87.07	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120516\
Data File : BF091432.D
Acq On : 5 Dec 2016 21:50
Operator : UM/SJ
Sample : H5838-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-17

Quant Time: Dec 06 00:46:27 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 00:16:00 2016
Response via : Initial Calibration

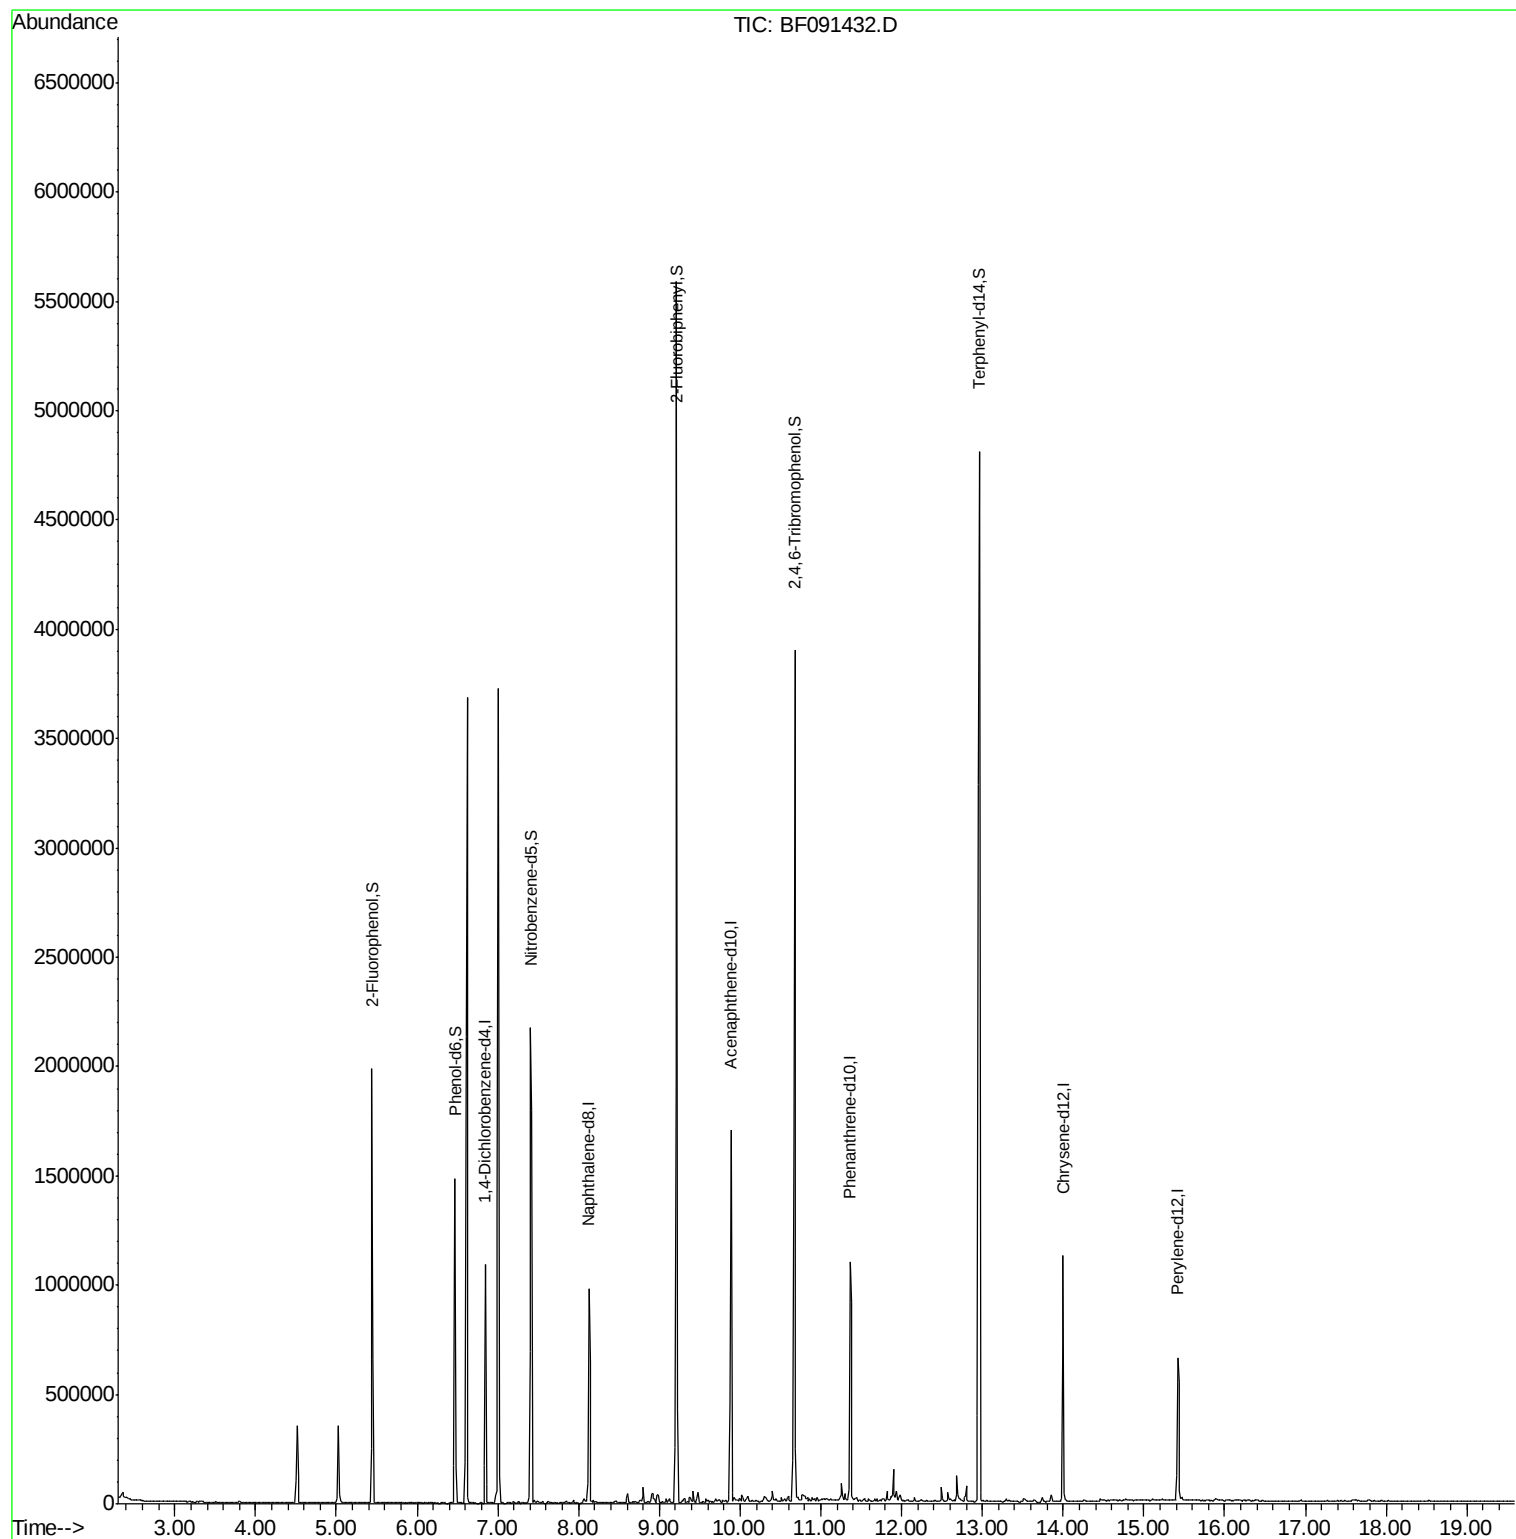


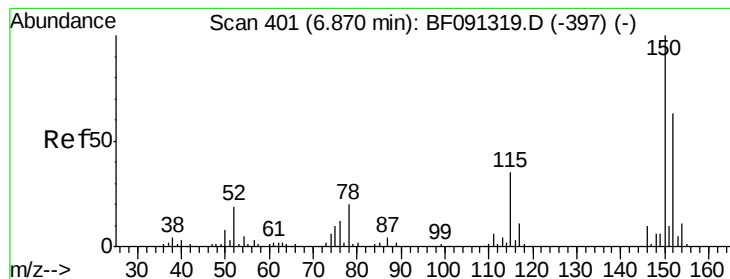




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.85 min Scan# 399
 Delta R.T. -0.00 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Instrument :
 BNA_F
 ClientSampleId :
 MW-17

Tot Ion:152 Resp: 148387
 Ion Ratio Lower Upper
 152 100
 150 153.3 122.5 183.7
 115 62.2 51.8 77.8

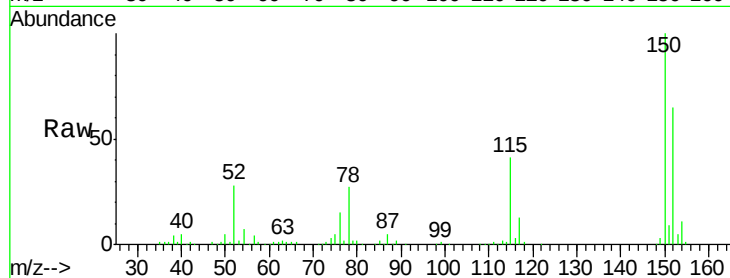


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

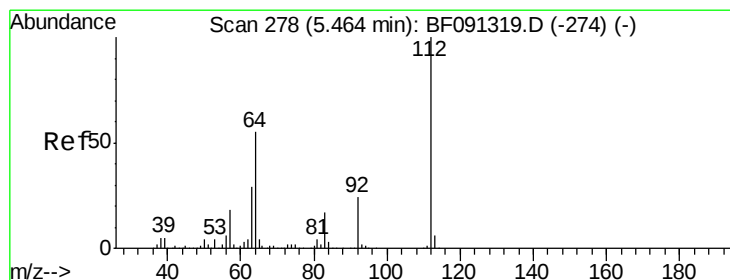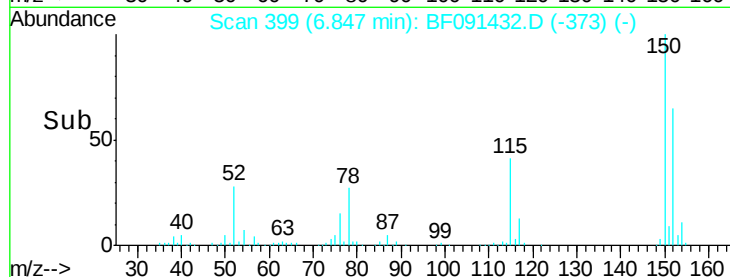
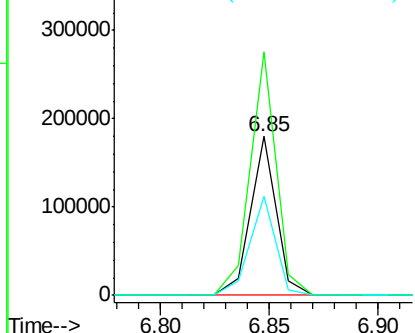


#5
 2-Fluorophenol
 Concen: 56.16 ng
 RT: 5.44 min Scan# 276
 Delta R.T. -0.00 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Tgt Ion:112 Resp: 510151
 Ion Ratio Lower Upper
 112 100
 64 79.6 61.5 92.3
 63 42.2 33.3 49.9

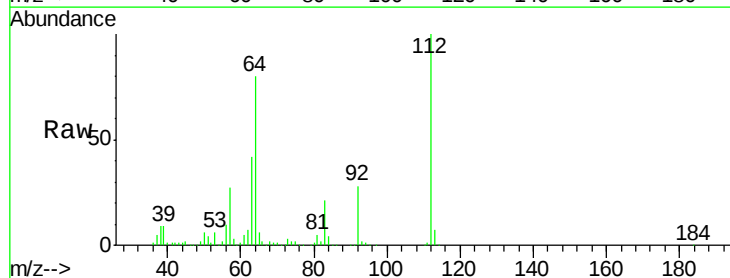

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

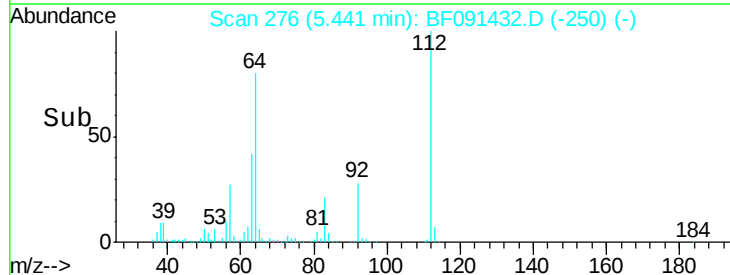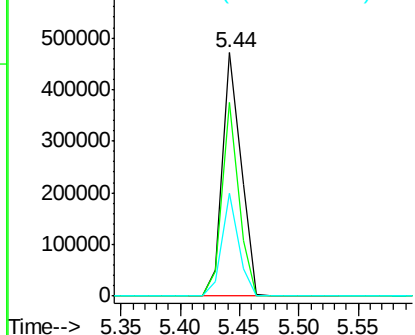



#7

Phenol-d6

Concen: 35.34 ng

RT: 6.47 min Scan# 366

Delta R.T. -0.01 min

Lab File: BF091432.D

Acq: 5 Dec 2016 21:50

Instrument :

BNA_F

ClientSampleId :

MW-17


Tot Ion: 99 Resp: 395156

Ion Ratio Lower Upper

99 100

42 24.8 20.6 31.0




71 38.0 29.9 44.9

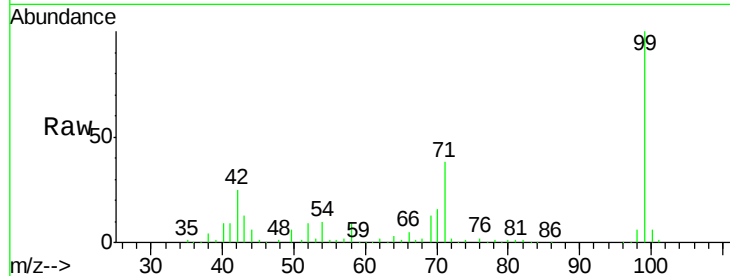

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

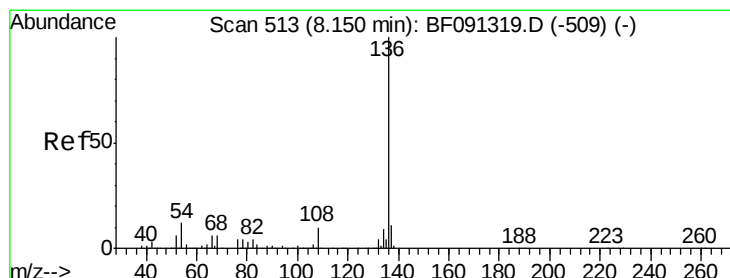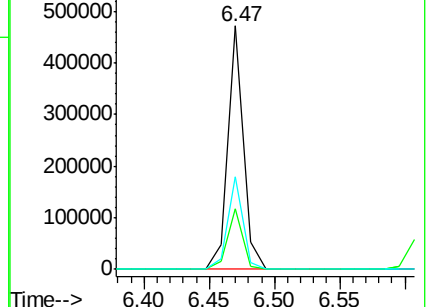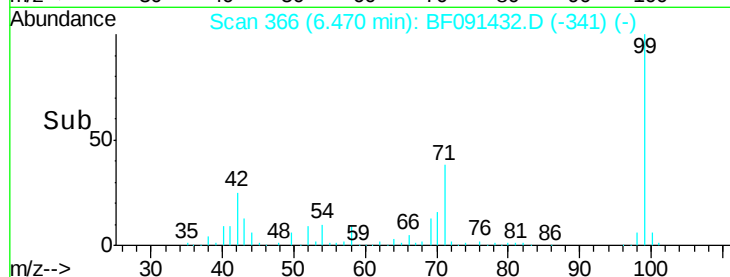

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.13 min Scan# 511

Delta R.T. -0.01 min

Lab File: BF091432.D

Acq: 5 Dec 2016 21:50

Tgt Ion: 136 Resp: 568689


Ion Ratio Lower Upper

136 100

137 11.2 9.1 13.7

54 14.2 9.1 13.7#

68 6.3 5.9 8.9


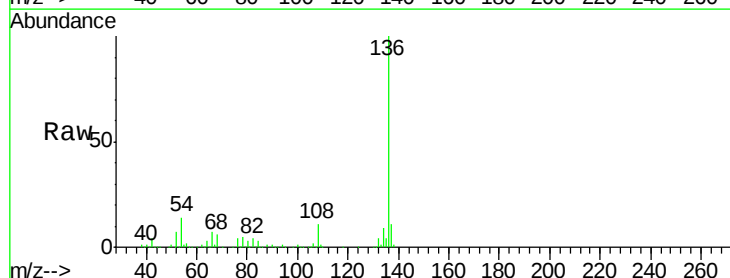


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

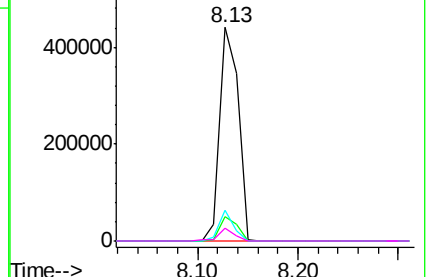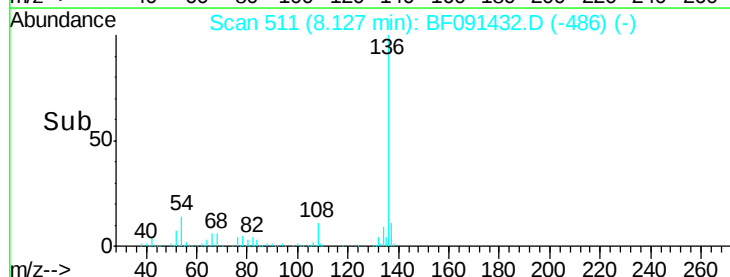







#23
 Nitrobenzene-d5
 Concen: 101.87 ng
 RT: 7.41 min Scan# 448
 Delta R.T. -0.01 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Instrument :
 BNA_F
 ClientSampled :
 MW-17

Tot Ion: 82 Resp: 1033800
 Ion Ratio Lower Upper
 82 100
 128 40.1 31.8 47.6
 54 68.0 49.1 73.7

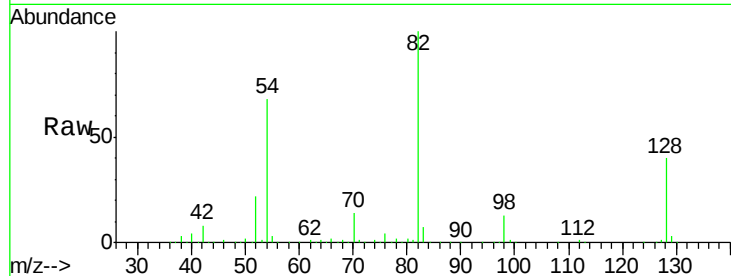


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

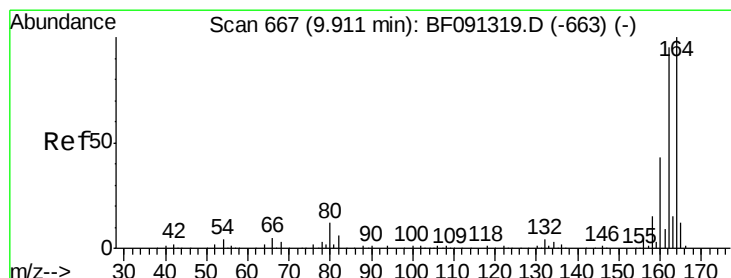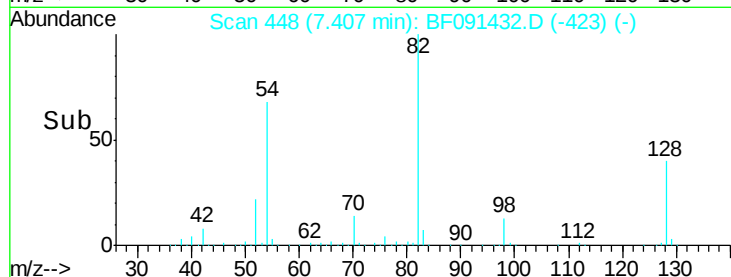
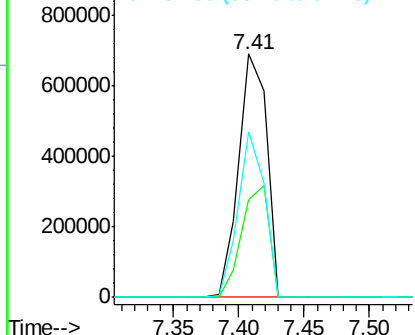



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 665
 Delta R.T. -0.00 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Tgt Ion: 164 Resp: 374463
 Ion Ratio Lower Upper
 164 100
 162 95.6 82.6 124.0
 160 43.5 36.7 55.1

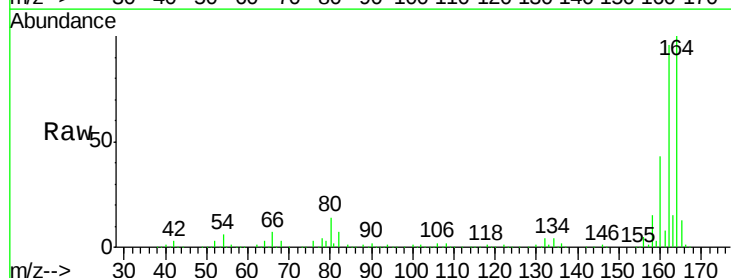

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

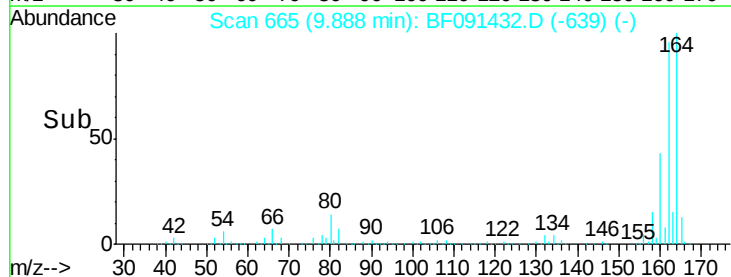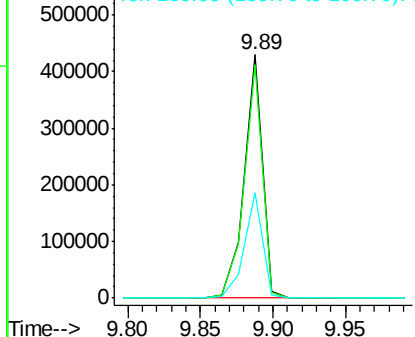


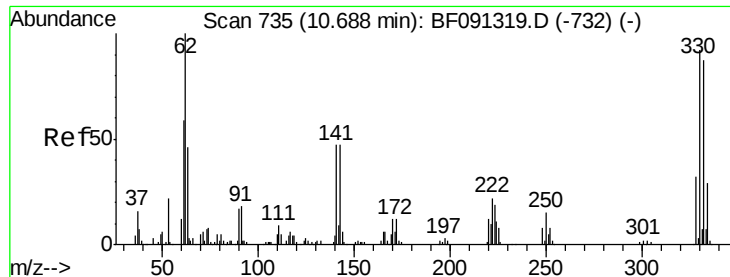




#41
 2,4,6-Tribromophenol
 Concen: 137.79 ng
 RT: 10.68 min Scan# 734
 Delta R.T. -0.00 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Instrument :
 BNA_F
 ClientSampleId :
 MW-17

Tot Ion:330 Resp: 488493
 Ion Ratio Lower Upper
 330 100
 332 95.8 76.2 114.4
 141 35.6 33.6 50.4

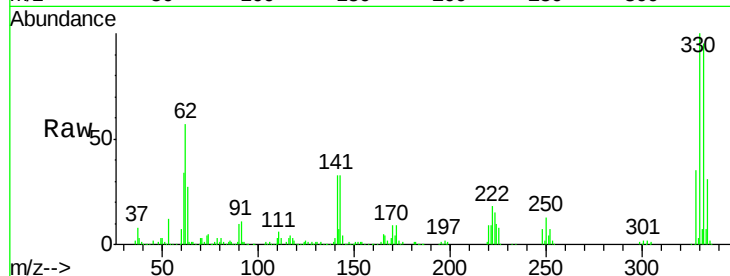


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

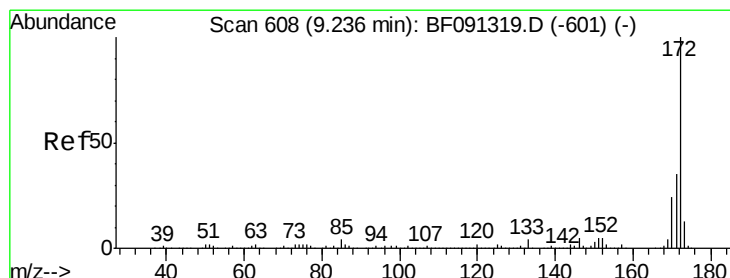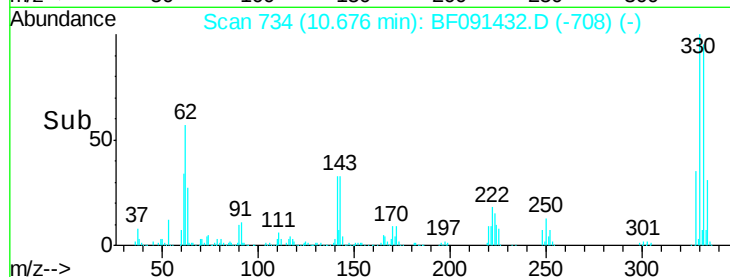
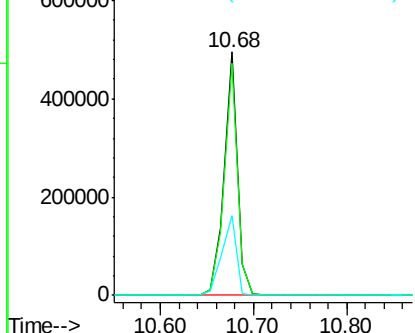



#44
 2-Fluorobiphenyl
 Concen: 89.69 ng
 RT: 9.21 min Scan# 606
 Delta R.T. -0.00 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Tgt Ion:172 Resp: 1854970
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.4 44.0
 170 24.3 19.7 29.5

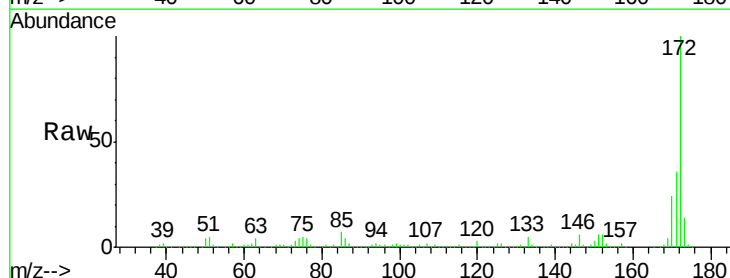

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

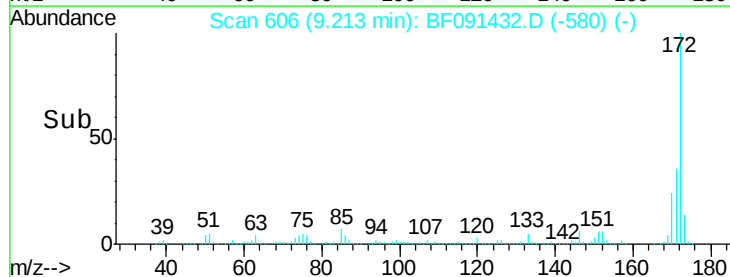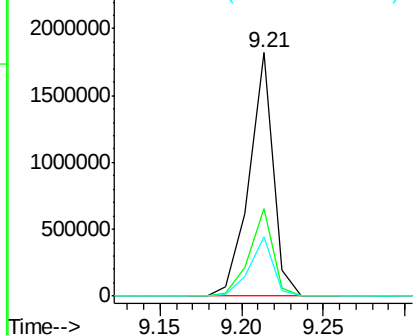


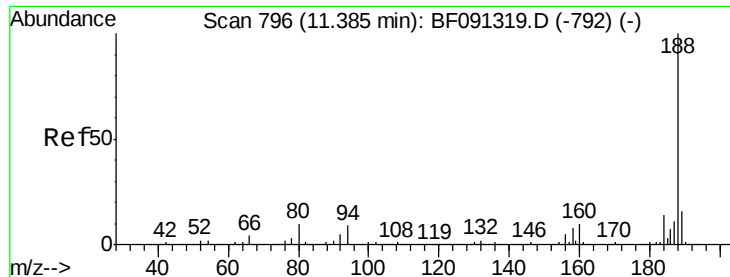


#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 794
Delta R.T. -0.01 min
Lab File: BF091432.D
Acq: 5 Dec 2016 21:50

Instrument :
BNA_F
ClientSampled :
MW-17



Tot Ion:188 Resp: 588184
Ion Ratio Lower Upper
188 100
94 10.1 9.2 13.8
80 11.6 10.5 15.7

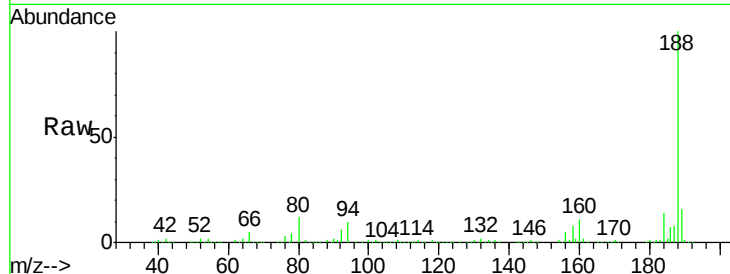

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

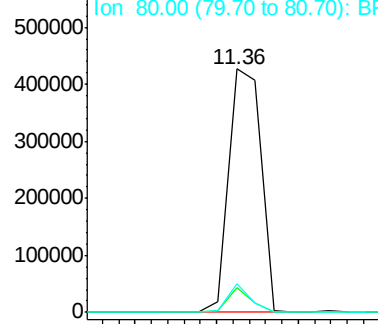


Time--> 11.30 11.35 11.40

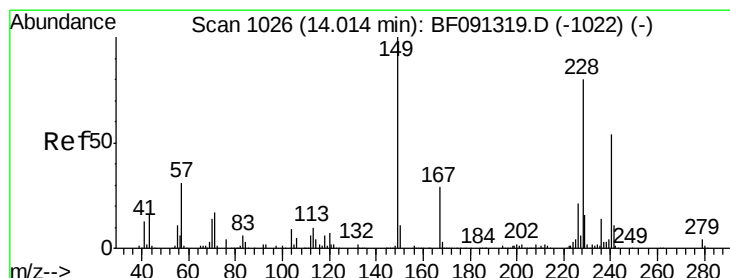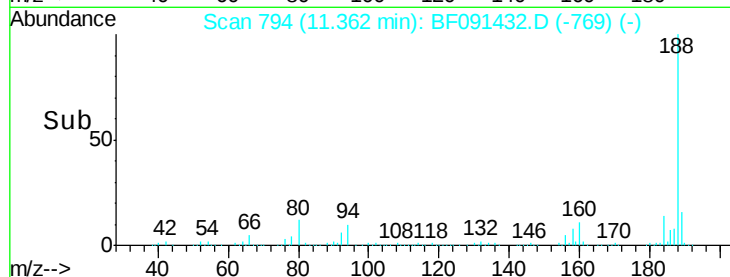


#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.00 min Scan# 1025
Delta R.T. -0.00 min
Lab File: BF091432.D
Acq: 5 Dec 2016 21:50


Tgt Ion:240 Resp: 507226
Ion Ratio Lower Upper
240 100
120 5.5 12.1 18.1#
236 25.2 21.0 31.6

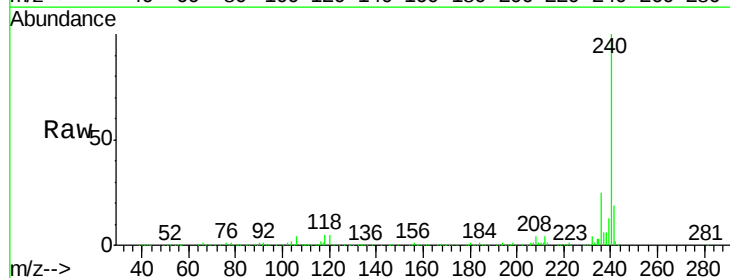


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

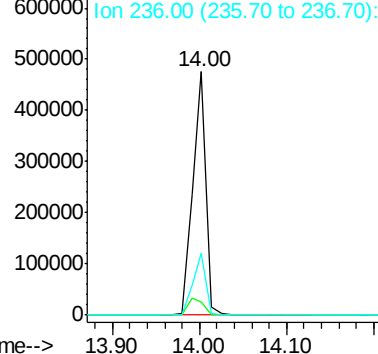

Time--> 13.90 14.00 14.10




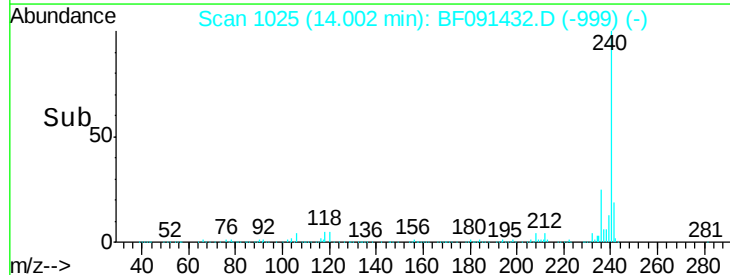


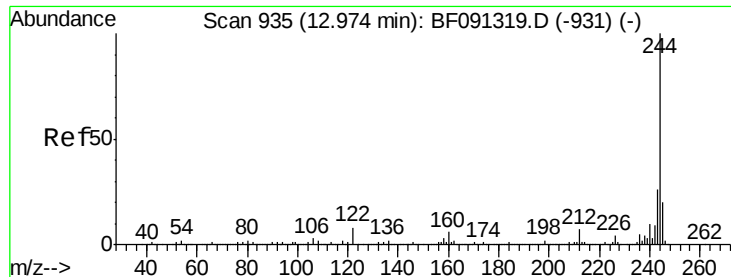

#78
 Terphenyl-d14
 Concen: 87.07 ng
 RT: 12.96 min Scan# 934
 Delta R.T. -0.00 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Instrument :
 BNA_F
 ClientSampleId :
 MW-17

Tot Ion:244 Resp: 2031948
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.5 9.7
 122 7.2 9.5 14.3#

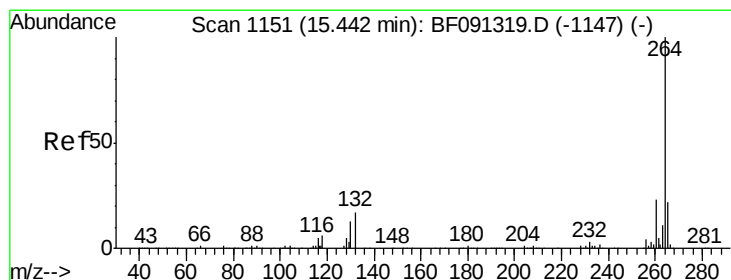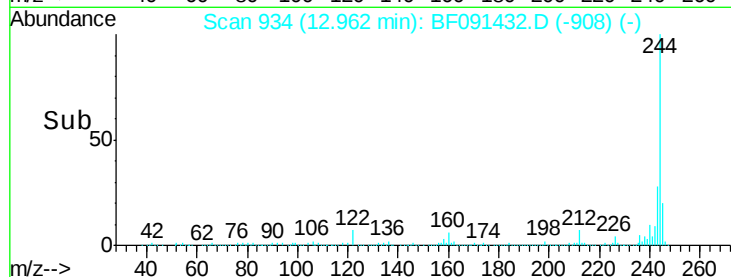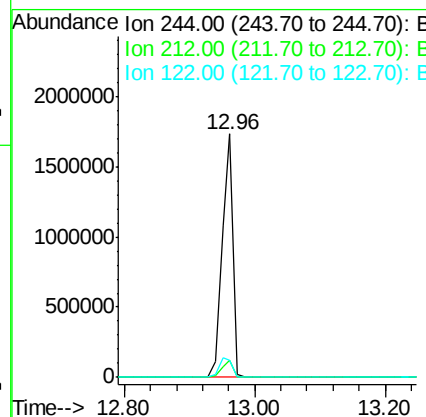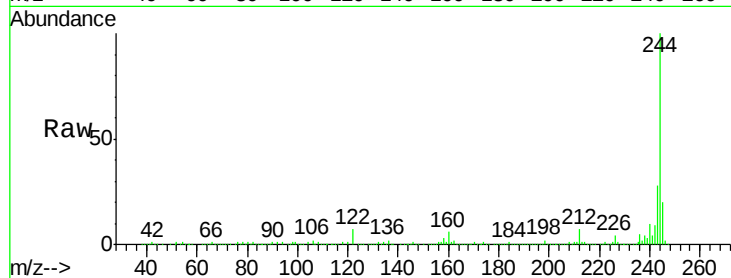

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.42 min Scan# 1149
 Delta R.T. -0.01 min
 Lab File: BF091432.D
 Acq: 5 Dec 2016 21:50

Tgt Ion:264 Resp: 375287
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.8 28.2
 265 22.2 17.0 25.6

