

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120516\
 Data File : BF091442.D
 Acq On : 6 Dec 2016 2:26
 Operator : UM/SJ
 Sample : H5802-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-05

Quant Time: Dec 06 04:23:18 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 00:16:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	124520	20.00	ng	0.00
21) Naphthalene-d8	8.14	136	514766	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	282420	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	513183	20.00	ng	0.00
75) Chrysene-d12	14.00	240	302375	20.00	ng	0.00
86) Perylene-d12	15.43	264	299852	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	561216	73.63	ng	0.01
7) Phenol-d6	6.48	99	544787	58.06	ng	0.00
23) Nitrobenzene-d5	7.42	82	1005298	109.44	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	392778	146.90	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	1479935	94.88	ng	0.00
78) Terphenyl-d14	12.96	244	1646157	118.33	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120516\
Data File : BF091442.D
Acq On : 6 Dec 2016 2:26
Operator : UM/SJ
Sample : H5802-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05

Quant Time: Dec 06 04:23:18 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 00:16:00 2016
Response via : Initial Calibration

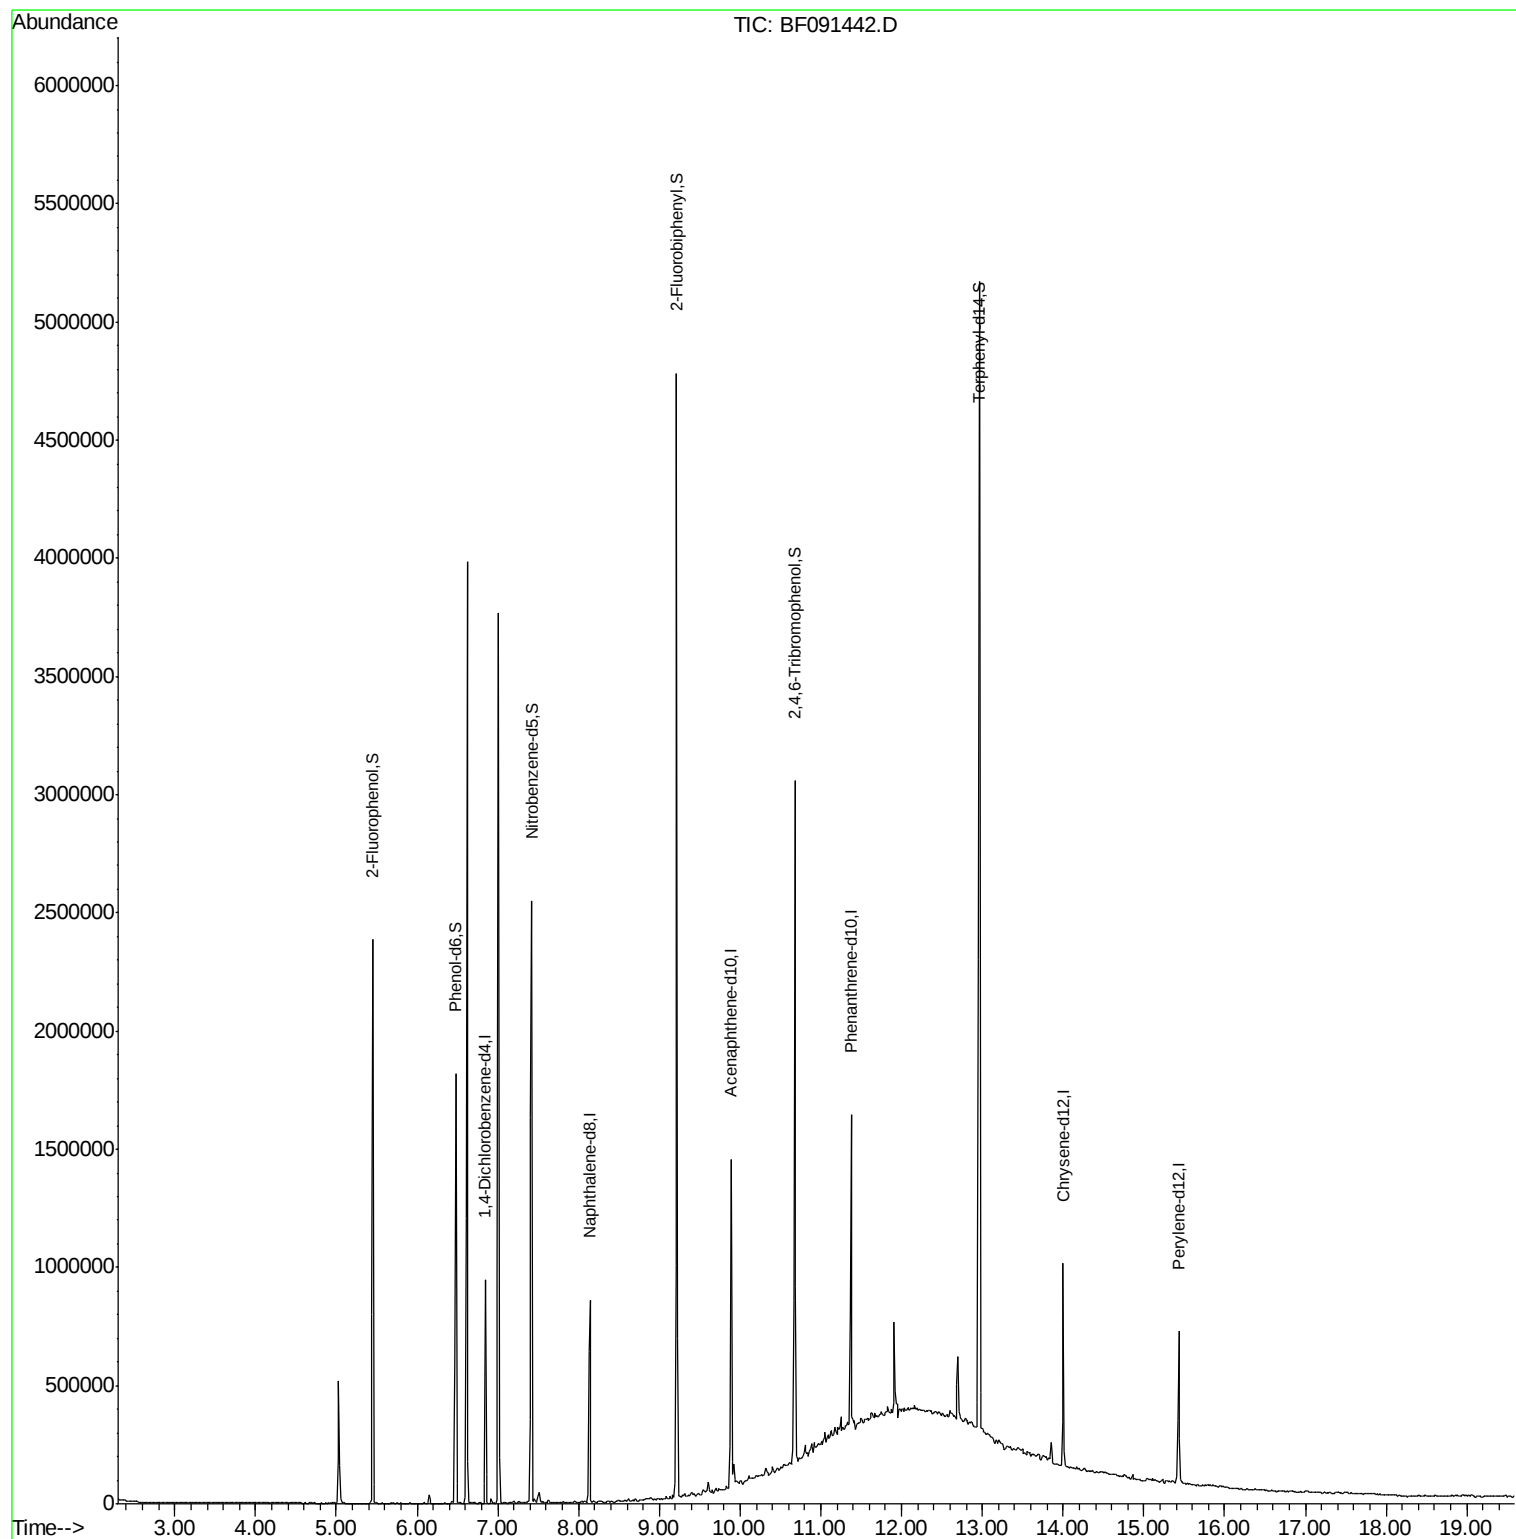

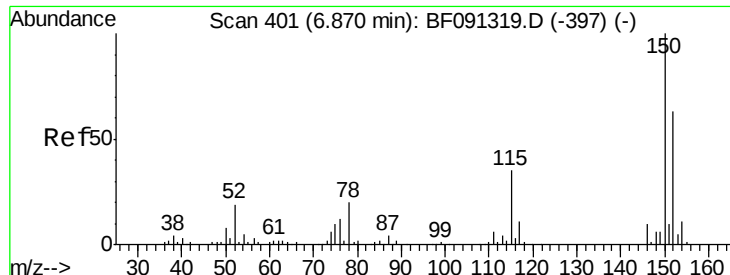

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 399

Delta R.T. -0.00 min

Lab File: BF091442.D

Acq: 6 Dec 2016 2:26

Instrument :

BNA_F

ClientSampleId :

MW-05


Tot Ion:152 Resp: 124520

Ion Ratio Lower Upper

152 100

150 157.8 122.5 183.7




115 63.5 51.8 77.8

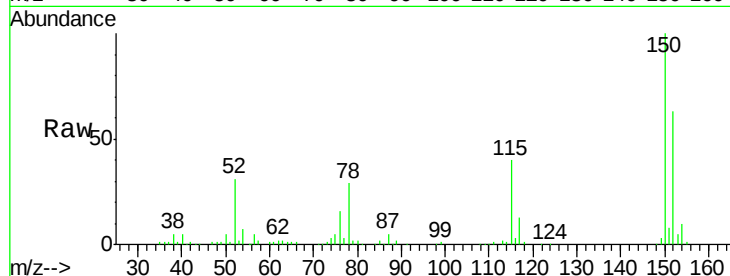

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

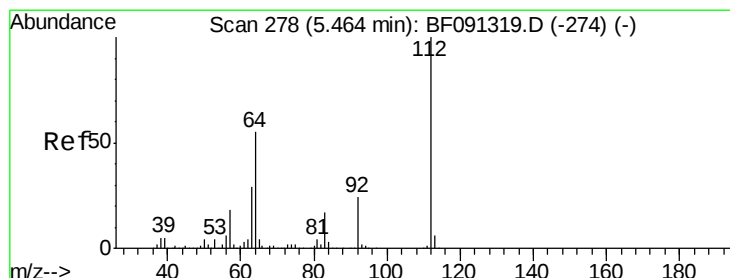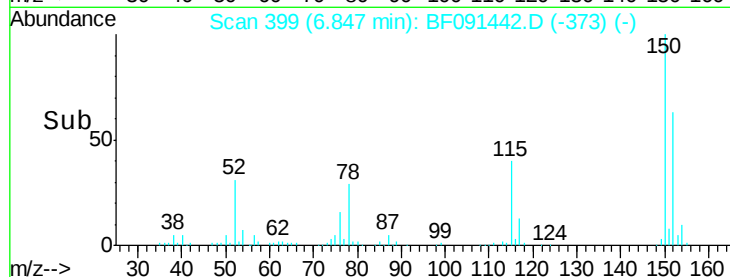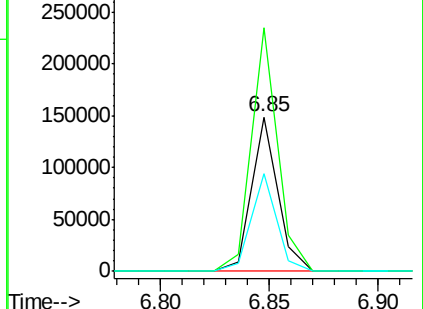

#5

2-Fluorophenol

Concen: 73.63 ng

RT: 5.45 min Scan# 277

Delta R.T. 0.01 min

Lab File: BF091442.D

Acq: 6 Dec 2016 2:26


Tgt Ion:112 Resp: 561216

Ion Ratio Lower Upper

112 100

64 71.7 61.5 92.3



63 39.0 33.3 49.9

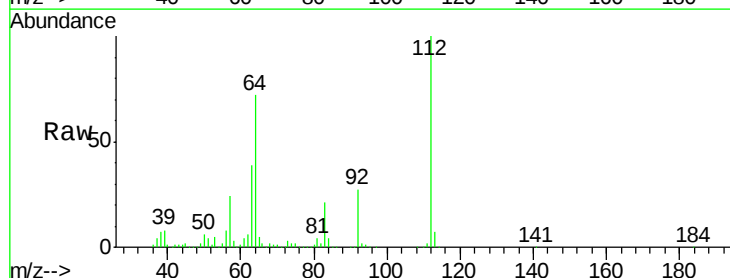


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

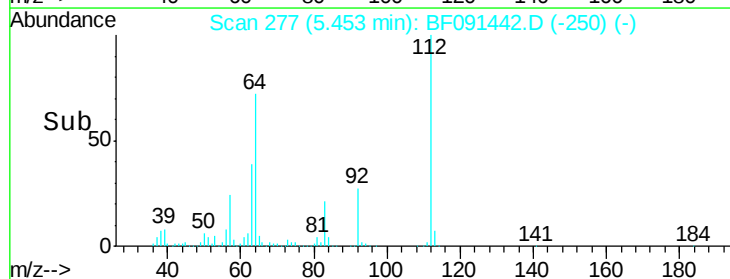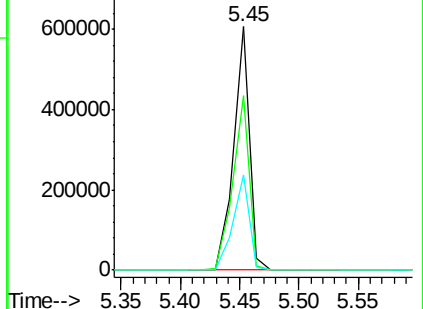

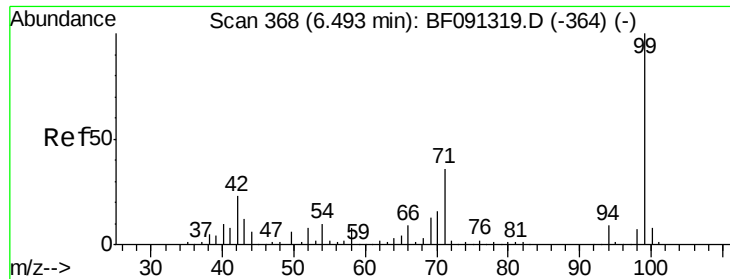

#7

Phenol-d6

Concen: 58.06 ng

RT: 6.48 min Scan# 367

Delta R.T. -0.00 min

Lab File: BF091442.D

Acq: 6 Dec 2016 2:26

Instrument :

BNA_F

ClientSampleId :

MW-05


Tot Ion: 99 Resp: 544787

Ion Ratio Lower Upper

99 100

42 21.3 20.6 31.0




71 36.0 29.9 44.9

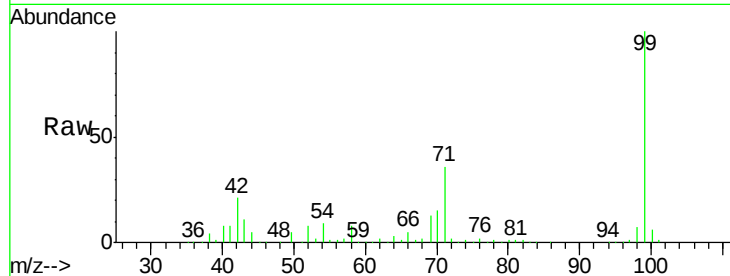

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

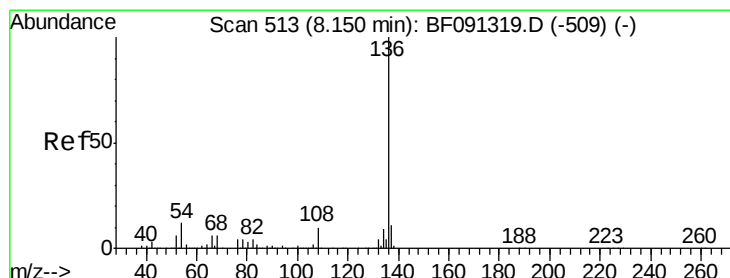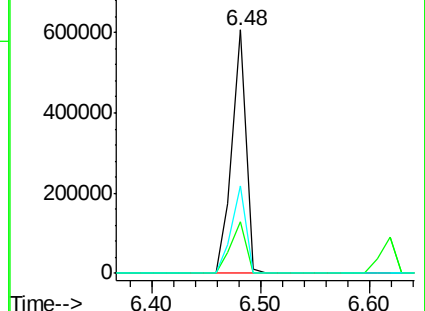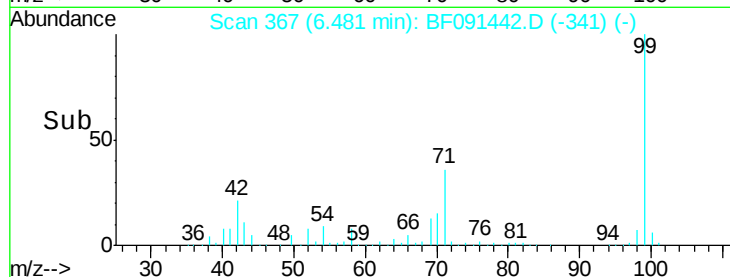

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 512

Delta R.T. -0.00 min

Lab File: BF091442.D

Acq: 6 Dec 2016 2:26

Tgt Ion: 136 Resp: 514766


Ion Ratio Lower Upper

136 100

137 10.9 9.1 13.7

54 7.3 9.1 13.7#

68 3.4 5.9 8.9#


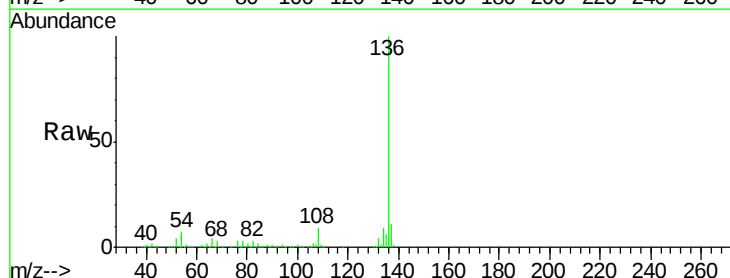



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

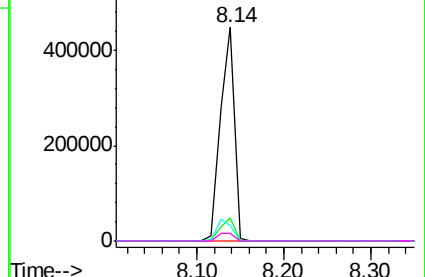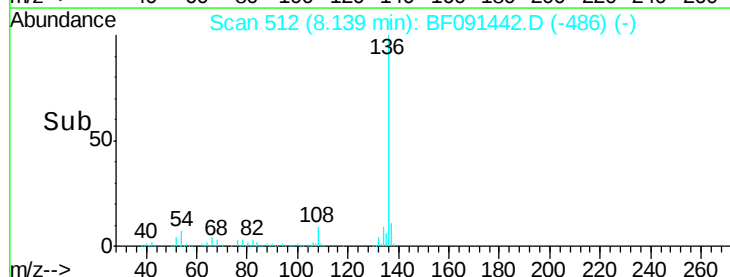


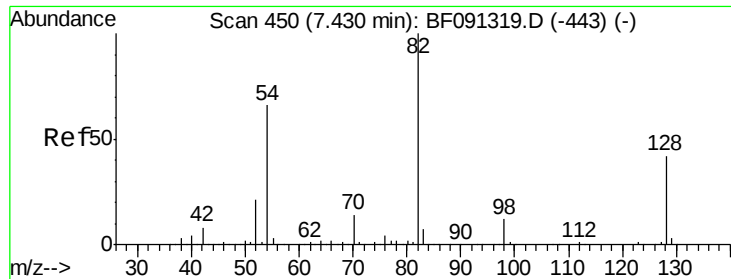




#23
 Nitrobenzene-d5
 Concen: 109.44 ng
 RT: 7.42 min Scan# 449
 Delta R.T. -0.00 min
 Lab File: BF091442.D
 Acq: 6 Dec 2016 2:26

Instrument :
 BNA_F
 ClientSampled :
 MW-05

Tot Ion: 82 Resp: 1005298
 Ion Ratio Lower Upper
 82 100
 128 45.2 31.8 47.6
 54 61.3 49.1 73.7

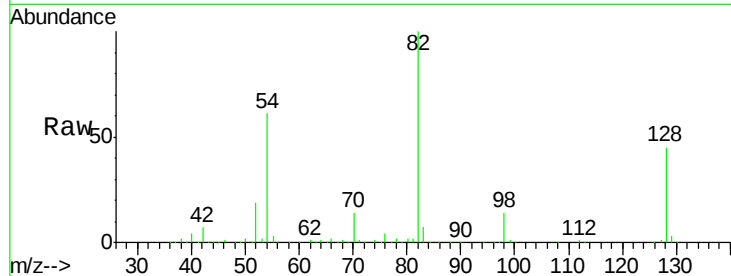


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

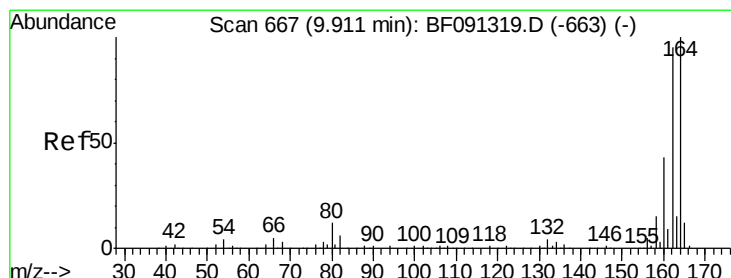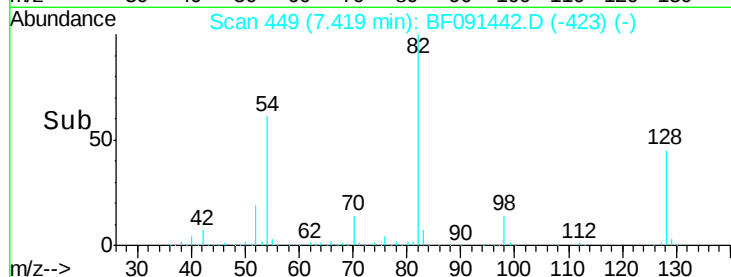
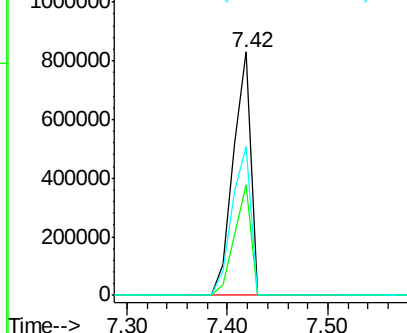



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 665
 Delta R.T. -0.00 min
 Lab File: BF091442.D
 Acq: 6 Dec 2016 2:26

Tgt Ion: 164 Resp: 282420
 Ion Ratio Lower Upper
 164 100
 162 95.8 82.6 124.0
 160 43.2 36.7 55.1

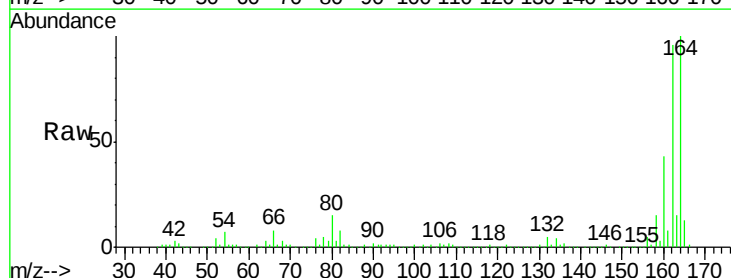

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

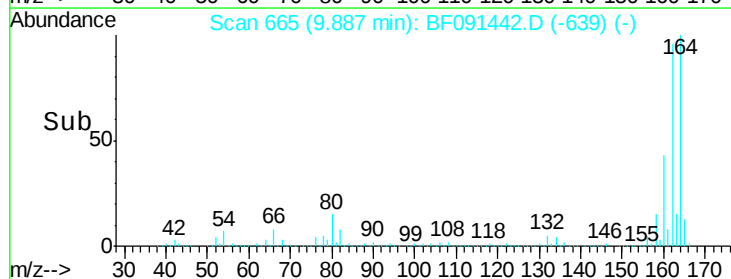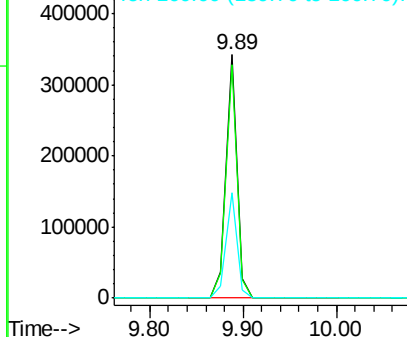


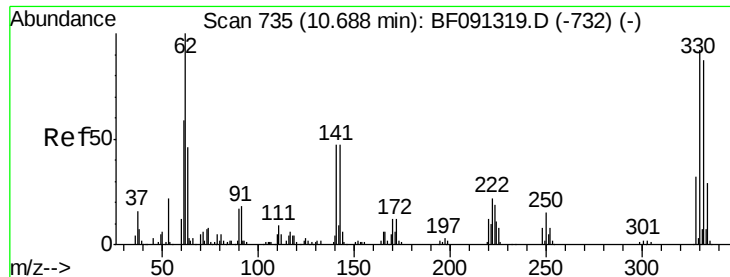




#41
 2,4,6-Tribromophenol
 Concen: 146.90 ng
 RT: 10.68 min Scan# 734
 Delta R.T. -0.00 min
 Lab File: BF091442.D
 Acq: 6 Dec 2016 2:26

Instrument :
 BNA_F
 ClientSampled :
 MW-05

Tot Ion:330 Resp: 392778
 Ion Ratio Lower Upper
 330 100
 332 96.1 76.2 114.4
 141 31.3 33.6 50.4#

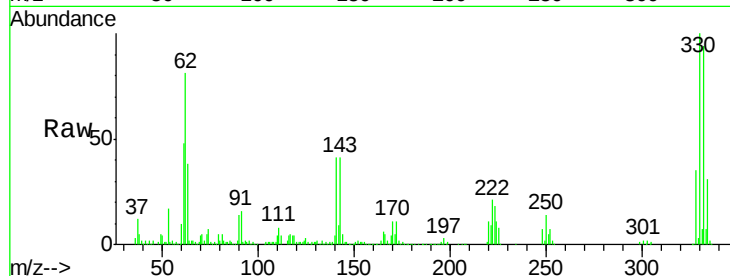


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

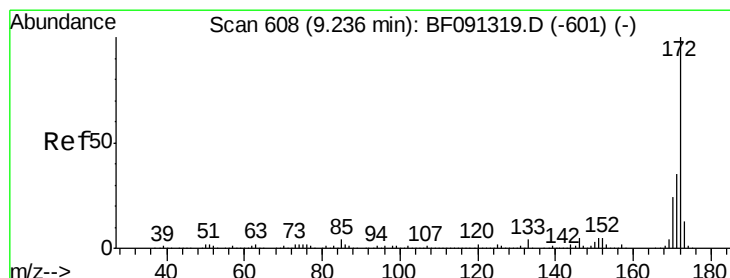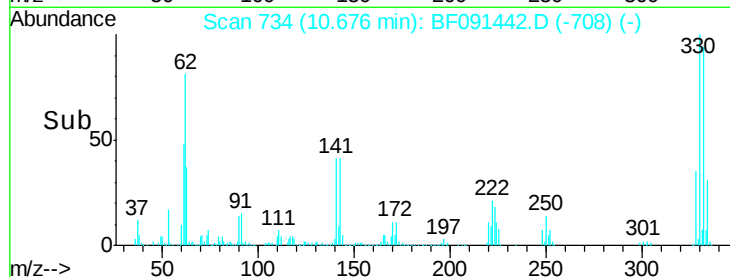
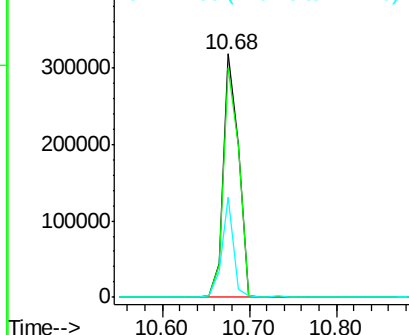



#44
 2-Fluorobiphenyl
 Concen: 94.88 ng
 RT: 9.21 min Scan# 606
 Delta R.T. -0.00 min
 Lab File: BF091442.D
 Acq: 6 Dec 2016 2:26

Tgt Ion:172 Resp: 1479935
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.4 44.0
 170 23.9 19.7 29.5

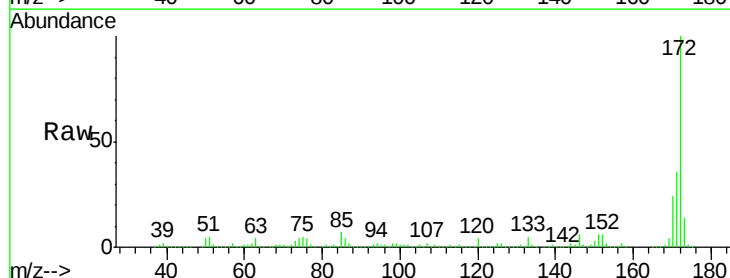

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

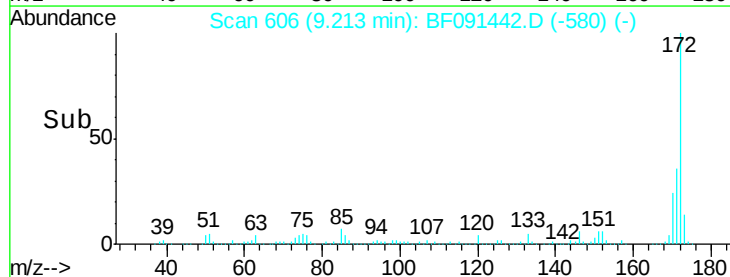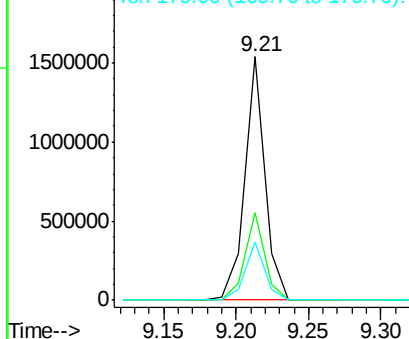

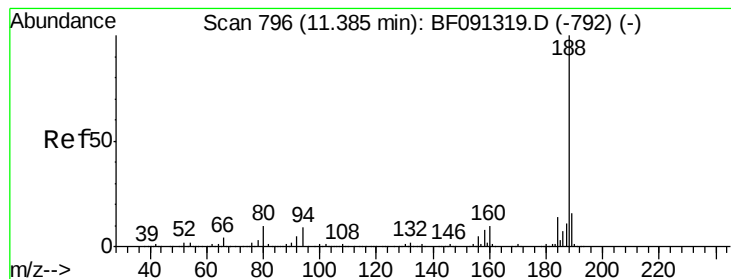

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.37 min Scan# 795

Delta R.T. -0.00 min

Lab File: BF091442.D

Acq: 6 Dec 2016 2:26

Instrument :

BNA_F

ClientSampleId :

MW-05


Tot Ion:188 Resp: 513183

Ion Ratio Lower Upper

188 100

94 6.2 9.2 13.8#




80 6.0 10.5 15.7#

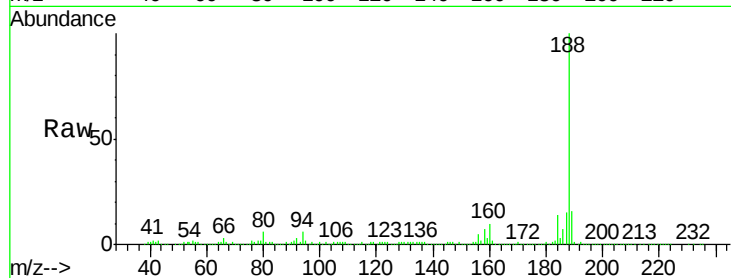

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

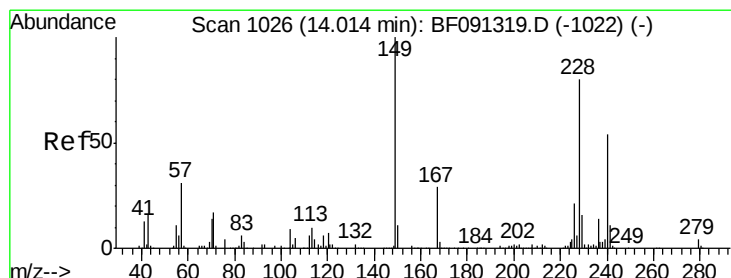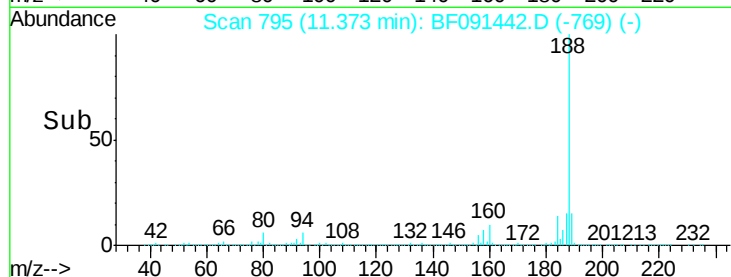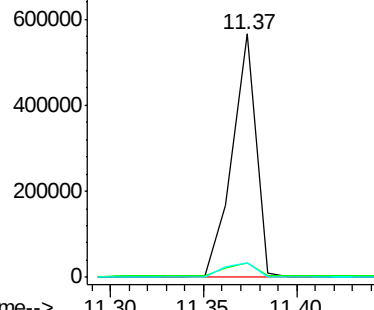

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.00 min Scan# 1025

Delta R.T. -0.00 min

Lab File: BF091442.D

Acq: 6 Dec 2016 2:26


Tgt Ion:240 Resp: 302375

Ion Ratio Lower Upper

240 100

120 6.9 12.1 18.1#



236 26.1 21.0 31.6

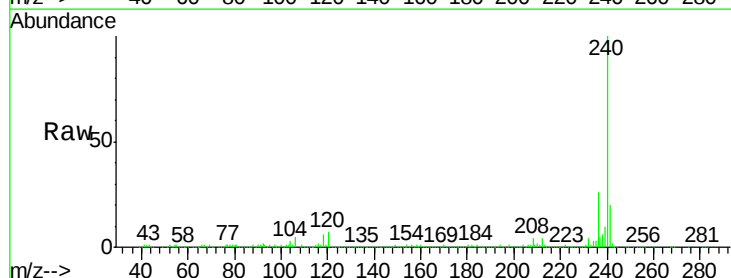


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

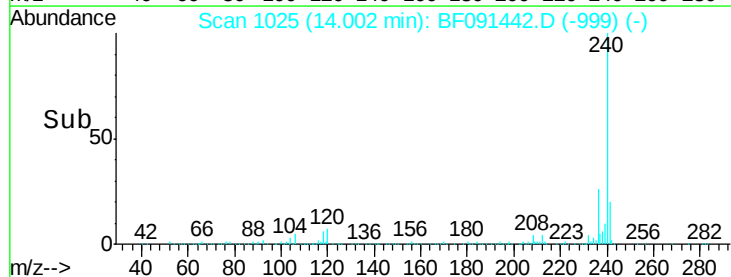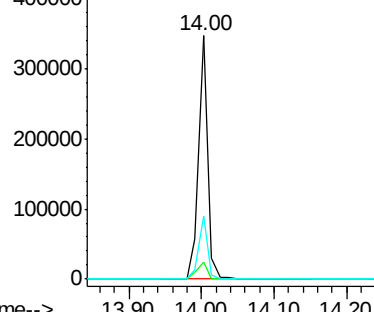




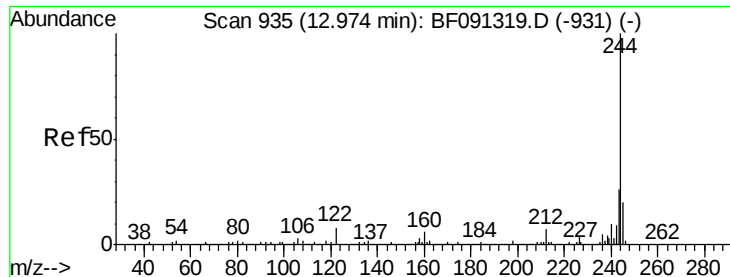


#78
 Terphenyl-d14
 Concen: 118.33 ng
 RT: 12.96 min Scan# 934
 Delta R.T. -0.00 min
 Lab File: BF091442.D
 Acq: 6 Dec 2016 2:26

Instrument :
 BNA_F
 ClientSampleId :
 MW-05

Tot Ion:244 Resp: 1646157

Ion	Ratio	Lower	Upper
244	100		
212	7.5	6.5	9.7
122	10.3	9.5	14.3

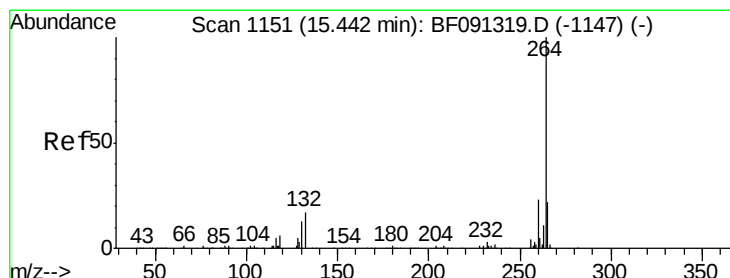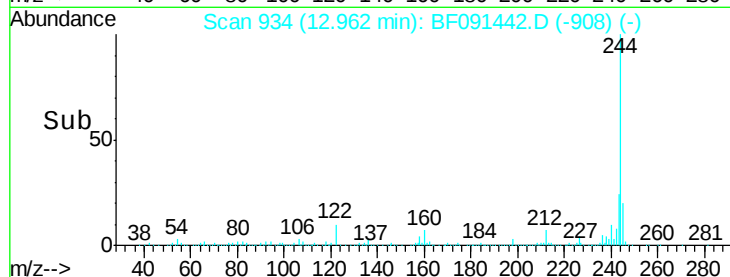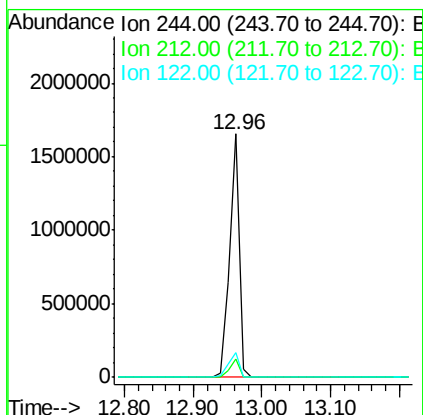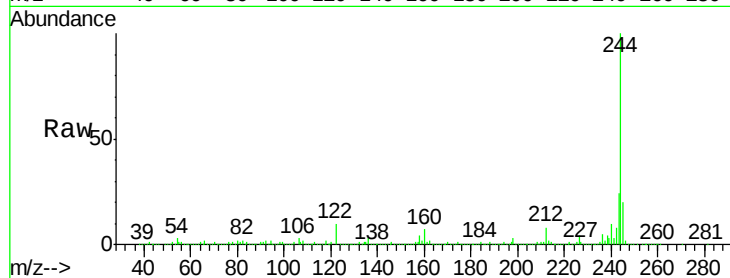

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.43 min Scan# 1150
 Delta R.T. -0.00 min
 Lab File: BF091442.D
 Acq: 6 Dec 2016 2:26

Tgt Ion:264 Resp: 299852

Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.8	28.2
265	22.3	17.0	25.6

