


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120516\
 Data File : BF091417.D
 Acq On : 5 Dec 2016 13:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

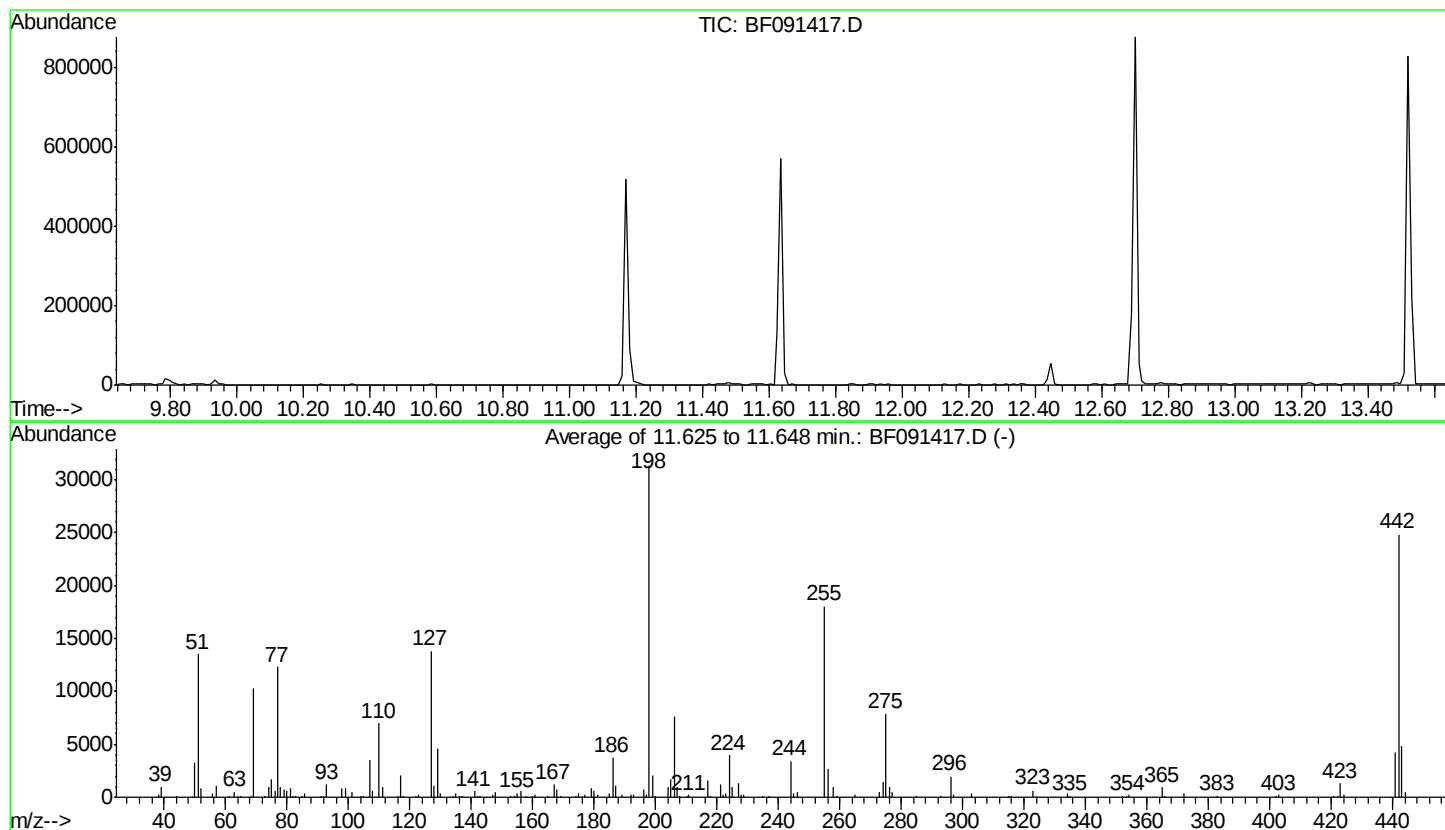

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	13554	PASS
68	69	0.00	2	1.6	165	PASS
69	198	0.00	100	33.0	10338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.1	13841	PASS
197	198	0.00	2	0.7	209	PASS
198	198	100	100	100.0	31351	PASS
199	198	5	9	6.7	2110	PASS
275	198	10	60	25.3	7925	PASS
365	198	1	100	3.0	927	PASS
441	442	0.01	24	16.9	4186	PASS
442	198	50	100	79.1	24814	PASS
443	442	15	24	19.5	4828	PASS