


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120516\
 Data File : BF091443.D
 Acq On : 6 Dec 2016 4:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

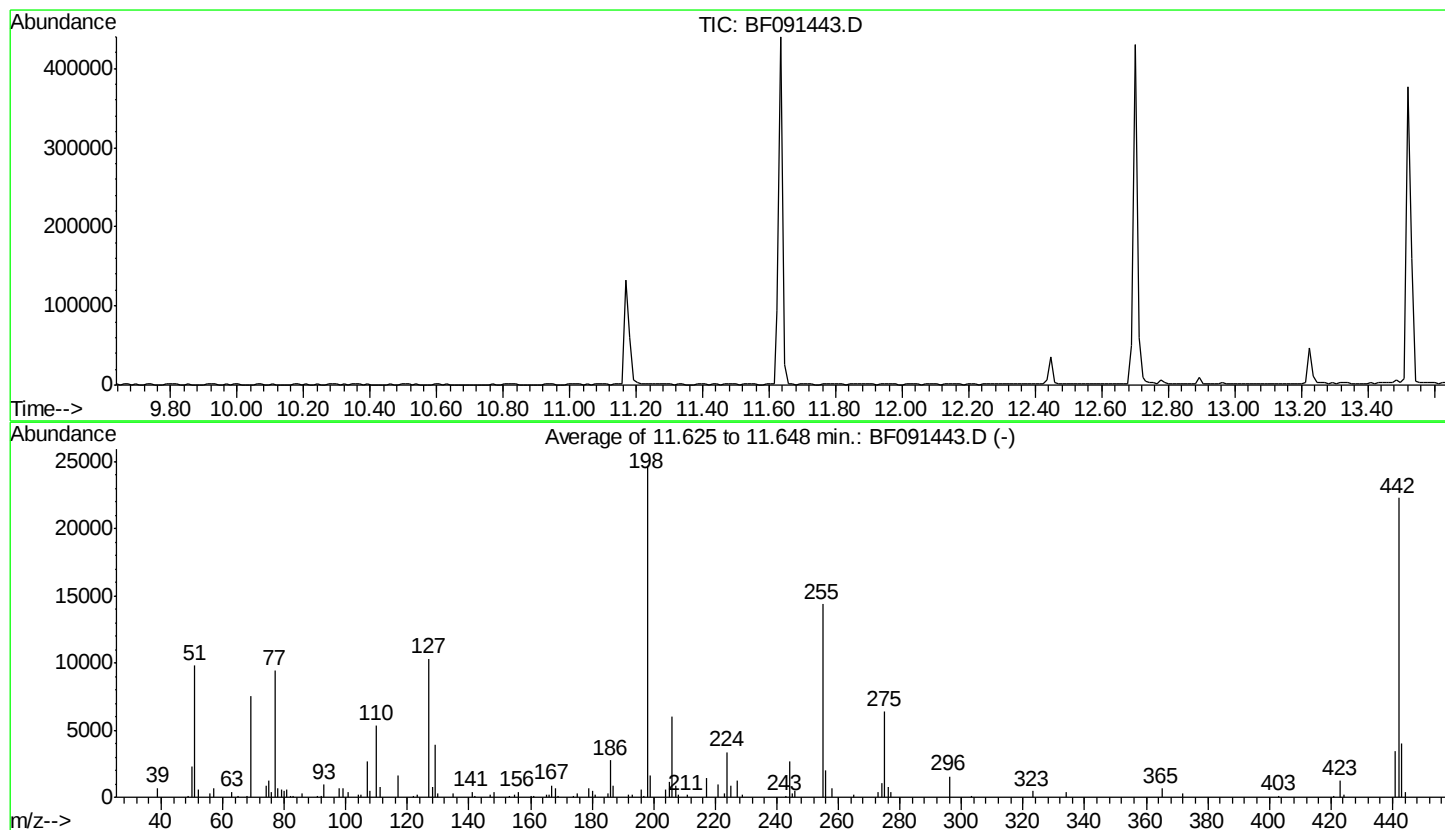

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	9800	PASS
68	69	0.00	2	1.5	111	PASS
69	198	0.00	100	30.3	7486	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	10304	PASS
197	198	0.00	2	0.5	130	PASS
198	198	100	100	100.0	24689	PASS
199	198	5	9	6.4	1580	PASS
275	198	10	60	25.8	6381	PASS
365	198	1	100	2.6	630	PASS
441	442	0.01	24	15.3	3415	PASS
442	198	50	100	90.3	22288	PASS
443	442	15	24	17.9	3985	PASS