
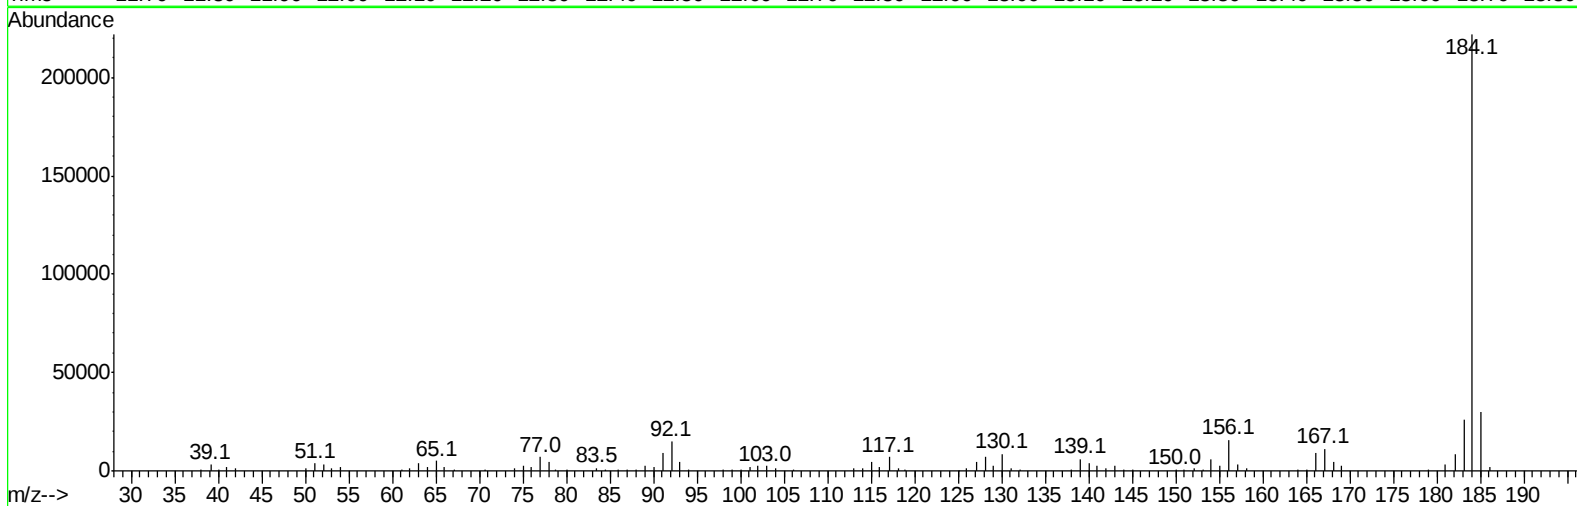


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120517\
Data File : BF101112.D
Acq On : 5 Dec 2017 9:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 07:28:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

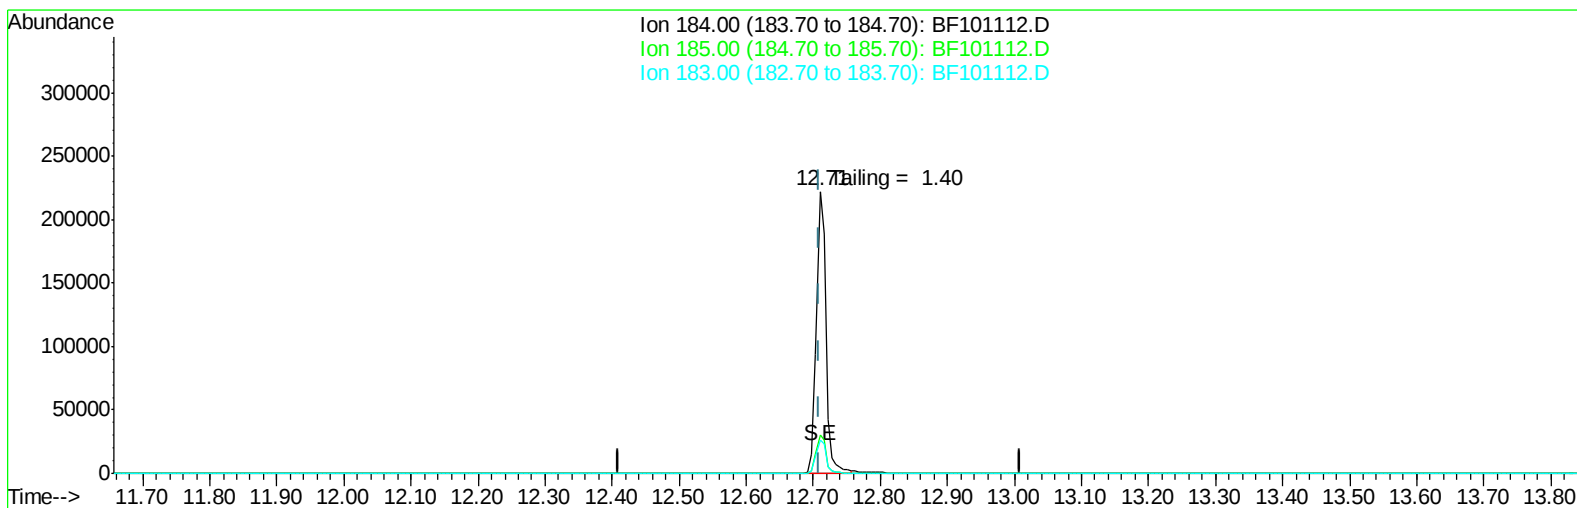

TIC: BF101112.D

(76) Benzidine



12.710min (+0.000) 0.00ng

response 213429

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.64
183.00	11.60	11.77
0.00	0.00	0.00

```
Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120517\  
Data File : BF101112.D  
Acq On    : 5 Dec 2017    9:14  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 06 07:28:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

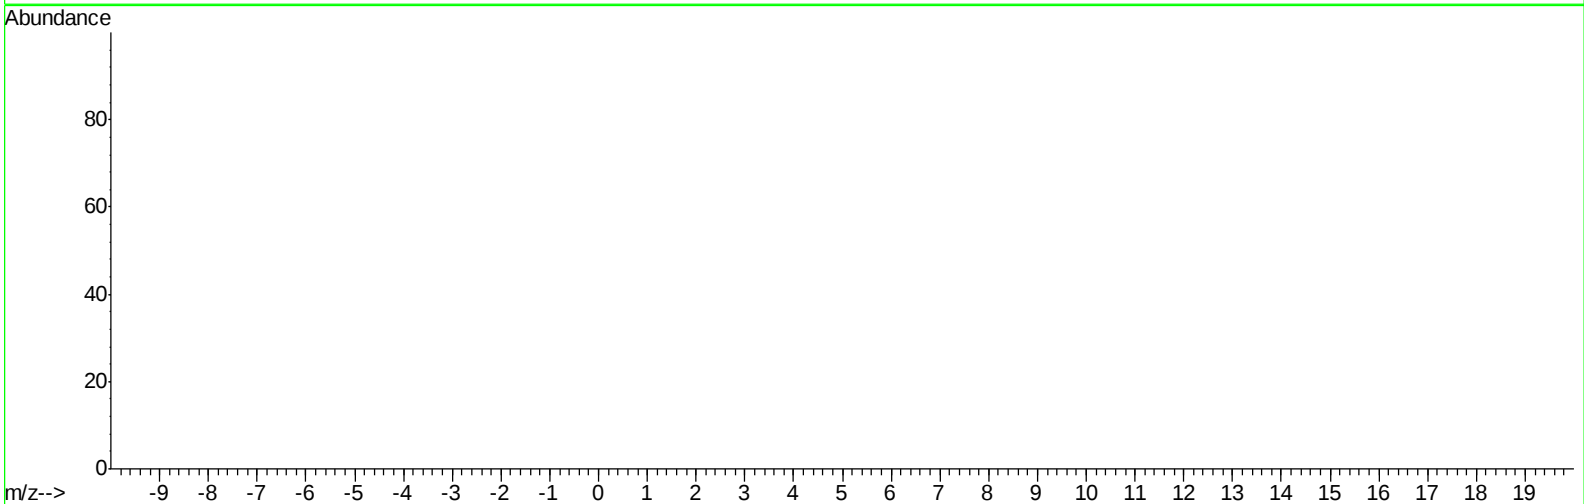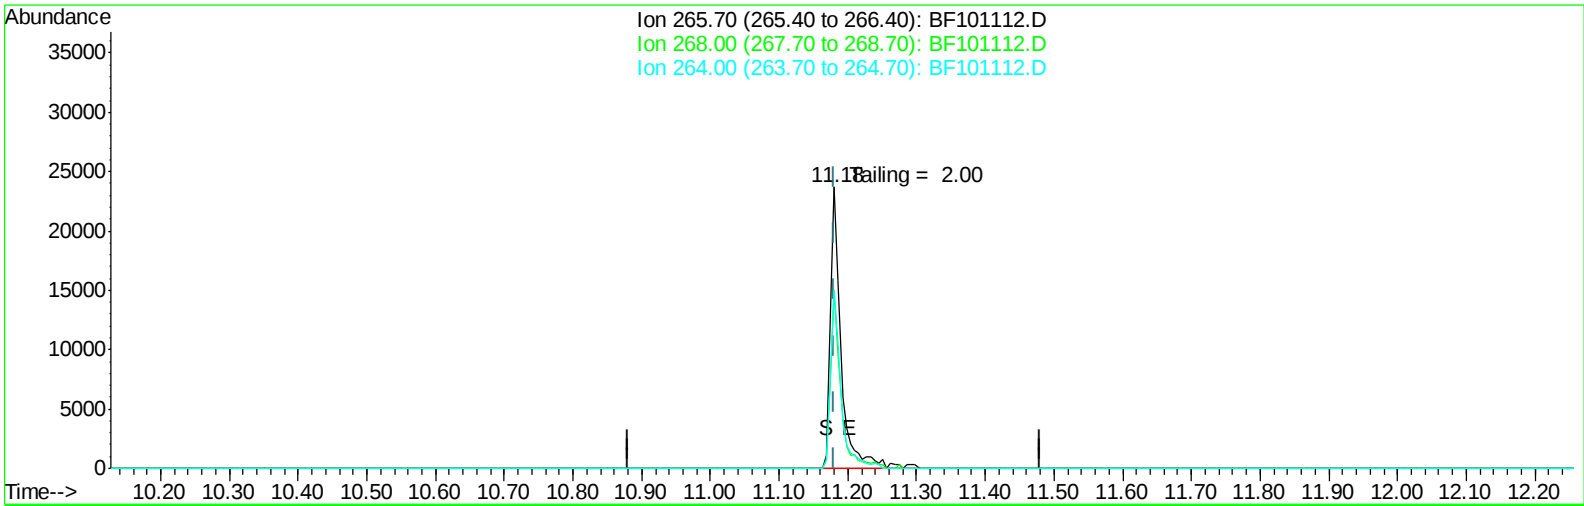

TIC: BF101112.D