
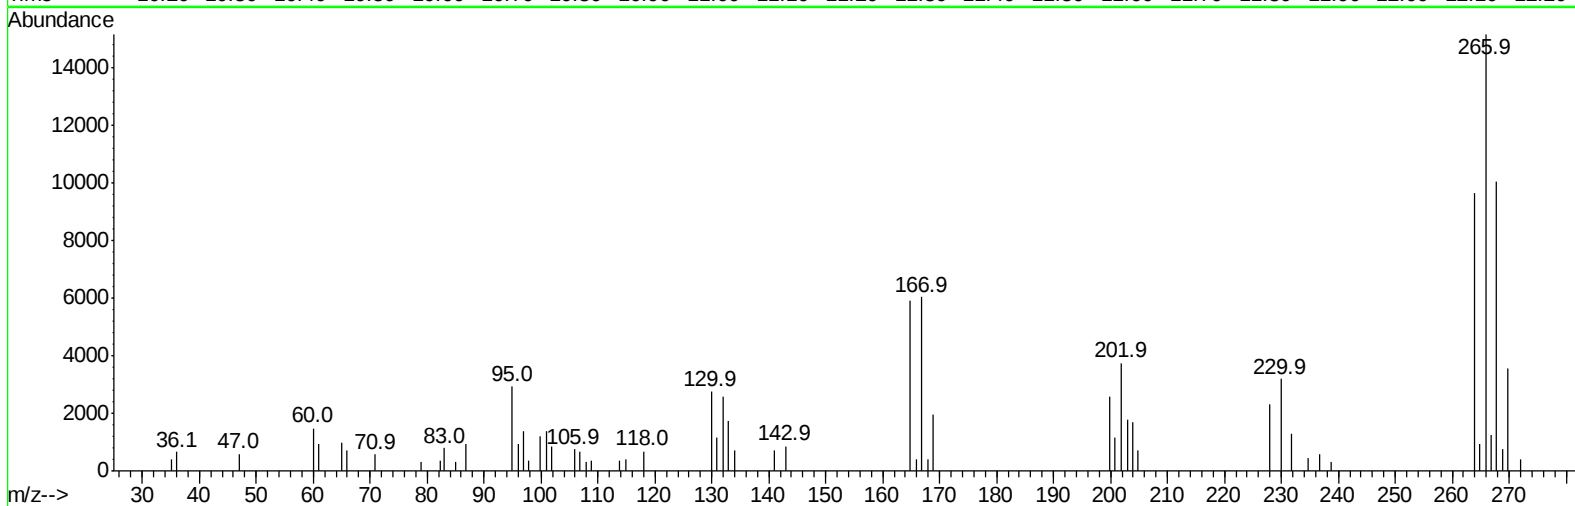


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120517\
Data File : BF101138.D
Acq On : 5 Dec 2017 22:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 07:31:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

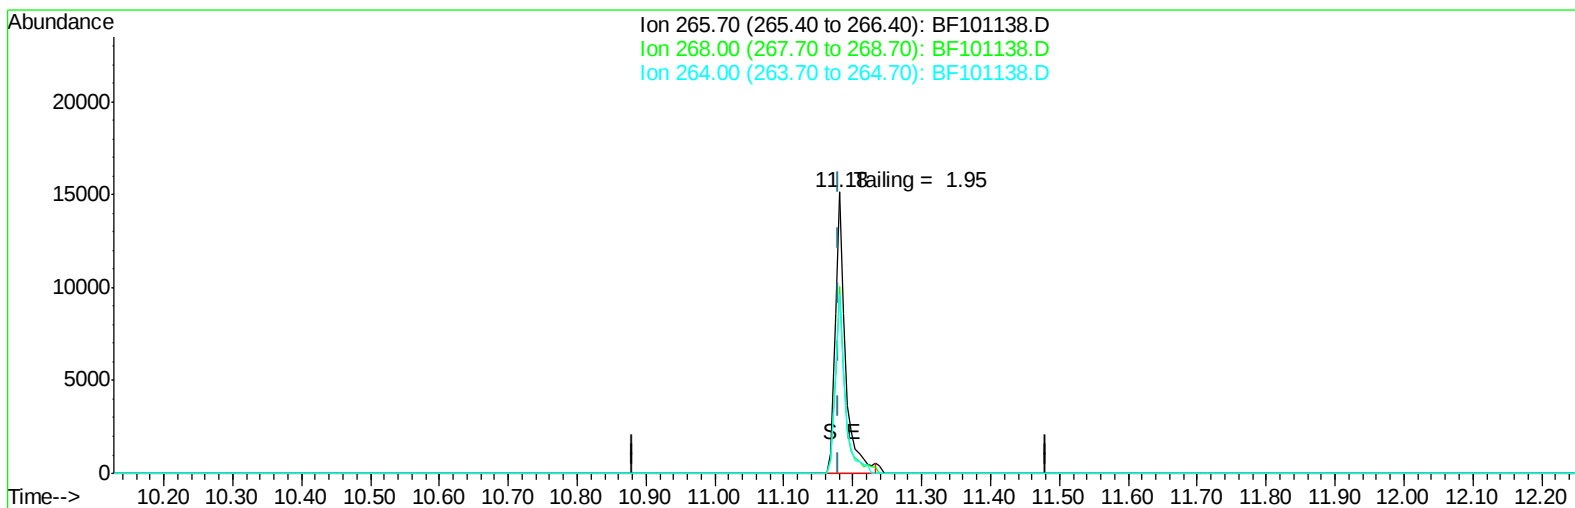

TIC: BF101138.D

(69) Pentachlorophenol (C)



11.180min (+0.000) 0.00ng

response 15682

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.26
264.00	61.90	63.54
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120517\
Data File : BF101138.D
Acq On : 5 Dec 2017 22:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 07:31:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

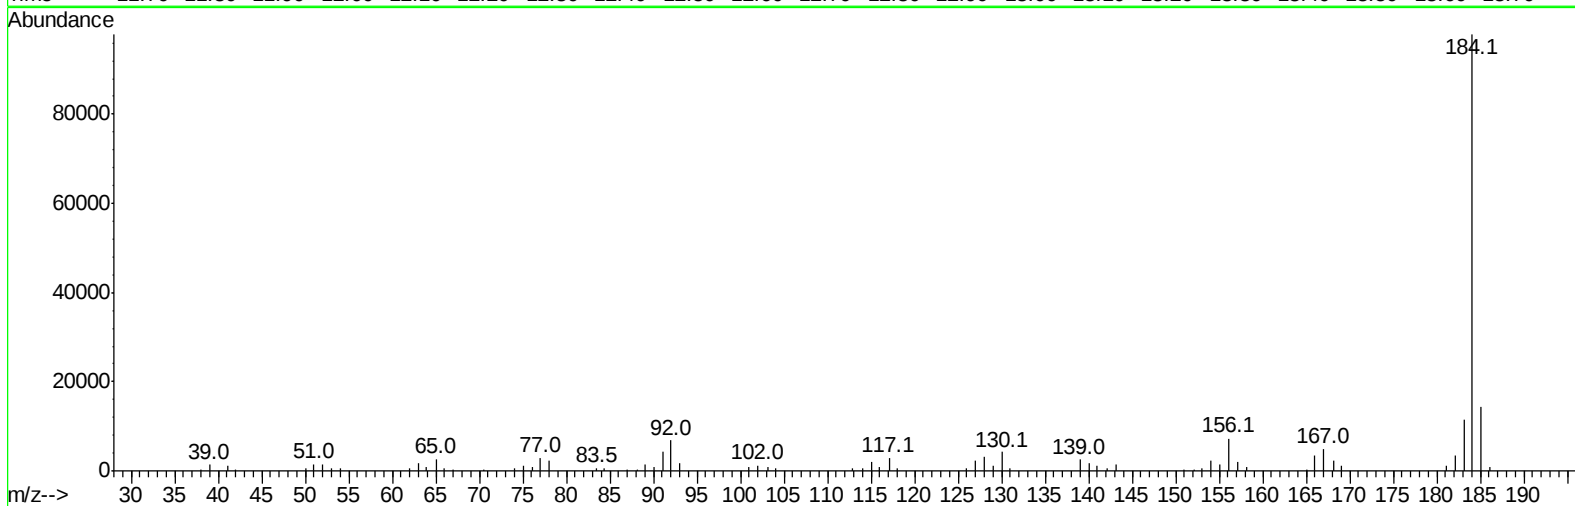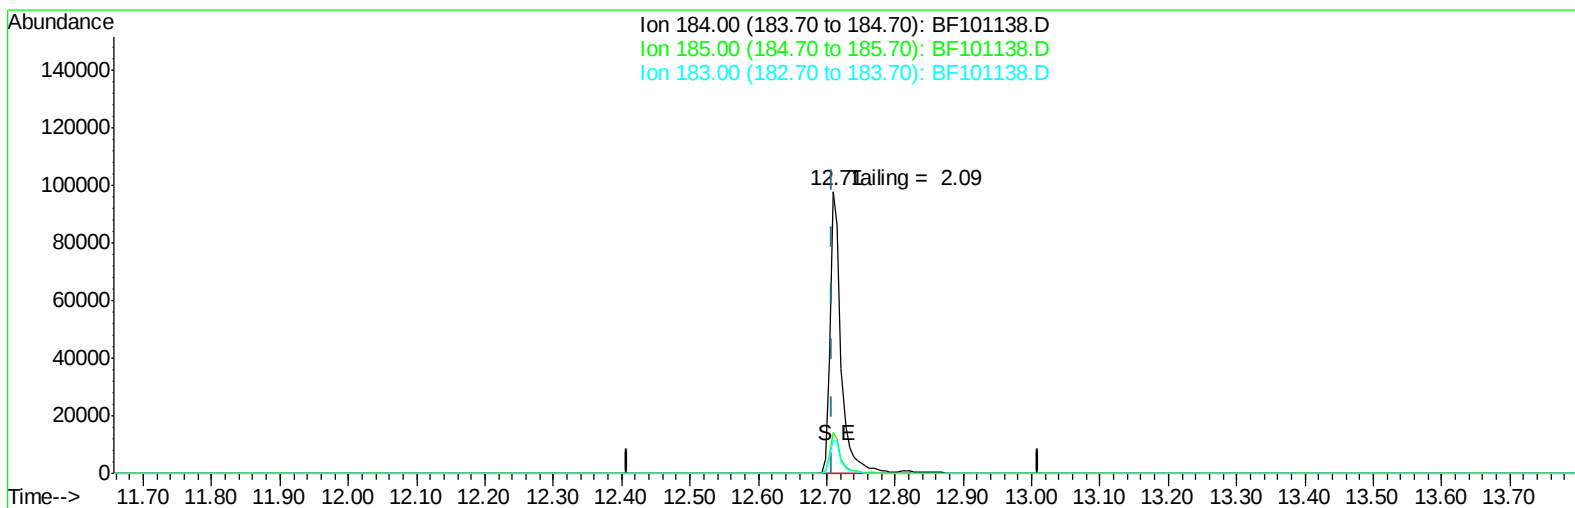

TIC: BF101138.D

(76) Benzidine

12.710min (+0.000) 0.00ng

response 110861

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.62
183.00	11.60	11.84
0.00	0.00	0.00