

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120517\
 Data File : BF101156.D
 Acq On : 6 Dec 2017 8:57
 Operator : SJ/JU
 Sample : I6696-01DL 20X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-TP102-ADL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	571	573	583	rBV	37930	43481	5.14%	0.470%
2	6.475	743	746	753	rBV	42258	45320	5.35%	0.489%
3	6.616	767	770	774	rBV	59663	52977	6.26%	0.572%
4	6.845	805	809	816	rBB	317643	266705	31.50%	2.881%
5	6.998	832	835	841	rBB	48676	43403	5.13%	0.469%
6	7.157	858	862	866	rBB	14820	13163	1.55%	0.142%
7	7.410	902	905	911	rBV	30346	31897	3.77%	0.345%
8	8.128	1018	1027	1030	rBV	434738	363901	42.98%	3.930%
9	8.939	1161	1165	1172	rBV	192729	160209	18.92%	1.730%
10	9.198	1206	1209	1212	rBV	84836	64058	7.57%	0.692%
11	9.304	1223	1227	1233	rVB	99488	79529	9.39%	0.859%
12	9.398	1239	1243	1250	rVV	154471	136673	16.14%	1.476%
13	9.469	1250	1255	1258	rVV	77475	103715	12.25%	1.120%
14	9.504	1258	1261	1263	rVV	15820	13838	1.63%	0.149%
15	9.539	1263	1267	1270	rVV	163083	160025	18.90%	1.728%
16	9.569	1270	1272	1275	rVV	59737	47576	5.62%	0.514%
17	9.610	1275	1279	1282	rVB2	12986	14811	1.75%	0.160%
18	9.657	1282	1287	1295	rBB	73980	77743	9.18%	0.840%
19	9.745	1299	1302	1307	rVB	87962	74603	8.81%	0.806%
20	9.863	1319	1322	1323	rBV	62412	48482	5.73%	0.524%
21	9.886	1323	1326	1328	rVV	420143	375428	44.34%	4.055%
22	9.916	1328	1331	1335	rVV	452255	374705	44.26%	4.047%
23	9.981	1339	1342	1347	rVV	30857	34666	4.09%	0.374%
24	10.081	1356	1359	1363	rVB3	42277	42810	5.06%	0.462%
25	10.122	1363	1366	1370	rVB	34566	32472	3.84%	0.351%
26	10.192	1374	1378	1381	rBV2	56471	56750	6.70%	0.613%
27	10.228	1381	1384	1386	rVV2	23844	21912	2.59%	0.237%
28	10.286	1390	1394	1396	rBV2	24116	31622	3.74%	0.342%
29	10.339	1400	1403	1405	rBV	66898	54833	6.48%	0.592%
30	10.404	1412	1414	1416	rBV	43214	30229	3.57%	0.326%
31	10.433	1416	1419	1424	rVB2	246564	225255	26.61%	2.433%
32	10.481	1424	1427	1428	rBV2	23210	18743	2.21%	0.202%
33	10.516	1431	1433	1435	rVB3	18305	14102	1.67%	0.152%
34	10.539	1435	1437	1440	rBV	50774	46581	5.50%	0.503%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120517\
 Data File : BF101156.D
 Acq On : 6 Dec 2017 8:57
 Operator : SJ/JU
 Sample : I6696-01DL 20X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-TP102-ADL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.616	1447	1450	1453	rVB	28023	25337	2.99%	0.274%
36	10.657	1453	1457	1459	rBV	83531	76723	9.06%	0.829%
37	10.792	1475	1480	1483	rBV4	23228	25140	2.97%	0.272%
38	10.980	1508	1512	1514	rBV	68849	81830	9.67%	0.884%
39	11.010	1514	1517	1520	rVV	41156	35819	4.23%	0.387%
40	11.063	1523	1526	1529	rVB	44698	34751	4.10%	0.375%
41	11.128	1533	1537	1540	rVV3	12458	16188	1.91%	0.175%
42	11.180	1544	1546	1549	rVB2	31607	22584	2.67%	0.244%
43	11.269	1556	1561	1569	rVB3	35972	52257	6.17%	0.564%
44	11.375	1575	1579	1581	rBV	433931	391384	46.23%	4.227%
45	11.398	1581	1583	1587	rVV	950339	846609	100.00%	9.144%
46	11.451	1589	1592	1595	rVV	255407	219476	25.92%	2.370%
47	11.480	1595	1597	1600	rVV2	19702	21962	2.59%	0.237%
48	11.663	1625	1628	1632	rVV	28149	24519	2.90%	0.265%
49	11.704	1632	1635	1641	rVB2	21673	27175	3.21%	0.294%
50	11.833	1652	1657	1661	rBV3	7774	12855	1.52%	0.139%
51	11.875	1661	1664	1666	rVV	211286	167266	19.76%	1.807%
52	11.904	1666	1669	1674	rVV	214221	178371	21.07%	1.926%
53	11.951	1674	1677	1680	rVV	91368	81855	9.67%	0.884%
54	11.986	1680	1683	1686	rVV2	250806	293715	34.69%	3.172%
55	12.010	1686	1687	1692	rVB	122280	70135	8.28%	0.757%
56	12.169	1711	1714	1718	rVB	95177	79078	9.34%	0.854%
57	12.316	1733	1739	1742	rBV	31319	33427	3.95%	0.361%
58	12.351	1742	1745	1747	rVV	32283	26993	3.19%	0.292%
59	12.375	1747	1749	1752	rVB	16786	13450	1.59%	0.145%
60	12.422	1752	1757	1760	rBV	118694	121688	14.37%	1.314%
61	12.463	1760	1764	1766	rVV2	57729	79487	9.39%	0.858%
62	12.480	1766	1767	1769	rVV	46828	29713	3.51%	0.321%
63	12.510	1769	1772	1777	rVV2	24380	43353	5.12%	0.468%
64	12.586	1781	1785	1789	rBV	356686	321070	37.92%	3.468%
65	12.686	1799	1802	1805	rBV	115503	105311	12.44%	1.137%
66	12.757	1808	1814	1819	rBV3	20920	24619	2.91%	0.266%
67	12.822	1819	1825	1831	rBV	462041	443855	52.43%	4.794%
68	12.869	1831	1833	1837	rBV2	18071	17780	2.10%	0.192%
69	12.951	1845	1847	1850	rVV	57067	42619	5.03%	0.460%
70	13.033	1857	1861	1867	rVB3	39403	57106	6.75%	0.617%
71	13.122	1872	1876	1877	rVV2	39429	40454	4.78%	0.437%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120517\
 Data File : BF101156.D
 Acq On : 6 Dec 2017 8:57
 Operator : SJ/JU
 Sample : I6696-01DL 20X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-TP102-ADL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.145	1877	1880	1883	rVB	82043	79724	9.42%	0.861%
73	13.210	1888	1891	1895	rVV	77076	70357	8.31%	0.760%
74	13.251	1895	1898	1901	rVV2	60195	51318	6.06%	0.554%
75	13.316	1905	1909	1912	rVV	46481	59066	6.98%	0.638%
76	13.345	1912	1914	1916	rVV	50001	45536	5.38%	0.492%
77	13.374	1916	1919	1926	rVB	58992	68537	8.10%	0.740%
78	13.627	1958	1962	1965	rBV3	14195	20701	2.45%	0.224%
79	13.745	1980	1982	1984	rBV2	13109	13646	1.61%	0.147%
80	13.792	1988	1990	1992	rVV	32344	26290	3.11%	0.284%
81	13.816	1992	1994	1997	rVB	16309	14503	1.71%	0.157%
82	14.016	2023	2028	2031	rBV2	374935	455091	53.75%	4.915%
83	14.045	2031	2033	2037	rVB	108774	92987	10.98%	1.004%
84	14.404	2089	2094	2098	rVV	40831	50313	5.94%	0.543%
85	14.439	2098	2100	2103	rVB	16783	13263	1.57%	0.143%
86	14.480	2103	2107	2109	rBV3	12781	18031	2.13%	0.195%
87	14.527	2113	2115	2117	rBV2	15458	12833	1.52%	0.139%
88	14.551	2117	2119	2121	rVB	20570	16035	1.89%	0.173%
89	15.063	2201	2206	2217	rBV	56074	117515	13.88%	1.269%
90	15.168	2220	2224	2235	rVB	23291	31392	3.71%	0.339%
91	15.368	2254	2258	2264	rBV	45350	57309	6.77%	0.619%
92	15.427	2264	2268	2273	rBV	85554	105916	12.51%	1.144%
93	15.492	2273	2279	2283	rVV	216027	259875	30.70%	2.807%
94	15.521	2283	2284	2291	rVB2	14283	18158	2.14%	0.196%
95	16.057	2371	2375	2380	rVB3	10720	15637	1.85%	0.169%
96	16.510	2445	2452	2453	rBV3	9916	15165	1.79%	0.164%
97	16.557	2453	2460	2470	rVB6	14844	56420	6.66%	0.609%
98	16.980	2525	2532	2541	rVB2	18293	38840	4.59%	0.419%
99	17.427	2602	2608	2615	rBV2	14827	31959	3.77%	0.345%
100	17.674	2643	2650	2656	rBV3	6244	14249	1.68%	0.154%


Sum of corrected areas: 9258837

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120517\
Data File : BF101156.D
Acq On : 6 Dec 2017 8:57
Operator : SJ/JU
Sample : I6696-01DL 20X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-TP102-ADL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

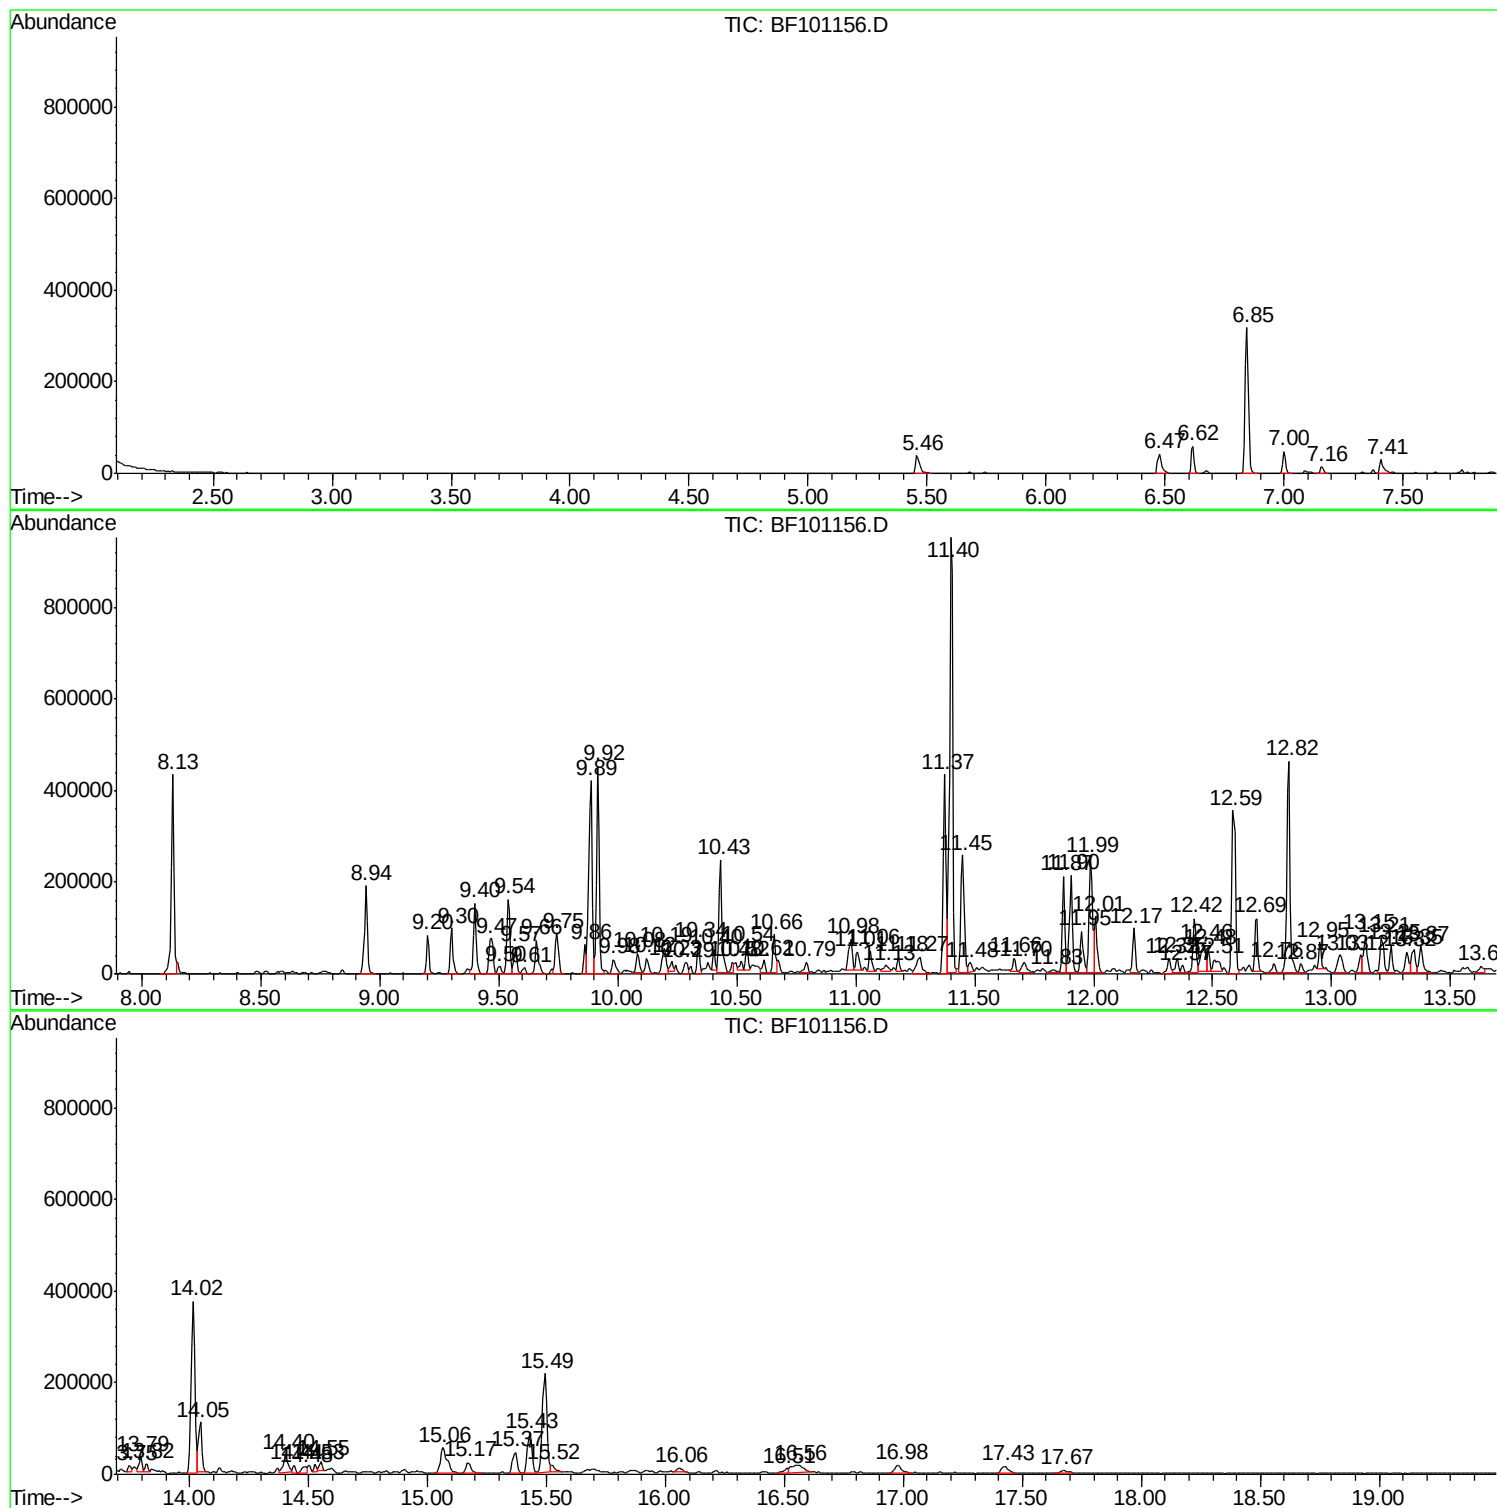

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120517\
Data_File : BF101156.D
Acq_On : 6-Dec-2017 8:577
Operator : SJ/JUU
Sample : I6696-01DL_20XX
Misc :
ALS_Vial : 43 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
CS-TP102-ADL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
