


Data Path : Z:\HPCHEM1\BNA F\DATA\BF120517\
 Data File : BF101138.D
 Acq On : 5 Dec 2017 22:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 04 13:07:49 2017

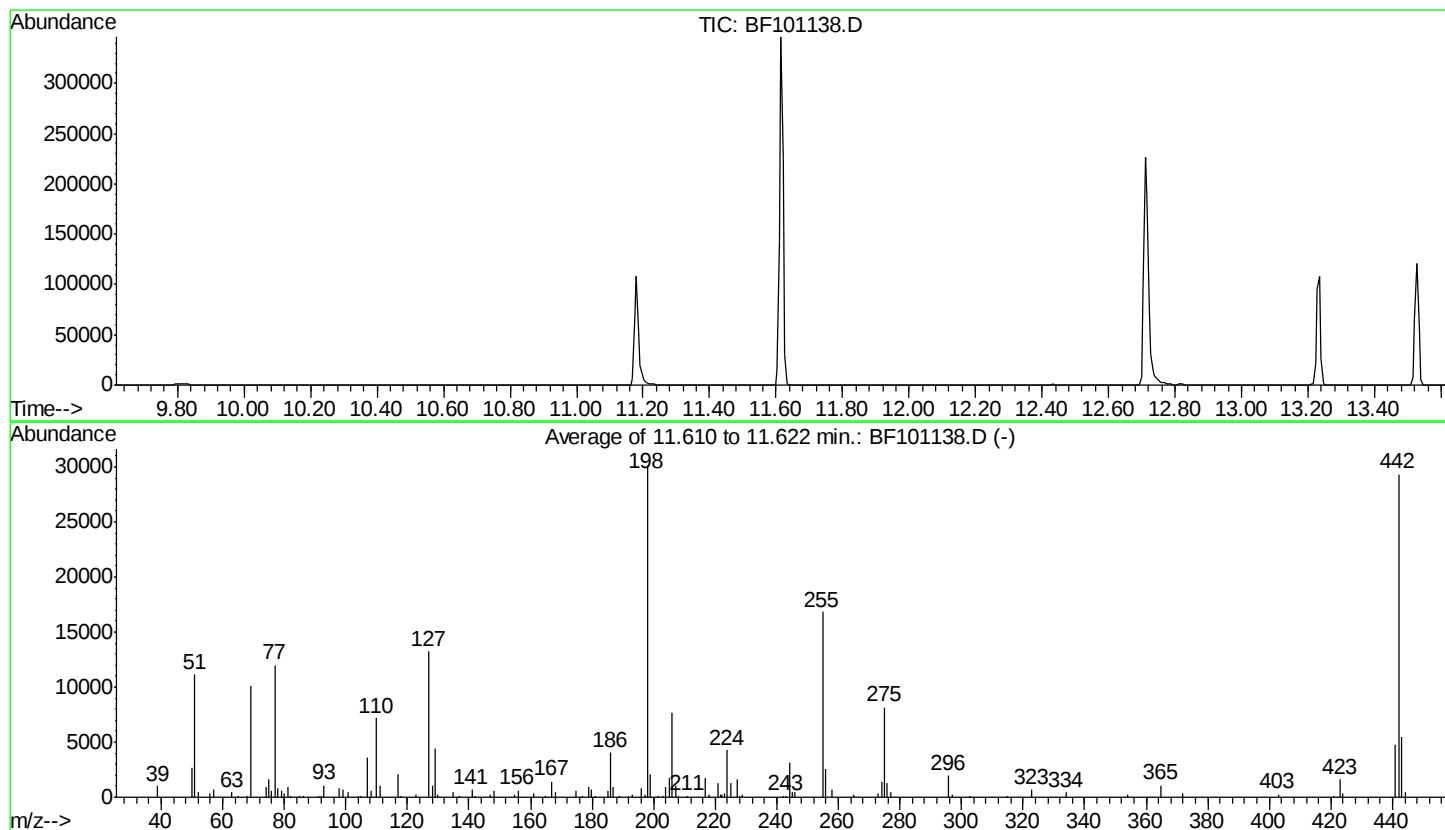

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	11134	PASS
68	69	0.00	2	1.1	109	PASS
69	198	0.00	100	33.6	10121	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	13205	PASS
197	198	0.00	2	0.7	208	PASS
198	198	100	100	100.0	30109	PASS
199	198	5	9	7.0	2121	PASS
275	198	10	60	27.2	8194	PASS
365	198	1	100	3.6	1070	PASS
441	443	0.01	100	86.1	4737	PASS
442	198	50	100	97.5	29343	PASS
443	442	15	24	18.8	5502	PASS