
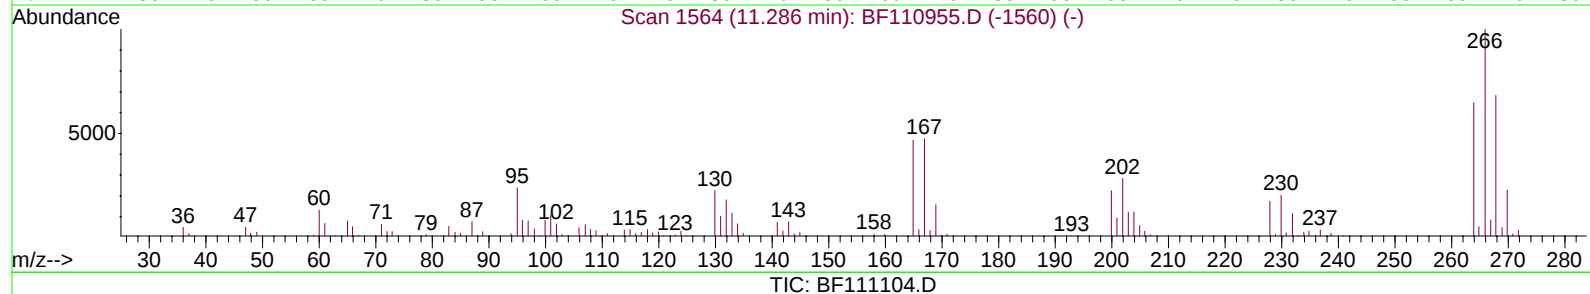
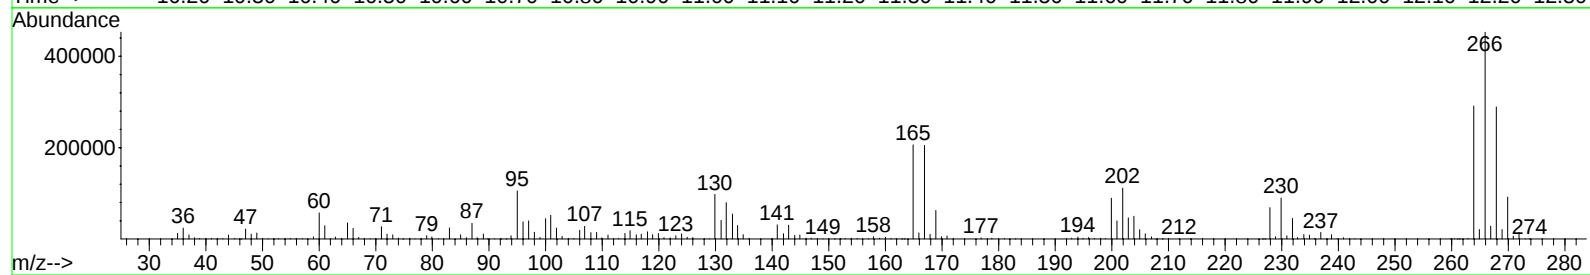


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120518\
Data File : BF111104.D
Acq On : 5 Dec 2018 13:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 13:40:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 29 10:35:31 2018
Response via : Initial Calibration

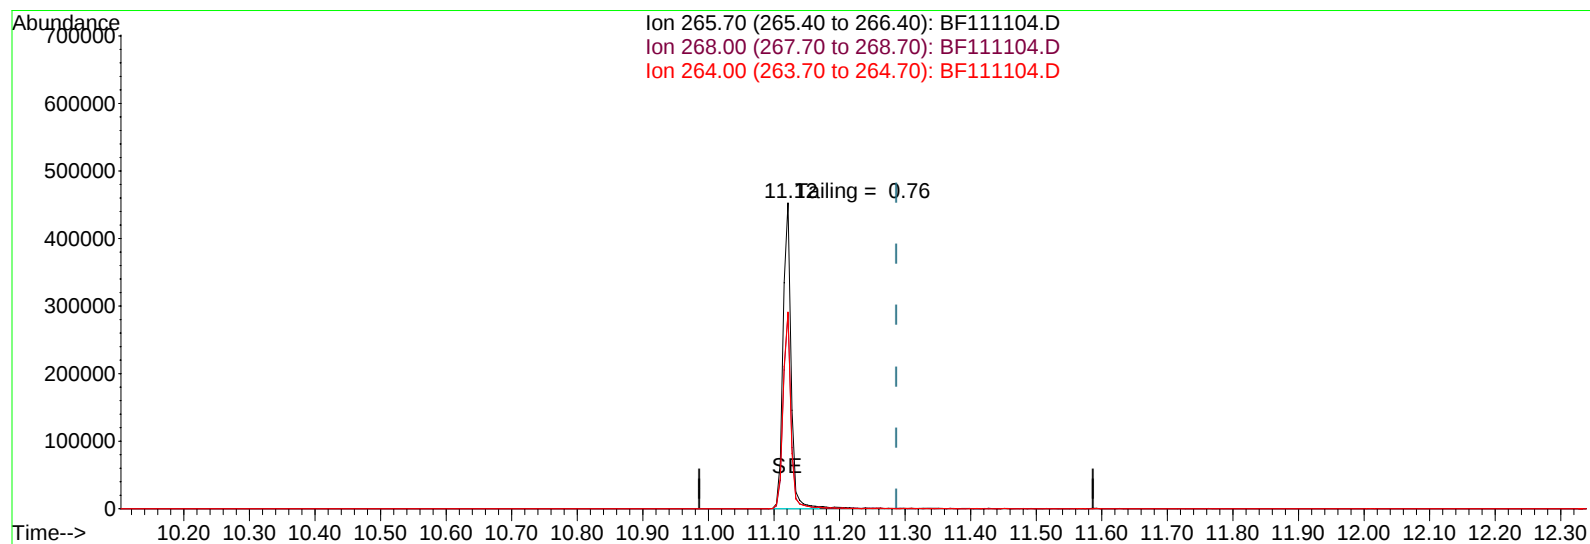

(70) Pentachlorophenol (C)




11.122min (-0.165) 50137.50ng

response 369535

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.86
264.00	63.20	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120518\
 Data File : BF111104.D
 Acq On : 5 Dec 2018 13:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 13:40:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 29 10:35:31 2018
 Response via : Initial Calibration

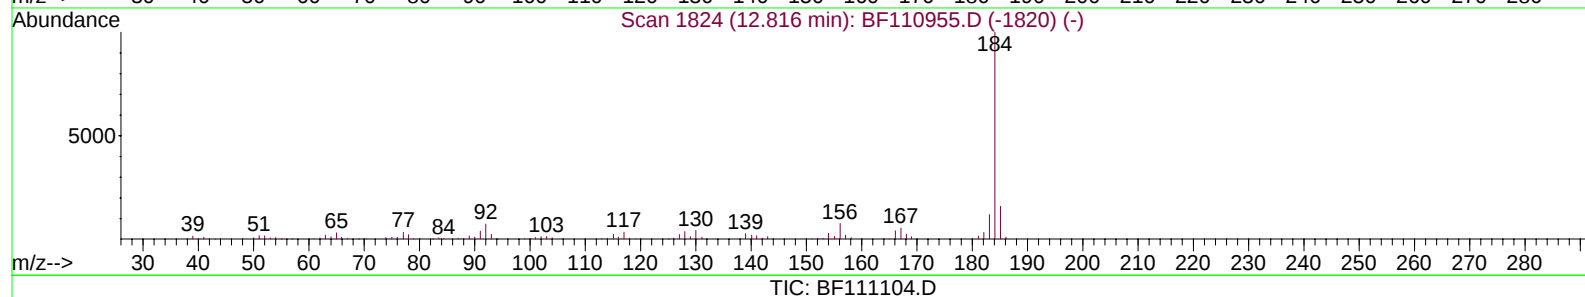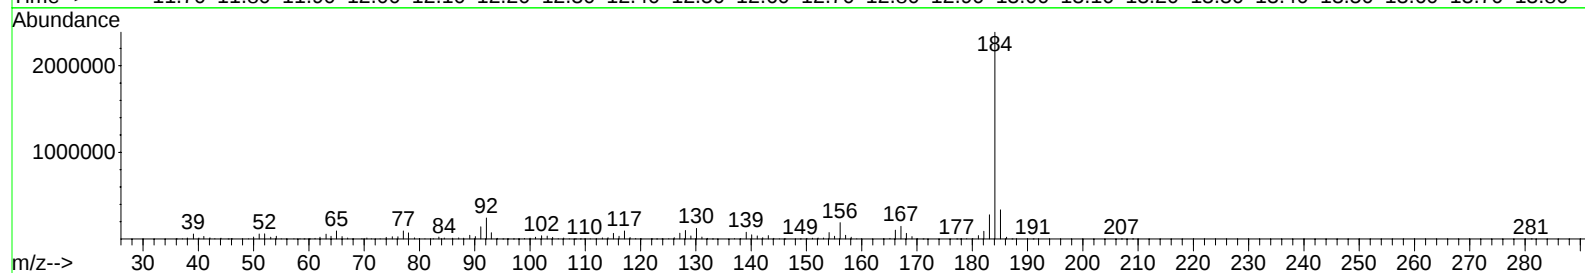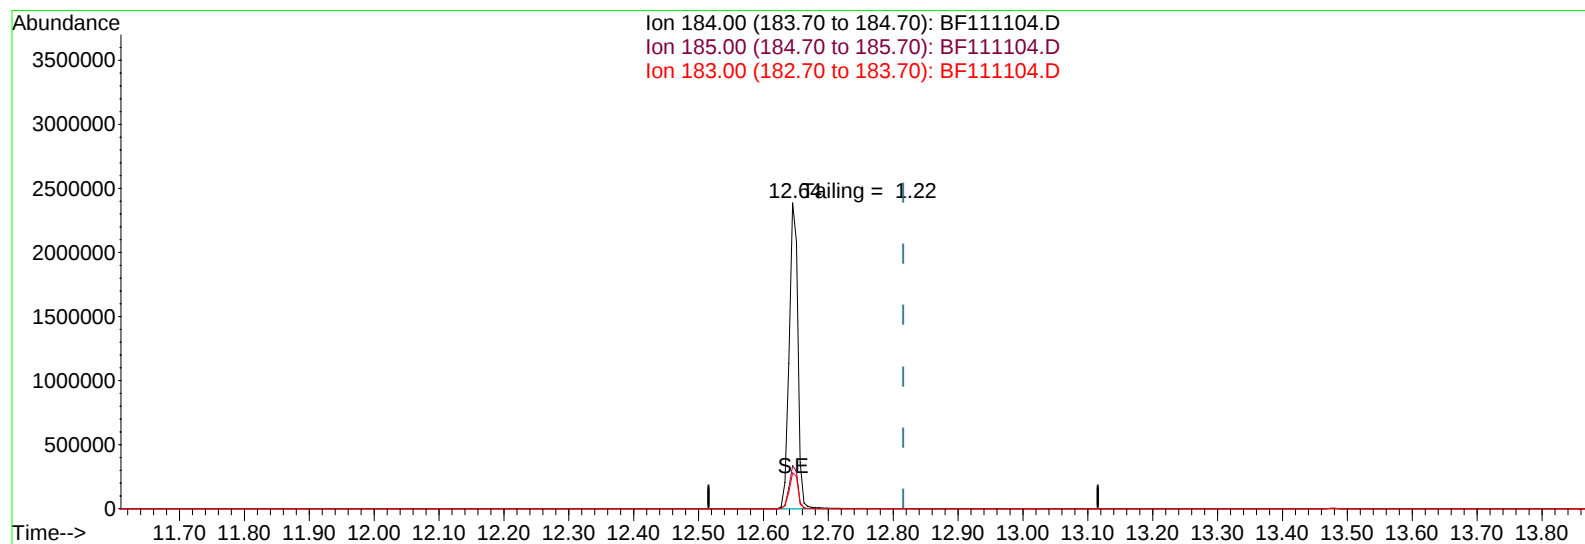

(77) Benzidine

12.645min (-0.171) 798469.20ng

response 2226135

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.11
183.00	11.80	11.73
0.00	0.00	0.00